

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054020.D
 Acq On : 01 May 2023 12:30
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Quant Time: May 02 05:31:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue May 02 05:29:54 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	306960	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	288402	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	139771	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	86849	37.410	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.820%
7) Chloroethane-d5	1.903	69	49648	32.579	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	65.160%#
11) 1,1-Dichloroethene-d2	2.546	63	124943	30.343	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	60.680%
21) 2-Butanone-d5	4.633	46	108920	82.261	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.260%
24) Chloroform-d	5.057	84	159198	37.337	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	74.680%
26) 1,2-Dichloroethane-d4	5.694	65	112135	40.960	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.920%
32) Benzene-d6	5.716	84	340241	40.080	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	80.160%
36) 1,2-Dichloropropane-d6	6.684	67	109041	40.688	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	81.380%
41) Toluene-d8	7.893	98	308960	40.312	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.620%
43) trans-1,3-Dichloroprop...	8.176	79	46457	35.029	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.060%
47) 2-Hexanone-d5	8.655	63	77686	80.933	ug/L	0.03
Spiked Amount	100.000	Range	45 - 130	Recovery	=	80.930%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	141157	39.987	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.980%
66) 1,2-Dichlorobenzene-d4	12.192	152	119299	43.692	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.380%
Target Compounds						
13) Acetone	2.642	43	22739	17.497	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054020.D
Acq On : 01 May 2023 12:30
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Time: May 02 05:31:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Tue May 02 05:29:54 2023
Response via : Initial Calibration

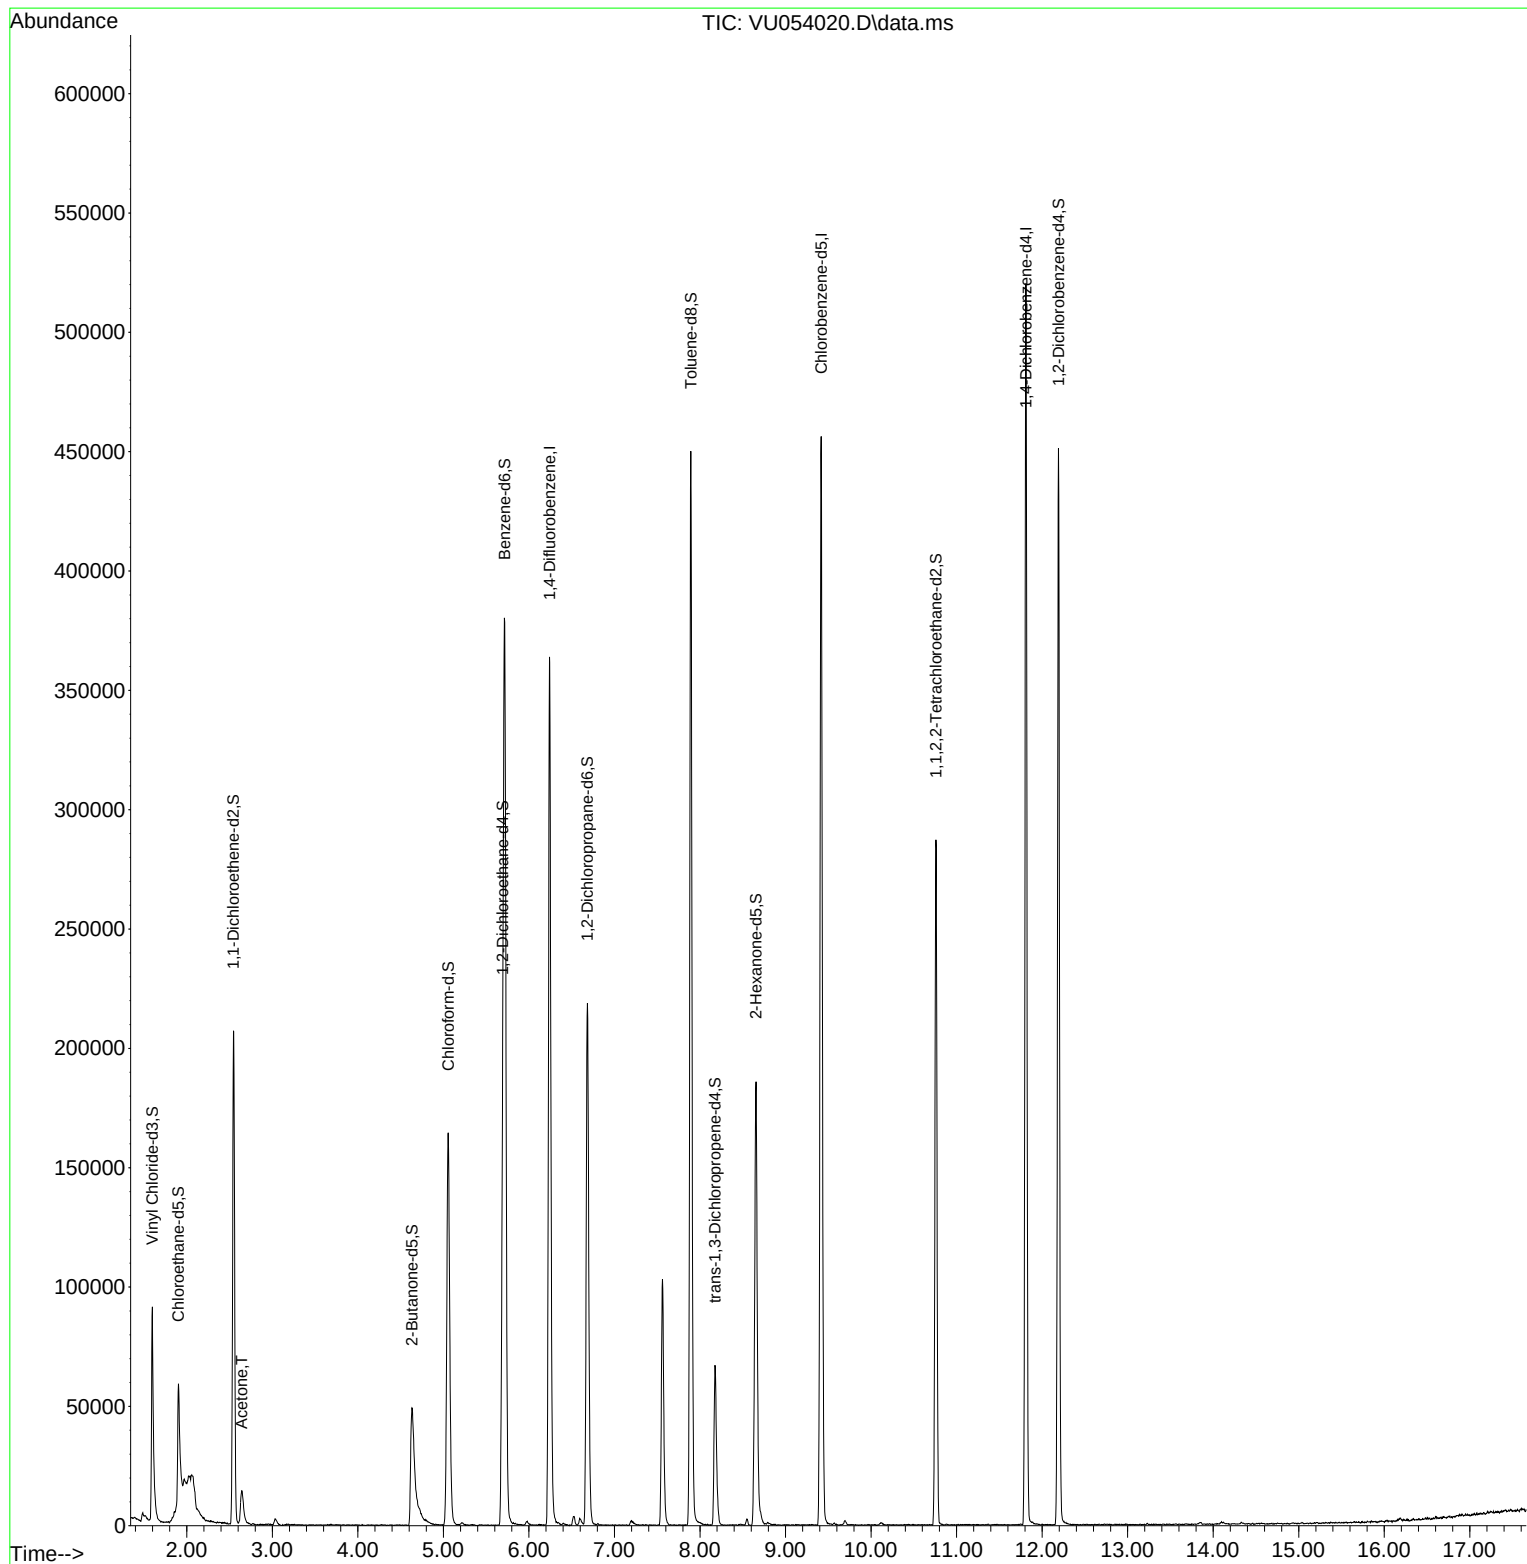

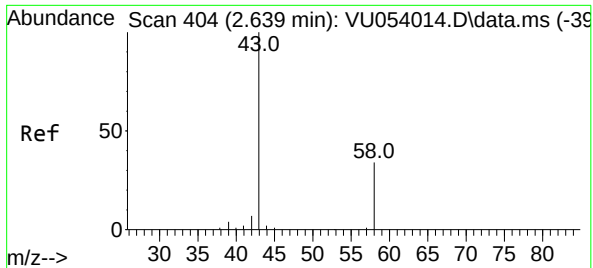

#13
 Acetone
 Concen: 17.497 ug/L
 RT: 2.642 min Scan# 40
 Delta R.T. 0.003 min
 Lab File: VU054020.D
 Acq: 01 May 2023 12:30

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Tgt Ion: 43 Resp: 22739
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 67.4

