

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054018.D
 Acq On : 01 May 2023 11:43
 Operator : JC/MD
 Sample : 02565-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054018.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	96	rVB	110132	135421	13.96%	1.899%
2	1.764	130	132	133	rBV	632	280	0.03%	0.004%
3	1.838	147	155	157	rBV4	702	1069	0.11%	0.015%
4	1.864	159	163	167	rVV5	1391	1620	0.17%	0.023%
5	1.909	169	177	193	rVB	78285	107320	11.06%	1.505%
6	2.562	368	380	399	rVV	197843	325627	33.57%	4.565%
7	2.636	399	403	411	rVB4	1574	2332	0.24%	0.033%
8	2.848	467	469	473	rVB2	438	304	0.03%	0.004%
9	2.954	500	502	507	rVB2	339	210	0.02%	0.003%
10	3.028	522	525	528	rBV3	575	485	0.05%	0.007%
11	3.108	547	550	553	rBV2	261	198	0.02%	0.003%
12	3.169	562	569	570	rBV2	1996	1722	0.18%	0.024%
13	3.301	606	610	612	rBV	238	207	0.02%	0.003%
14	3.427	645	649	652	rBV2	208	231	0.02%	0.003%
15	3.867	776	786	797	rBV4	1264	2046	0.21%	0.029%
16	3.915	799	801	804	rBV	297	201	0.02%	0.003%
17	3.967	814	817	823	rVB	251	200	0.02%	0.003%
18	4.025	832	835	840	rVB2	292	247	0.03%	0.003%
19	4.253	902	906	911	rBV2	208	194	0.02%	0.003%
20	4.359	932	939	941	rBV	282	244	0.03%	0.003%
21	4.385	942	947	952	rVB2	284	303	0.03%	0.004%
22	4.620	1008	1020	1065	rVV	73285	191967	19.79%	2.691%
23	4.944	1118	1121	1126	rVB	358	302	0.03%	0.004%
24	4.983	1130	1133	1135	rBV2	320	216	0.02%	0.003%
25	5.057	1140	1156	1175	rBV	171076	378553	39.02%	5.307%
26	5.314	1230	1236	1238	rBV3	606	587	0.06%	0.008%
27	5.459	1276	1281	1284	rBV2	257	218	0.02%	0.003%
28	5.587	1317	1321	1323	rBV2	285	237	0.02%	0.003%
29	5.719	1340	1362	1399	rBV2	355338	970087	100.00%	13.601%
30	6.111	1481	1484	1487	rBV2	337	262	0.03%	0.004%
31	6.243	1511	1525	1549	rBV	279136	535816	55.23%	7.512%
32	6.414	1574	1578	1582	rBV2	340	266	0.03%	0.004%
33	6.526	1602	1613	1623	rVB6	1887	3653	0.38%	0.051%
34	6.603	1633	1637	1642	rBV2	252	275	0.03%	0.004%
35	6.684	1649	1662	1684	rBV	221965	436104	44.96%	6.114%
36	6.806	1696	1700	1707	rVB5	1054	1174	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054018.D
 Acq On : 01 May 2023 11:43
 Operator : JC/MD
 Sample : 02565-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.951	1737	1745	1748	rBV	293	376	0.04%	0.005%
38	7.156	1804	1809	1813	rBV2	181	217	0.02%	0.003%
39	7.182	1813	1817	1818	rVV	396	276	0.03%	0.004%
40	7.208	1822	1825	1829	rVB2	267	193	0.02%	0.003%
41	7.324	1858	1861	1866	rVB2	199	206	0.02%	0.003%
42	7.381	1870	1879	1881	rBV2	249	387	0.04%	0.005%
43	7.423	1889	1892	1898	rBV2	266	329	0.03%	0.005%
44	7.472	1904	1907	1910	rVB2	246	197	0.02%	0.003%
45	7.491	1910	1913	1917	rBV	325	261	0.03%	0.004%
46	7.558	1919	1934	1958	rBV	120431	217921	22.46%	3.055%
47	7.674	1968	1970	1972	rVV	279	192	0.02%	0.003%
48	7.693	1972	1976	1984	rVB3	597	805	0.08%	0.011%
49	7.799	2006	2009	2012	rBV3	461	363	0.04%	0.005%
50	7.893	2024	2038	2067	rBV	443136	778019	80.20%	10.908%
51	8.172	2114	2125	2149	rBV	85445	147991	15.26%	2.075%
52	8.298	2160	2164	2169	rBV2	230	272	0.03%	0.004%
53	8.462	2207	2215	2217	rBV4	2234	2391	0.25%	0.034%
54	8.549	2233	2242	2254	rVB4	7255	11587	1.19%	0.162%
55	8.629	2254	2267	2308	rBV3	213470	408416	42.10%	5.726%
56	8.889	2343	2348	2353	rVB2	279	371	0.04%	0.005%
57	8.928	2357	2360	2363	rBV3	356	220	0.02%	0.003%
58	9.047	2394	2397	2402	rBV2	246	252	0.03%	0.004%
59	9.172	2432	2436	2440	rBV2	344	376	0.04%	0.005%
60	9.250	2457	2460	2463	rBV2	264	236	0.02%	0.003%
61	9.410	2498	2510	2535	rBV	378801	640654	66.04%	8.982%
62	9.558	2554	2556	2562	rVB2	318	205	0.02%	0.003%
63	9.896	2653	2661	2664	rBV2	198	346	0.04%	0.005%
64	10.127	2729	2733	2737	rBV2	290	316	0.03%	0.004%
65	10.291	2780	2784	2790	rBV2	308	391	0.04%	0.005%
66	10.475	2838	2841	2847	rVB3	394	401	0.04%	0.006%
67	10.510	2847	2852	2855	rVB	204	224	0.02%	0.003%
68	10.594	2876	2878	2882	rBV2	304	225	0.02%	0.003%
69	10.751	2915	2927	2945	rVV	294167	467537	48.20%	6.555%
70	10.889	2963	2970	2979	rVB4	1961	3101	0.32%	0.043%
71	11.082	3027	3030	3032	rBV	344	208	0.02%	0.003%
72	11.426	3133	3137	3142	rBV2	283	310	0.03%	0.004%
73	11.458	3142	3147	3148	rBV2	294	216	0.02%	0.003%
74	11.513	3161	3164	3168	rVB	300	224	0.02%	0.003%
75	11.645	3201	3205	3207	rBV	256	194	0.02%	0.003%
76	11.674	3211	3214	3216	rBV	280	206	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054018.D
 Acq On : 01 May 2023 11:43
 Operator : JC/MD
 Sample : 02565-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.806	3243	3255	3277	rBV	391412	625704	64.50%	8.772%
78	11.909	3283	3287	3290	rBV2	440	368	0.04%	0.005%
79	12.140	3355	3359	3361	rBV2	287	243	0.03%	0.003%
80	12.188	3361	3374	3396	rBV	436325	707744	72.96%	9.923%
81	12.327	3414	3417	3419	rBV2	359	190	0.02%	0.003%
82	12.401	3438	3440	3444	rVB	409	231	0.02%	0.003%
83	12.423	3444	3447	3454	rBV2	312	435	0.04%	0.006%
84	12.799	3561	3564	3569	rBV2	344	324	0.03%	0.005%
85	13.262	3705	3708	3712	rVB	289	210	0.02%	0.003%
86	13.346	3731	3734	3737	rBV2	360	219	0.02%	0.003%
87	13.481	3773	3776	3779	rBV2	273	207	0.02%	0.003%
88	13.526	3786	3790	3791	rBV	261	207	0.02%	0.003%
89	13.690	3836	3841	3844	rBV2	242	271	0.03%	0.004%
90	13.802	3872	3876	3878	rBV	415	309	0.03%	0.004%
91	13.847	3884	3890	3897	rVB5	1489	2199	0.23%	0.031%
92	13.934	3914	3917	3919	rBV2	369	247	0.03%	0.003%
93	14.011	3937	3941	3945	rBV2	338	284	0.03%	0.004%
94	14.060	3953	3956	3958	rBV2	295	197	0.02%	0.003%
95	14.095	3958	3967	3975	rBV4	1313	2793	0.29%	0.039%
96	14.333	4036	4041	4048	rVB6	1444	1702	0.18%	0.024%
97	14.982	4241	4243	4245	rBV2	471	266	0.03%	0.004%
98	15.108	4278	4282	4287	rBV3	543	599	0.06%	0.008%
99	15.175	4297	4303	4305	rBV3	526	537	0.06%	0.008%
100	15.844	4509	4511	4515	rBV3	561	422	0.04%	0.006%




Sum of corrected areas: 7132698

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054018.D
Acq On : 01 May 2023 11:43
Operator : JC/MD
Sample : 02565-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

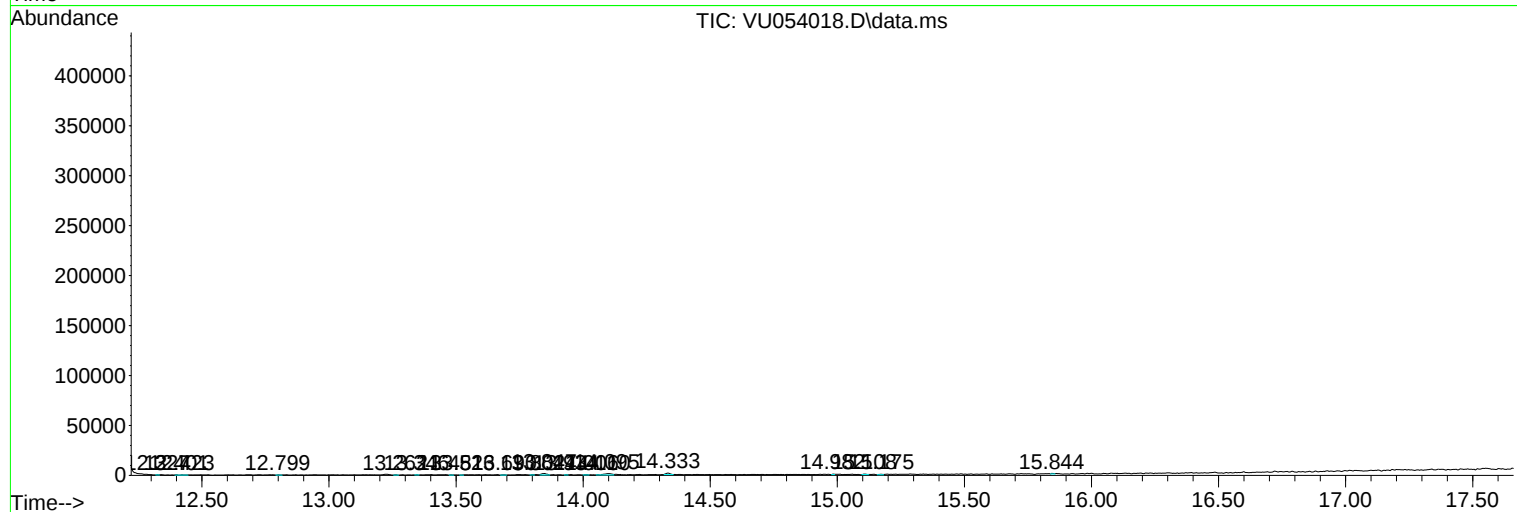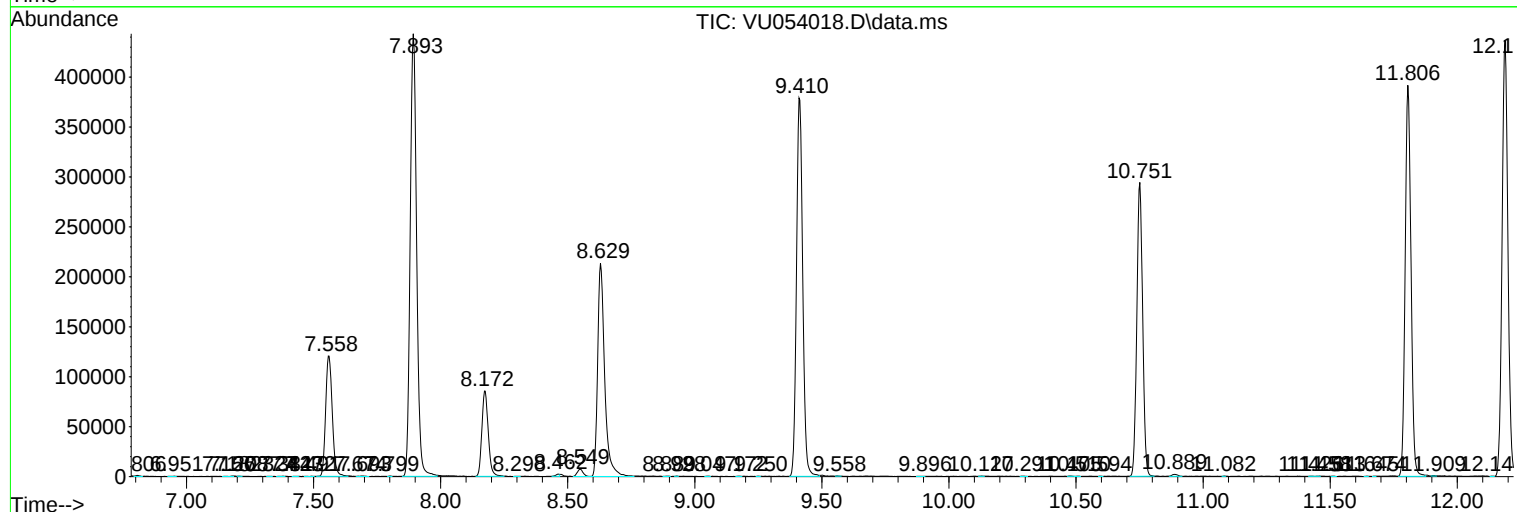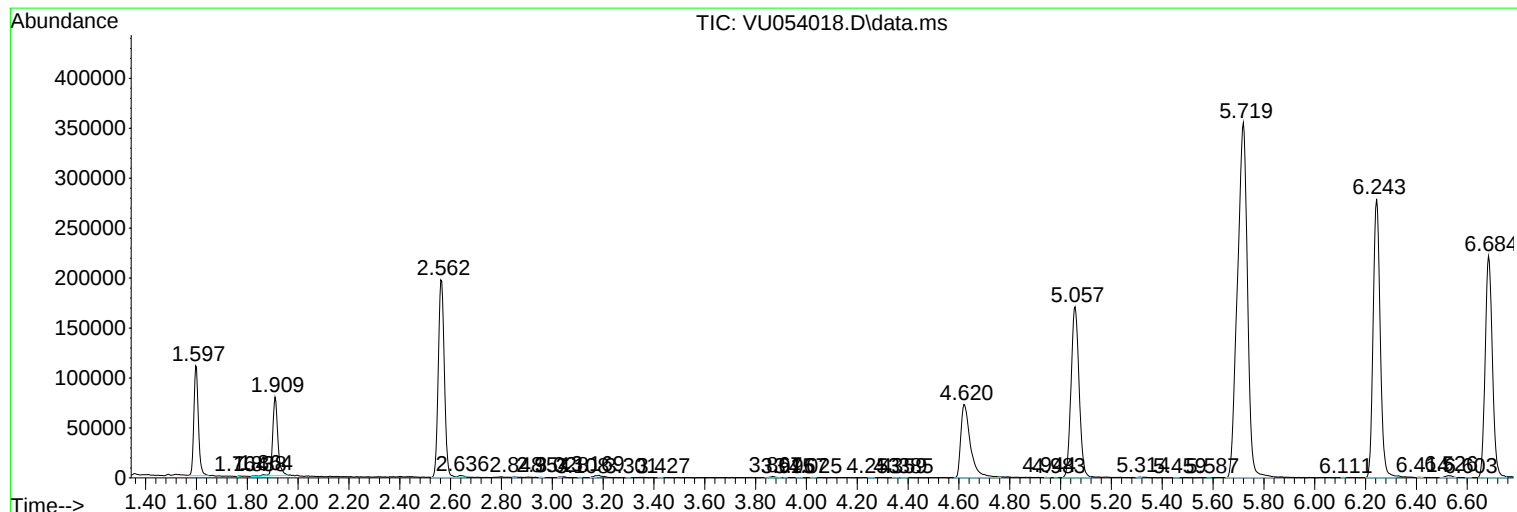

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054018.D
Acq On : 01 May 2023 11:43
Operator : JC/MD
Sample : 02565-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054018.D
Acq On : 01 May 2023 11:43
Operator : JC/MD
Sample : 02565-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc