

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054019.D
 Acq On : 01 May 2023 12:07
 Operator : JC/MD
 Sample : 02526-10ME
 Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rBV4	2482	3449	0.47%	0.064%
2	1.597	72	80	102	rVB	58140	91231	12.43%	1.705%
3	1.819	146	149	150	rBV2	1005	638	0.09%	0.012%
4	1.903	168	175	189	rBV	37138	72358	9.86%	1.352%
5	2.546	363	375	392	rBV	131055	211362	28.80%	3.949%
6	2.645	395	406	416	rBV3	4747	10732	1.46%	0.201%
7	2.816	455	459	463	rBV3	487	451	0.06%	0.008%
8	2.851	467	470	475	rVB2	360	296	0.04%	0.006%
9	2.880	475	479	482	rBV2	268	196	0.03%	0.004%
10	2.928	488	494	497	rBV2	450	508	0.07%	0.009%
11	3.034	518	527	537	rBV6	2759	4948	0.67%	0.092%
12	3.179	567	572	573	rBV6	337	255	0.03%	0.005%
13	3.240	587	591	592	rBV	389	238	0.03%	0.004%
14	3.317	612	615	617	rBV	235	189	0.03%	0.004%
15	3.443	649	654	657	rBV2	331	363	0.05%	0.007%
16	3.652	712	719	722	rBV2	264	324	0.04%	0.006%
17	3.694	729	732	739	rBV2	290	367	0.05%	0.007%
18	3.896	793	795	799	rVB	380	227	0.03%	0.004%
19	3.928	799	805	809	rBV2	243	229	0.03%	0.004%
20	4.099	849	858	863	rVB2	353	547	0.07%	0.010%
21	4.137	863	870	872	rBV	229	313	0.04%	0.006%
22	4.266	906	910	915	rBV	235	222	0.03%	0.004%
23	4.349	931	936	940	rBV2	286	369	0.05%	0.007%
24	4.417	950	957	959	rBV2	250	337	0.05%	0.006%
25	4.433	959	962	965	rVB2	310	196	0.03%	0.004%
26	4.517	983	988	991	rBV	226	243	0.03%	0.005%
27	4.632	1013	1024	1053	rBV2	39769	138145	18.82%	2.581%
28	4.944	1118	1121	1126	rVB2	306	245	0.03%	0.005%
29	5.057	1138	1156	1184	rBV	120855	297121	40.48%	5.551%
30	5.214	1196	1205	1206	rBV2	1122	1493	0.20%	0.028%
31	5.298	1228	1231	1234	rVB2	341	194	0.03%	0.004%
32	5.713	1340	1360	1385	rBV2	277916	733997	100.00%	13.714%
33	5.861	1402	1406	1412	rVB	269	302	0.04%	0.006%
34	5.970	1434	1440	1441	rBV3	1361	1275	0.17%	0.024%
35	6.131	1486	1490	1493	rVB	323	301	0.04%	0.006%
36	6.150	1493	1496	1498	rBV2	265	212	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054019.D
 Acq On : 01 May 2023 12:07
 Operator : JC/MD
 Sample : 02526-10ME
 Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.240	1511	1524	1551	rVV	234124	471314	64.21%	8.806%
38	6.394	1567	1572	1577	rBV5	468	671	0.09%	0.013%
39	6.481	1594	1599	1603	rBV2	363	366	0.05%	0.007%
40	6.520	1604	1611	1622	rVV6	3181	5654	0.77%	0.106%
41	6.600	1625	1636	1648	rVV5	2504	6026	0.82%	0.113%
42	6.684	1648	1662	1686	rVV2	167914	342546	46.67%	6.400%
43	6.771	1686	1689	1690	rVV	329	194	0.03%	0.004%
44	6.796	1694	1697	1698	rBV	248	182	0.02%	0.003%
45	6.822	1703	1705	1711	rVB2	212	192	0.03%	0.004%
46	7.189	1814	1819	1820	rBV4	1313	1091	0.15%	0.020%
47	7.343	1864	1867	1869	rBV	356	188	0.03%	0.004%
48	7.484	1908	1911	1916	rVB2	184	188	0.03%	0.004%
49	7.517	1916	1921	1923	rBV2	288	259	0.04%	0.005%
50	7.562	1923	1935	1964	rVB	74213	145027	19.76%	2.710%
51	7.716	1979	1983	1985	rBV3	401	324	0.04%	0.006%
52	7.893	2024	2038	2057	rBV	284401	511732	69.72%	9.561%
53	8.031	2079	2081	2084	rVB2	313	190	0.03%	0.004%
54	8.176	2115	2126	2148	rVV	50410	101667	13.85%	1.900%
55	8.359	2181	2183	2187	rBV3	280	202	0.03%	0.004%
56	8.420	2198	2202	2205	rVB2	259	223	0.03%	0.004%
57	8.465	2213	2216	2224	rVV2	462	564	0.08%	0.011%
58	8.545	2235	2241	2252	rBV5	3620	5572	0.76%	0.104%
59	8.658	2259	2276	2304	rBV	143770	324103	44.16%	6.055%
60	8.931	2357	2361	2364	rVB2	282	232	0.03%	0.004%
61	8.954	2364	2368	2372	rBV2	300	305	0.04%	0.006%
62	9.050	2391	2398	2404	rBV2	334	561	0.08%	0.010%
63	9.243	2455	2458	2461	rBV2	230	190	0.03%	0.004%
64	9.417	2498	2512	2535	rBV	274806	534872	72.87%	9.993%
65	9.632	2576	2579	2581	rBV	244	198	0.03%	0.004%
66	9.700	2592	2600	2607	rBV3	1132	2076	0.28%	0.039%
67	9.825	2636	2639	2643	rVV	254	223	0.03%	0.004%
68	10.021	2697	2700	2703	rBV	202	185	0.03%	0.003%
69	10.115	2720	2729	2731	rBV3	758	1170	0.16%	0.022%
70	10.253	2768	2772	2774	rBV2	209	214	0.03%	0.004%
71	10.324	2791	2794	2797	rBV2	253	188	0.03%	0.004%
72	10.468	2834	2839	2841	rBV2	358	380	0.05%	0.007%
73	10.555	2860	2866	2868	rVB2	234	210	0.03%	0.004%
74	10.761	2917	2930	2944	rBV	226403	364956	49.72%	6.819%
75	10.889	2968	2970	2976	rVV2	412	392	0.05%	0.007%
76	10.922	2978	2980	2985	rBV	225	206	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054019.D
 Acq On : 01 May 2023 12:07
 Operator : JC/MD
 Sample : 02526-10ME
 Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCF4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.018	3007	3010	3020	rVV2	237	375	0.05%	0.007%
78	11.372	3118	3120	3126	rVB3	310	217	0.03%	0.004%
79	11.471	3146	3151	3156	rBV2	400	489	0.07%	0.009%
80	11.578	3180	3184	3187	rBV2	195	207	0.03%	0.004%
81	11.745	3231	3236	3242	rBV2	530	571	0.08%	0.011%
82	11.812	3245	3257	3274	rBV	297746	474124	64.59%	8.858%
83	12.066	3333	3336	3340	rBV	295	262	0.04%	0.005%
84	12.192	3363	3375	3397	rBV	290714	467417	63.68%	8.733%
85	12.414	3441	3444	3449	rBV2	279	336	0.05%	0.006%
86	12.491	3465	3468	3471	rBV	258	226	0.03%	0.004%
87	12.690	3527	3530	3532	rBV2	264	197	0.03%	0.004%
88	13.227	3692	3697	3699	rBV2	537	572	0.08%	0.011%
89	13.294	3715	3718	3721	rBV2	329	239	0.03%	0.004%
90	13.632	3821	3823	3827	rBV2	230	194	0.03%	0.004%
91	13.751	3858	3860	3865	rBV2	340	268	0.04%	0.005%
92	13.854	3884	3892	3901	rVB4	1407	1889	0.26%	0.035%
93	14.098	3962	3968	3971	rBV2	1309	1386	0.19%	0.026%
94	14.330	4035	4040	4048	rBV5	1441	2050	0.28%	0.038%
95	14.712	4156	4159	4163	rBV2	387	273	0.04%	0.005%
96	14.918	4217	4223	4226	rBV3	457	615	0.08%	0.011%
97	14.976	4234	4241	4247	rBV3	611	747	0.10%	0.014%
98	15.005	4247	4250	4251	rBV3	429	229	0.03%	0.004%
99	15.079	4270	4273	4274	rBV3	411	232	0.03%	0.004%
100	15.323	4347	4349	4351	rBV2	392	207	0.03%	0.004%




Sum of corrected areas: 5352228

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054019.D
Acq On : 01 May 2023 12:07
Operator : JC/MD
Sample : 02526-10ME
Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

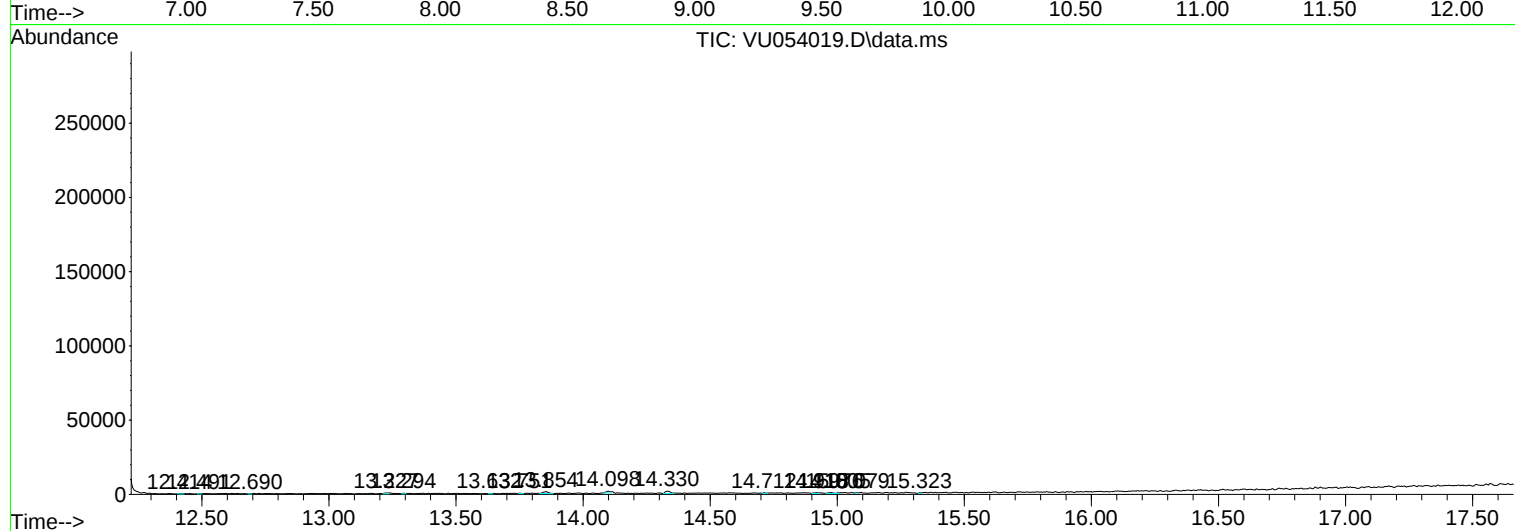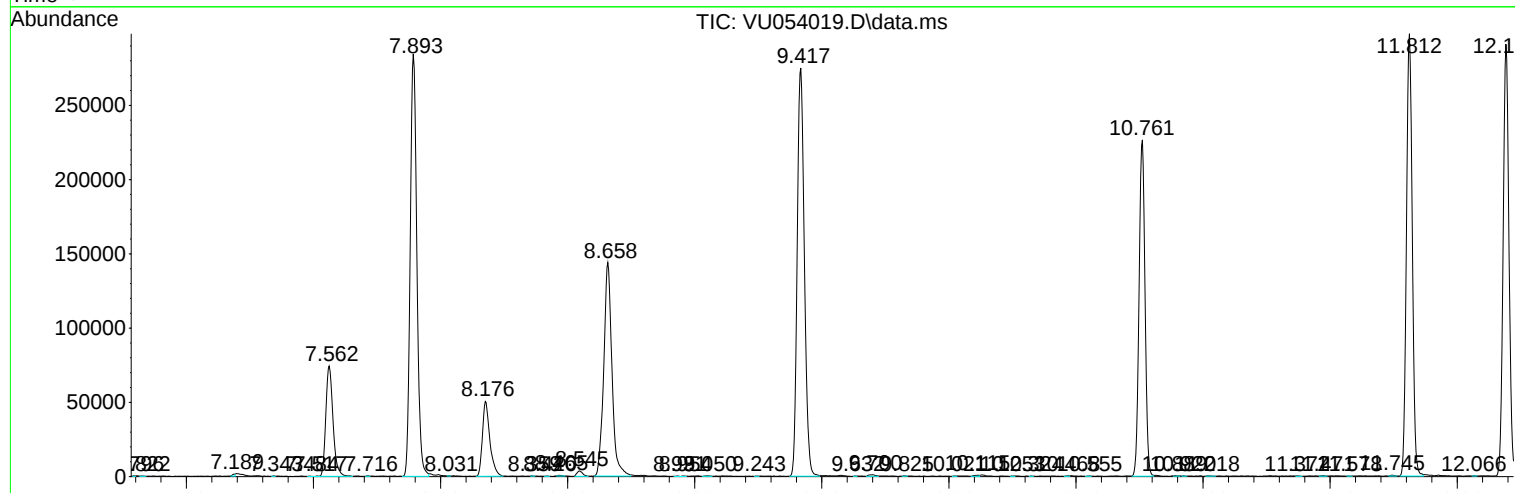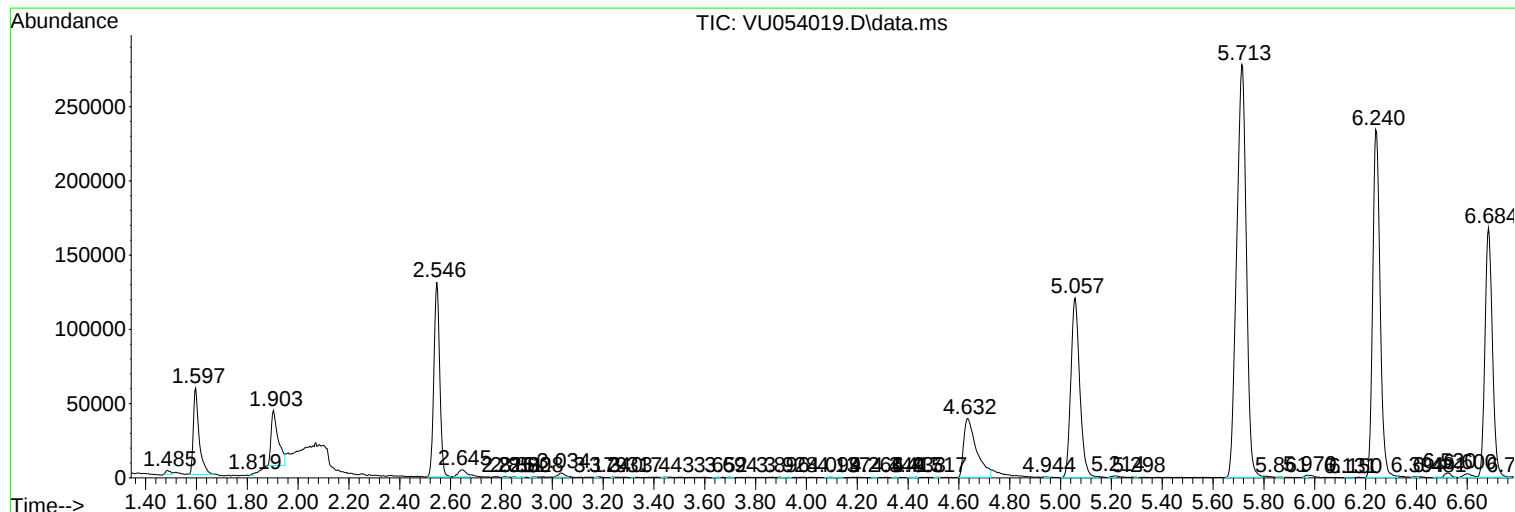

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054019.D
Acq On : 01 May 2023 12:07
Operator : JC/MD
Sample : 02526-10ME
Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054019.D
Acq On : 01 May 2023 12:07
Operator : JC/MD
Sample : 02526-10ME
Misc : 5.87g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCF4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------