

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054020.D
 Acq On : 01 May 2023 12:30
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054020.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	38	45	52	rBV4	3597	6226	0.63%	0.080%
2	1.597	72	80	110	rVB	90091	139665	14.06%	1.797%
3	1.903	168	175	191	rBV	50695	95921	9.65%	1.234%
4	2.417	332	335	337	rBV3	495	264	0.03%	0.003%
5	2.546	363	375	393	rBV	206441	337769	34.00%	4.345%
6	2.642	393	405	425	rVV	13645	33994	3.42%	0.437%
7	2.774	440	446	451	rBV3	634	872	0.09%	0.011%
8	2.977	506	509	512	rVB2	373	232	0.02%	0.003%
9	3.031	519	526	537	rBV3	2501	4978	0.50%	0.064%
10	3.166	566	568	571	rBV2	394	264	0.03%	0.003%
11	3.356	622	627	630	rVB2	262	274	0.03%	0.004%
12	3.433	646	651	656	rBV2	255	352	0.04%	0.005%
13	3.514	672	676	680	rBV2	227	235	0.02%	0.003%
14	3.649	715	718	723	rVB2	325	278	0.03%	0.004%
15	3.678	723	727	728	rBV2	403	269	0.03%	0.003%
16	3.874	783	788	790	rBV	266	215	0.02%	0.003%
17	3.973	815	819	821	rBV2	259	211	0.02%	0.003%
18	4.051	838	843	847	rBV	312	239	0.02%	0.003%
19	4.276	906	913	920	rBV2	338	508	0.05%	0.007%
20	4.375	939	944	946	rBV2	225	213	0.02%	0.003%
21	4.552	995	999	1003	rBV2	260	282	0.03%	0.004%
22	4.633	1012	1024	1057	rBV	49225	172340	17.35%	2.217%
23	4.912	1106	1111	1114	rBV3	321	292	0.03%	0.004%
24	5.057	1138	1156	1186	rBV2	164425	391572	39.41%	5.038%
25	5.198	1197	1200	1201	rBV2	363	228	0.02%	0.003%
26	5.276	1220	1224	1228	rBV2	311	236	0.02%	0.003%
27	5.420	1266	1269	1273	rBV	310	343	0.03%	0.004%
28	5.520	1297	1300	1304	rVB2	310	238	0.02%	0.003%
29	5.562	1309	1313	1318	rVB2	231	282	0.03%	0.004%
30	5.713	1341	1360	1390	rBV2	380110	993545	100.00%	12.782%
31	5.980	1431	1443	1452	rBV6	1637	3230	0.33%	0.042%
32	6.083	1472	1475	1480	rVB2	270	243	0.02%	0.003%
33	6.115	1480	1485	1487	rBV2	408	323	0.03%	0.004%
34	6.240	1511	1524	1548	rBV	363632	709980	71.46%	9.134%
35	6.401	1569	1574	1578	rBV4	588	597	0.06%	0.008%
36	6.449	1585	1589	1596	rVB2	486	620	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054020.D
 Acq On : 01 May 2023 12:30
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.478	1596	1598	1603	rBV	393	321	0.03%	0.004%
38	6.526	1603	1613	1624	rVV4	3785	7319	0.74%	0.094%
39	6.594	1626	1634	1648	rBV3	2773	5869	0.59%	0.076%
40	6.684	1648	1662	1687	rVB	218340	447367	45.03%	5.755%
41	6.806	1693	1700	1705	rVB3	725	856	0.09%	0.011%
42	6.925	1731	1737	1741	rVB	228	231	0.02%	0.003%
43	7.012	1759	1764	1767	rVB2	260	209	0.02%	0.003%
44	7.140	1802	1804	1808	rVB	289	232	0.02%	0.003%
45	7.198	1813	1822	1825	rBV4	2034	2858	0.29%	0.037%
46	7.369	1868	1875	1877	rBV2	369	405	0.04%	0.005%
47	7.414	1885	1889	1893	rVB2	273	273	0.03%	0.004%
48	7.562	1923	1935	1960	rVB	103125	195905	19.72%	2.520%
49	7.893	2024	2038	2062	rBV	449916	802900	80.81%	10.329%
50	8.089	2096	2099	2104	rVB3	477	355	0.04%	0.005%
51	8.176	2112	2126	2150	rBV2	67101	133842	13.47%	1.722%
52	8.456	2209	2213	2215	rBV3	367	300	0.03%	0.004%
53	8.549	2234	2242	2250	rBV4	2601	3822	0.38%	0.049%
54	8.655	2257	2275	2306	rBV	185894	397629	40.02%	5.116%
55	8.793	2312	2318	2322	rBV4	760	840	0.08%	0.011%
56	8.874	2341	2343	2351	rVB3	442	455	0.05%	0.006%
57	8.973	2368	2374	2377	rBV2	183	217	0.02%	0.003%
58	9.041	2391	2395	2400	rVB2	237	243	0.02%	0.003%
59	9.076	2400	2406	2409	rBV	261	301	0.03%	0.004%
60	9.140	2424	2426	2435	rVB2	264	410	0.04%	0.005%
61	9.417	2498	2512	2534	rBV	456206	841394	84.69%	10.825%
62	9.568	2553	2559	2564	rBV	700	830	0.08%	0.011%
63	9.639	2579	2581	2585	rBV	238	212	0.02%	0.003%
64	9.697	2593	2599	2607	rVB4	1707	2606	0.26%	0.034%
65	9.963	2679	2682	2686	rBV	259	225	0.02%	0.003%
66	10.037	2700	2705	2708	rBV2	263	241	0.02%	0.003%
67	10.118	2720	2730	2737	rVV5	951	1981	0.20%	0.025%
68	10.491	2844	2846	2849	rVB2	384	226	0.02%	0.003%
69	10.555	2861	2866	2869	rBV2	234	284	0.03%	0.004%
70	10.629	2884	2889	2892	rBV2	212	229	0.02%	0.003%
71	10.758	2917	2929	2949	rBV	287198	464654	46.77%	5.978%
72	10.880	2963	2967	2971	rBV2	322	408	0.04%	0.005%
73	11.018	3004	3010	3014	rBV	354	378	0.04%	0.005%
74	11.044	3014	3018	3024	rBV2	284	375	0.04%	0.005%
75	11.073	3024	3027	3030	rBV	249	222	0.02%	0.003%
76	11.144	3045	3049	3051	rBV2	273	219	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054020.D
 Acq On : 01 May 2023 12:30
 Operator : JC/MD
 Sample : 02525-19ME
 Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCM2ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.468	3148	3150	3156	rVB2	294	315	0.03%	0.004%
78	11.745	3233	3236	3237	rBV	329	222	0.02%	0.003%
79	11.812	3244	3257	3278	rBV	520095	825789	83.12%	10.624%
80	12.002	3311	3316	3321	rVB2	380	415	0.04%	0.005%
81	12.192	3362	3375	3393	rBV	450900	724154	72.89%	9.316%
82	12.481	3461	3465	3470	rBV2	242	288	0.03%	0.004%
83	12.616	3503	3507	3513	rBV2	300	363	0.04%	0.005%
84	12.668	3519	3523	3528	rVB	343	339	0.03%	0.004%
85	12.732	3538	3543	3546	rBV	340	329	0.03%	0.004%
86	12.803	3562	3565	3571	rVB2	291	236	0.02%	0.003%
87	12.848	3575	3579	3581	rBV2	272	246	0.02%	0.003%
88	12.979	3617	3620	3623	rBV	446	316	0.03%	0.004%
89	13.230	3693	3698	3703	rBV4	585	582	0.06%	0.007%
90	13.304	3719	3721	3724	rBV2	397	270	0.03%	0.003%
91	13.327	3725	3728	3734	rBV2	235	250	0.03%	0.003%
92	13.751	3857	3860	3865	rBV3	461	425	0.04%	0.005%
93	14.044	3949	3951	3954	rBV2	303	210	0.02%	0.003%
94	14.086	3960	3964	3965	rBV2	478	343	0.03%	0.004%
95	14.327	4037	4039	4044	rVB3	491	325	0.03%	0.004%
96	14.462	4075	4081	4086	rVB2	577	665	0.07%	0.009%
97	14.484	4086	4088	4091	rBV	348	269	0.03%	0.003%
98	15.741	4474	4479	4482	rBV5	722	682	0.07%	0.009%
99	15.851	4510	4513	4515	rBV3	674	438	0.04%	0.006%
100	16.102	4588	4591	4593	rBV2	628	486	0.05%	0.006%


Sum of corrected areas: 7772930

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054020.D
Acq On : 01 May 2023 12:30
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

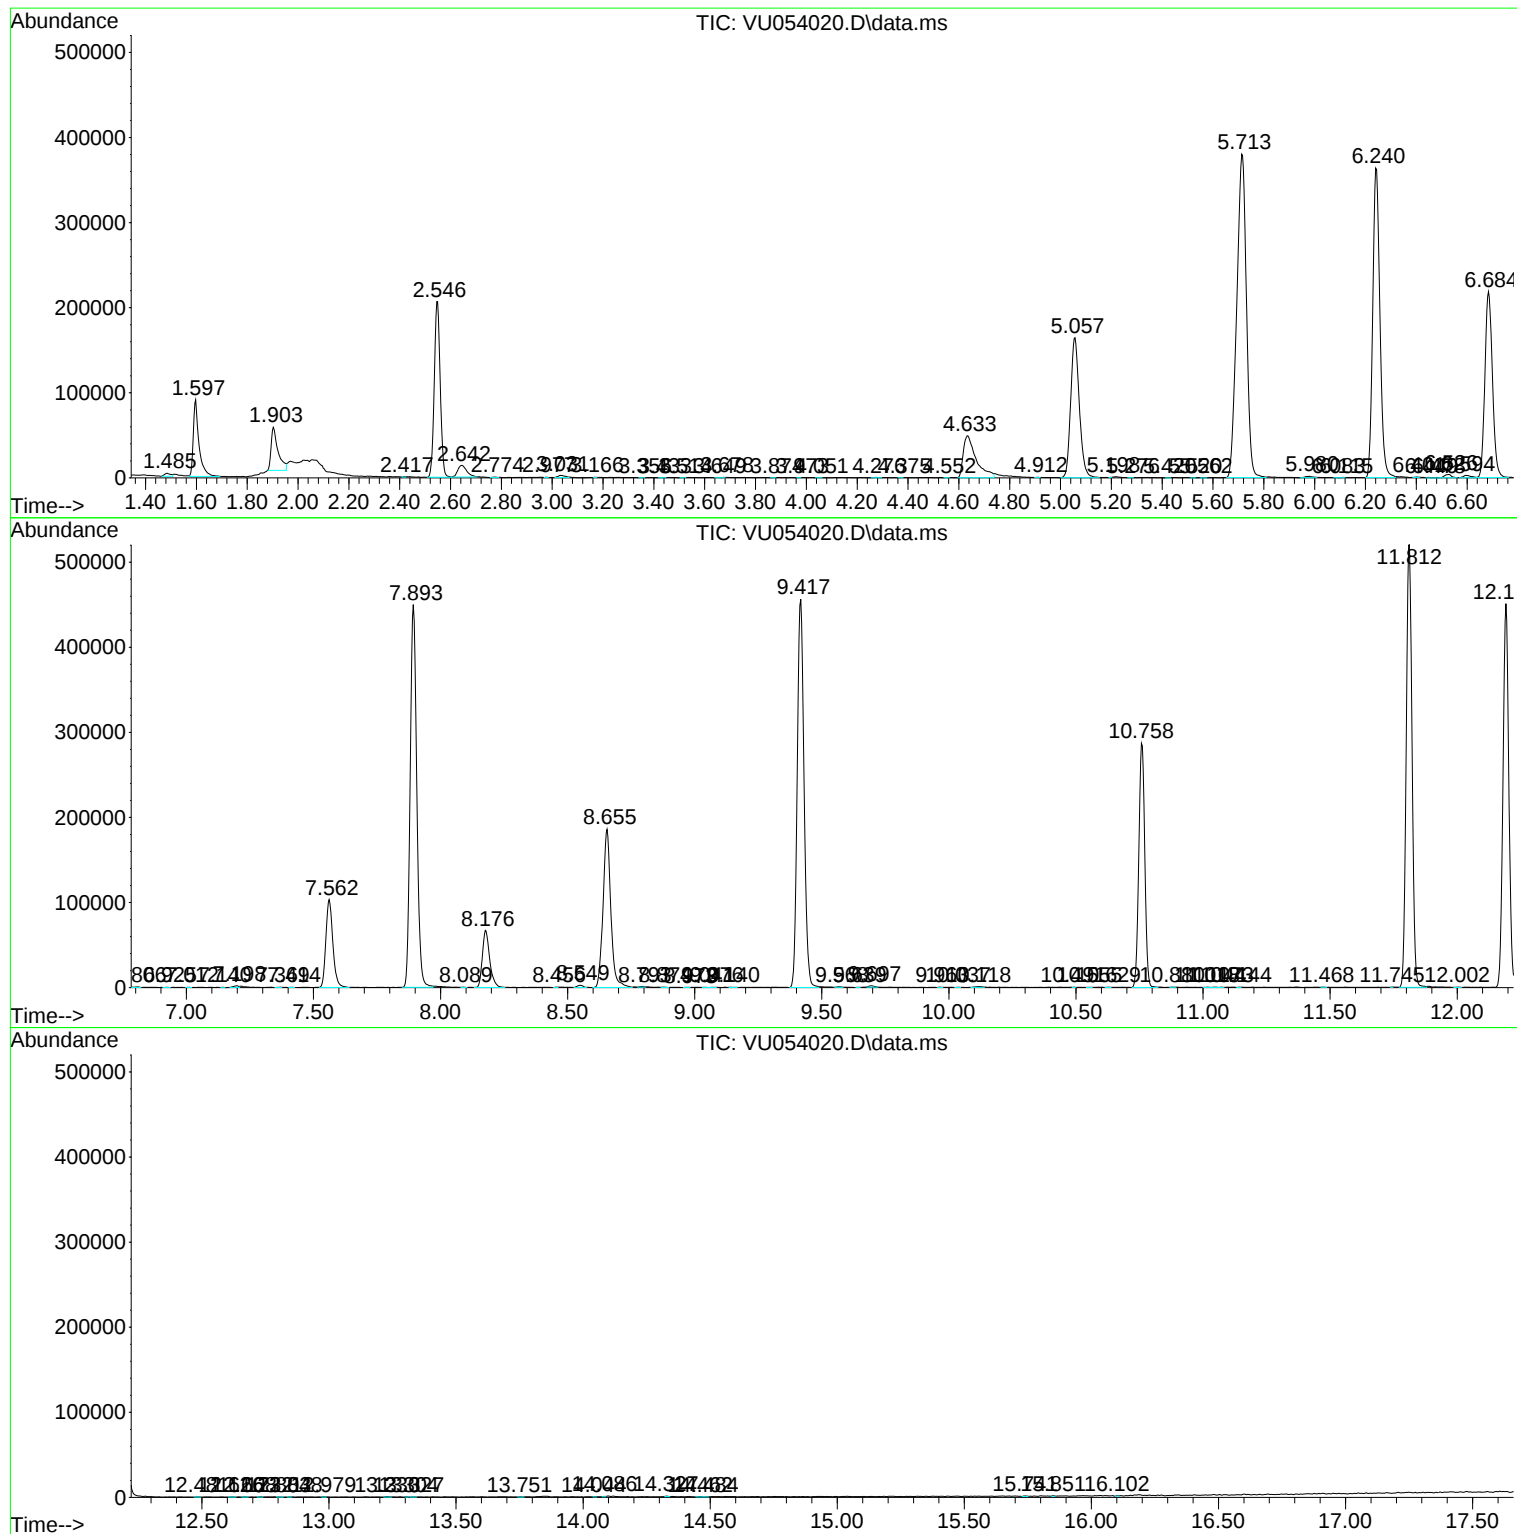

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054020.D
Acq On : 01 May 2023 12:30
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054020.D
Acq On : 01 May 2023 12:30
Operator : JC/MD
Sample : 02525-19ME
Misc : 5.80g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCM2ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------