

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054024.D
 Acq On : 01 May 2023 14:32
 Operator : JC/MD
 Sample : 02525-04ME
 Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCC4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	93187	111651	12.41%	1.705%
2	1.909	169	177	193	rBV	68504	92065	10.23%	1.406%
3	2.562	368	380	398	rBV	162455	265825	29.54%	4.060%
4	2.675	413	415	418	rBV2	361	228	0.03%	0.003%
5	2.916	489	490	494	rBV	240	185	0.02%	0.003%
6	3.044	518	530	542	rBV3	4496	9177	1.02%	0.140%
7	3.237	587	590	595	rVB2	303	272	0.03%	0.004%
8	3.263	595	598	601	rBV2	388	215	0.02%	0.003%
9	3.408	639	643	646	rBV2	201	188	0.02%	0.003%
10	3.562	689	691	695	rBV	145	80	0.01%	0.001%
11	3.748	746	749	752	rBV	224	161	0.02%	0.002%
12	3.810	764	768	771	rBV	241	261	0.03%	0.004%
13	3.838	775	777	781	rVB2	215	143	0.02%	0.002%
14	3.893	792	794	796	rBV	206	98	0.01%	0.001%
15	3.961	813	815	818	rVB	164	91	0.01%	0.001%
16	3.983	819	822	830	rVB2	208	205	0.02%	0.003%
17	4.067	845	848	850	rBV2	226	167	0.02%	0.003%
18	4.231	896	899	902	rBV	196	177	0.02%	0.003%
19	4.273	909	912	914	rBV2	227	145	0.02%	0.002%
20	4.301	919	921	922	rBV	120	66	0.01%	0.001%
21	4.318	922	926	929	rBV	236	178	0.02%	0.003%
22	4.337	929	932	934	rBV	206	131	0.01%	0.002%
23	4.459	967	970	973	rBV	175	85	0.01%	0.001%
24	4.623	1009	1021	1052	rBV	69356	185471	20.61%	2.833%
25	4.964	1125	1127	1128	rBV	233	94	0.01%	0.001%
26	5.057	1139	1156	1178	rBV	157293	348747	38.75%	5.327%
27	5.317	1234	1237	1239	rBV2	138	85	0.01%	0.001%
28	5.337	1239	1243	1246	rVV2	301	183	0.02%	0.003%
29	5.443	1273	1276	1277	rBV2	123	53	0.01%	0.001%
30	5.478	1284	1287	1289	rBV2	214	151	0.02%	0.002%
31	5.639	1336	1337	1340	rVB	228	106	0.01%	0.002%
32	5.719	1340	1362	1382	rBV2	324091	899924	100.00%	13.745%
33	5.925	1423	1426	1428	rVB2	391	249	0.03%	0.004%
34	5.941	1428	1431	1433	rBV2	258	161	0.02%	0.002%
35	5.980	1440	1443	1447	rBV2	219	182	0.02%	0.003%
36	6.012	1449	1453	1455	rBV	326	220	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054024.D
 Acq On : 01 May 2023 14:32
 Operator : JC/MD
 Sample : 02525-04ME
 Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCC4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.031	1457	1459	1462	rVB2	201	109	0.01%	0.002%
38	6.244	1511	1525	1541	rBV	268487	508892	56.55%	7.772%
39	6.462	1591	1593	1598	rVB	260	160	0.02%	0.002%
40	6.491	1599	1602	1605	rBV	339	314	0.03%	0.005%
41	6.607	1637	1638	1640	rVB	225	86	0.01%	0.001%
42	6.684	1648	1662	1683	rBV	212539	411500	45.73%	6.285%
43	6.845	1710	1712	1713	rBV	279	112	0.01%	0.002%
44	6.877	1720	1722	1725	rBV	141	95	0.01%	0.001%
45	6.957	1744	1747	1753	rVB2	346	363	0.04%	0.006%
46	6.986	1753	1756	1758	rBV	231	160	0.02%	0.002%
47	7.060	1776	1779	1781	rBV2	247	154	0.02%	0.002%
48	7.089	1786	1788	1791	rBV	227	156	0.02%	0.002%
49	7.224	1829	1830	1831	rBV	219	68	0.01%	0.001%
50	7.237	1831	1834	1837	rVV	192	181	0.02%	0.003%
51	7.340	1862	1866	1867	rBV	185	134	0.01%	0.002%
52	7.382	1877	1879	1881	rBV	157	63	0.01%	0.001%
53	7.430	1891	1894	1895	rBV	182	101	0.01%	0.002%
54	7.559	1923	1934	1954	rBV	100122	175979	19.55%	2.688%
55	7.684	1968	1973	1976	rBV2	540	443	0.05%	0.007%
56	7.751	1992	1994	1996	rBV	171	121	0.01%	0.002%
57	7.893	2024	2038	2061	rBV	380335	676385	75.16%	10.331%
58	8.173	2114	2125	2144	rBV	72055	121746	13.53%	1.859%
59	8.295	2160	2163	2167	rBV2	211	167	0.02%	0.003%
60	8.314	2167	2169	2172	rBV2	143	110	0.01%	0.002%
61	8.459	2209	2214	2222	rVB3	383	491	0.05%	0.007%
62	8.549	2236	2242	2247	rBV3	1315	1542	0.17%	0.024%
63	8.629	2254	2267	2300	rBV2	218654	417692	46.41%	6.380%
64	8.851	2334	2336	2337	rBV	163	85	0.01%	0.001%
65	8.944	2362	2365	2371	rBV2	381	497	0.06%	0.008%
66	9.166	2432	2434	2437	rVB2	267	149	0.02%	0.002%
67	9.250	2457	2460	2462	rBV	249	167	0.02%	0.003%
68	9.301	2474	2476	2479	rVB	201	71	0.01%	0.001%
69	9.411	2498	2510	2535	rBV	371650	621483	69.06%	9.492%
70	9.575	2559	2561	2563	rBV	360	177	0.02%	0.003%
71	9.636	2577	2580	2581	rBV	256	146	0.02%	0.002%
72	9.742	2609	2613	2615	rBV2	287	261	0.03%	0.004%
73	9.906	2660	2664	2668	rBV2	239	237	0.03%	0.004%
74	10.269	2775	2777	2785	rBV2	225	267	0.03%	0.004%
75	10.356	2801	2804	2806	rBV	280	218	0.02%	0.003%
76	10.751	2914	2927	2946	rBV	285592	468097	52.02%	7.149%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054024.D
Acq On : 01 May 2023 14:32
Operator : JC/MD
Sample : 02525-04ME
Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCC4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

77	10.957	2987	2991	2994	rBV	349	276	0.03%	0.004%
78	11.076	3024	3028	3030	rBV	227	175	0.02%	0.003%
79	11.806	3240	3255	3278	rBV	369738	590069	65.57%	9.012%
80	12.189	3361	3374	3399	rBV	385523	630070	70.01%	9.623%
81	13.099	3655	3657	3661	rBV2	310	199	0.02%	0.003%




Sum of corrected areas: 6547388

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054024.D
Acq On : 01 May 2023 14:32
Operator : JC/MD
Sample : 02525-04ME
Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCC4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

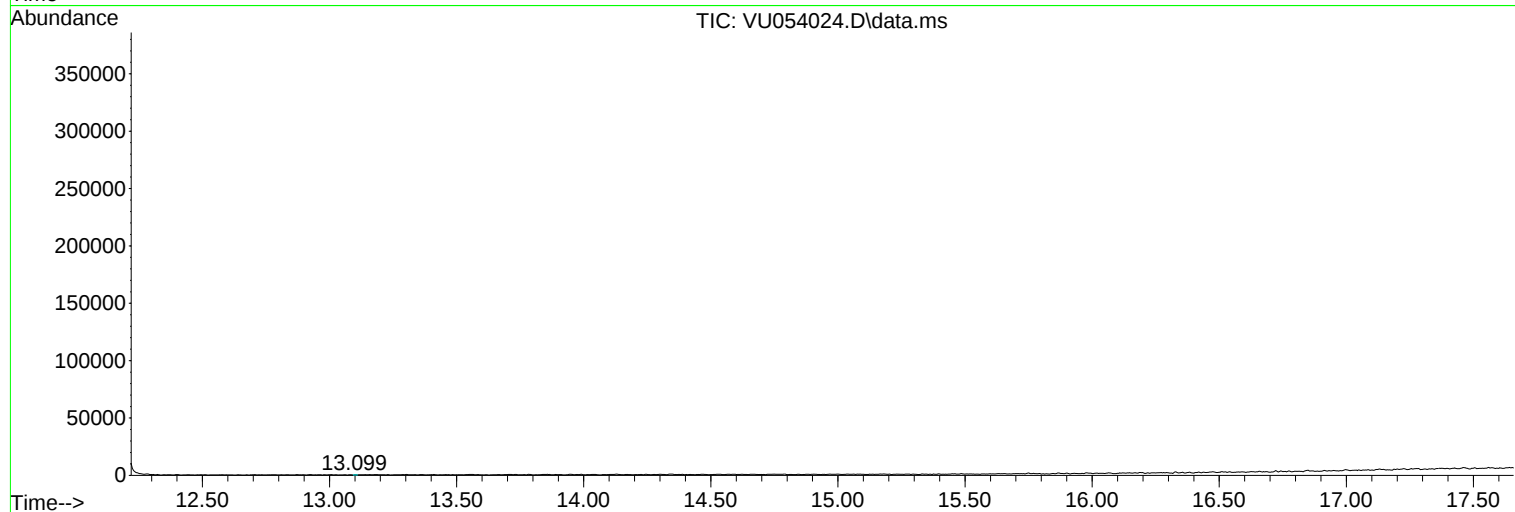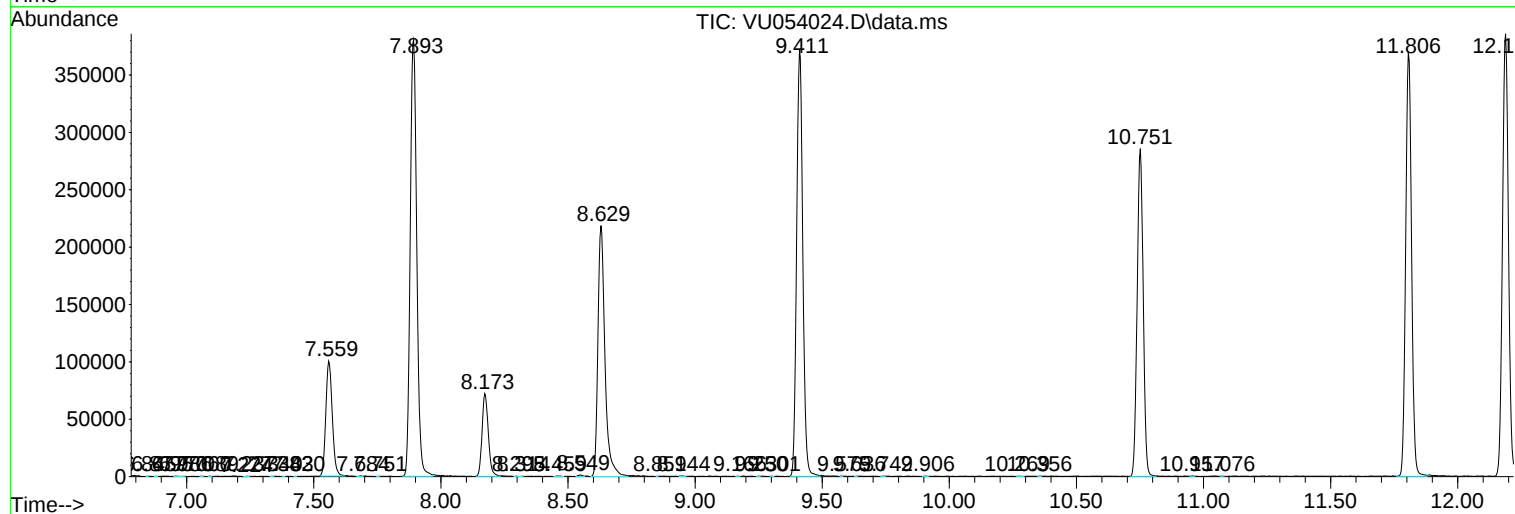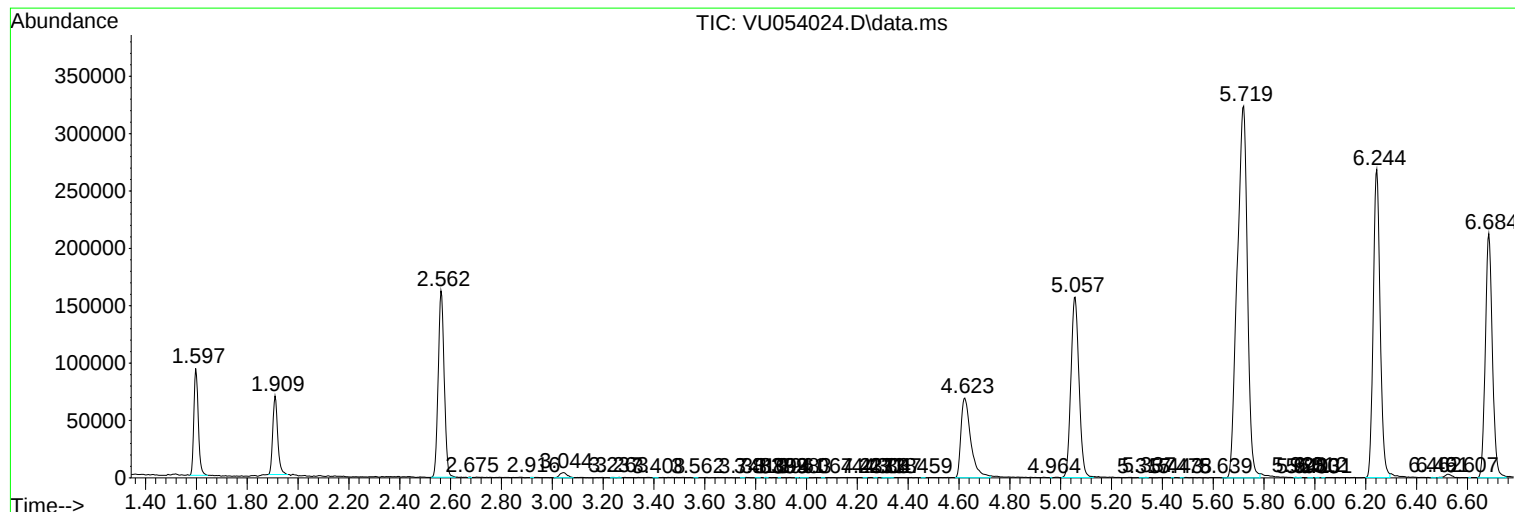

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054024.D
Acq On : 01 May 2023 14:32
Operator : JC/MD
Sample : 02525-04ME
Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCC4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054024.D
Acq On : 01 May 2023 14:32
Operator : JC/MD
Sample : 02525-04ME
Misc : 5.67g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCC4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc