

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054029.D
 Acq On : 01 May 2023 16:30
 Operator : JC/MD
 Sample : 02565-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054029.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	102	rVB	104676	127719	13.74%	1.700%
2	1.909	169	177	189	rBV	73533	97893	10.53%	1.303%
3	2.562	368	380	395	rVV	193030	312027	33.57%	4.152%
4	3.044	526	530	536	rVB3	958	1021	0.11%	0.014%
5	3.121	552	554	557	rVB2	375	188	0.02%	0.003%
6	3.173	563	570	572	rBV3	1431	1686	0.18%	0.022%
7	3.395	637	639	643	rVB	357	229	0.02%	0.003%
8	3.417	643	646	648	rBV	257	192	0.02%	0.003%
9	3.739	743	746	750	rVV2	205	203	0.02%	0.003%
10	3.896	789	795	798	rBV2	209	240	0.03%	0.003%
11	3.919	799	802	806	rBV2	226	210	0.02%	0.003%
12	4.269	907	911	918	rVB2	200	251	0.03%	0.003%
13	4.301	918	921	925	rBV	272	277	0.03%	0.004%
14	4.620	1008	1020	1058	rBV	73864	196275	21.11%	2.612%
15	4.858	1092	1094	1099	rBV2	223	227	0.02%	0.003%
16	4.983	1130	1133	1138	rVB3	357	285	0.03%	0.004%
17	5.057	1138	1156	1181	rBV	167672	367952	39.58%	4.896%
18	5.163	1186	1189	1195	rVB3	495	531	0.06%	0.007%
19	5.218	1203	1206	1209	rBV3	248	194	0.02%	0.003%
20	5.240	1211	1213	1217	rVB	520	340	0.04%	0.005%
21	5.311	1221	1235	1249	rBV3	29880	67840	7.30%	0.903%
22	5.600	1322	1325	1328	rBV	382	301	0.03%	0.004%
23	5.719	1341	1362	1385	rBV2	341038	929616	100.00%	12.371%
24	5.967	1436	1439	1443	rVV2	223	198	0.02%	0.003%
25	6.025	1452	1457	1459	rBV	269	183	0.02%	0.002%
26	6.066	1465	1470	1472	rBV	279	189	0.02%	0.003%
27	6.185	1504	1507	1512	rBV2	224	253	0.03%	0.003%
28	6.243	1512	1525	1546	rBV	315523	599684	64.51%	7.980%
29	6.536	1602	1616	1634	rBV	141082	265975	28.61%	3.539%
30	6.684	1648	1662	1683	rBV	217663	419632	45.14%	5.584%
31	6.796	1695	1697	1699	rBV	556	340	0.04%	0.005%
32	7.189	1814	1819	1821	rVV2	359	298	0.03%	0.004%
33	7.459	1896	1903	1904	rBV	229	206	0.02%	0.003%
34	7.558	1923	1934	1958	rVV	118752	211475	22.75%	2.814%
35	7.693	1971	1976	1980	rBV3	378	380	0.04%	0.005%
36	7.783	1999	2004	2008	rBV	355	316	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054029.D
 Acq On : 01 May 2023 16:30
 Operator : JC/MD
 Sample : 02565-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	7.893	2024	2038	2068	rBV	429150	746745	80.33%	9.937%
38	8.176	2113	2126	2145	rBV	83409	143315	15.42%	1.907%
39	8.308	2158	2167	2171	rBV2	432	531	0.06%	0.007%
40	8.394	2190	2194	2197	rBV	220	186	0.02%	0.002%
41	8.468	2208	2217	2229	rVB3	1315	2328	0.25%	0.031%
42	8.629	2256	2267	2293	rBV2	220287	415890	44.74%	5.534%
43	8.832	2327	2330	2336	rVB3	363	361	0.04%	0.005%
44	9.002	2379	2383	2385	rBV2	270	262	0.03%	0.003%
45	9.098	2407	2413	2418	rVB2	354	457	0.05%	0.006%
46	9.131	2419	2423	2428	rBV2	200	224	0.02%	0.003%
47	9.156	2428	2431	2435	rBV	222	247	0.03%	0.003%
48	9.256	2459	2462	2465	rBV2	268	205	0.02%	0.003%
49	9.410	2497	2510	2537	rVV	433697	722245	77.69%	9.611%
50	9.571	2557	2560	2564	rVB3	298	227	0.02%	0.003%
51	9.626	2574	2577	2582	rVB2	311	303	0.03%	0.004%
52	9.661	2582	2588	2590	rBV2	216	239	0.03%	0.003%
53	9.758	2615	2618	2621	rBV2	279	248	0.03%	0.003%
54	9.841	2641	2644	2650	rVB2	259	260	0.03%	0.003%
55	9.999	2690	2693	2697	rVB	305	212	0.02%	0.003%
56	10.102	2722	2725	2728	rBV	251	213	0.02%	0.003%
57	10.143	2735	2738	2743	rVB2	279	227	0.02%	0.003%
58	10.394	2812	2816	2819	rBV2	253	266	0.03%	0.004%
59	10.462	2833	2837	2840	rVB2	251	207	0.02%	0.003%
60	10.523	2850	2856	2862	rVB	309	332	0.04%	0.004%
61	10.555	2862	2866	2872	rBV2	309	329	0.04%	0.004%
62	10.629	2886	2889	2895	rVB2	218	198	0.02%	0.003%
63	10.751	2915	2927	2945	rVV	284404	460723	49.56%	6.131%
64	10.893	2962	2971	2982	rBV4	1232	2103	0.23%	0.028%
65	10.941	2982	2986	2990	rBV2	217	236	0.03%	0.003%
66	10.989	2996	3001	3002	rBV	299	241	0.03%	0.003%
67	11.031	3010	3014	3020	rBV2	247	311	0.03%	0.004%
68	11.259	3081	3085	3088	rBV2	301	245	0.03%	0.003%
69	11.346	3109	3112	3115	rBV	320	215	0.02%	0.003%
70	11.465	3146	3149	3152	rBV2	357	242	0.03%	0.003%
71	11.587	3184	3187	3191	rBV2	364	385	0.04%	0.005%
72	11.661	3208	3210	3217	rBV	226	232	0.02%	0.003%
73	11.751	3236	3238	3243	rVB2	282	194	0.02%	0.003%
74	11.806	3243	3255	3279	rBV	447145	707523	76.11%	9.415%
75	12.069	3334	3337	3340	rBV	294	234	0.03%	0.003%
76	12.188	3360	3374	3399	rBV	420369	692353	74.48%	9.213%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054029.D
 Acq On : 01 May 2023 16:30
 Operator : JC/MD
 Sample : 02565-08
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	12.378	3428	3433	3440	rVB2	283	501	0.05%	0.007%
78	12.410	3440	3443	3447	rBV	397	347	0.04%	0.005%
79	12.677	3522	3526	3531	rVB2	307	307	0.03%	0.004%
80	12.777	3555	3557	3560	rVB2	367	194	0.02%	0.003%
81	12.799	3561	3564	3570	rBV2	461	502	0.05%	0.007%
82	12.909	3593	3598	3600	rBV3	300	291	0.03%	0.004%
83	12.967	3609	3616	3621	rBV2	310	433	0.05%	0.006%
84	12.989	3621	3623	3627	rBV2	312	206	0.02%	0.003%
85	13.253	3700	3705	3707	rBV2	213	251	0.03%	0.003%
86	13.323	3724	3727	3731	rBV2	229	216	0.02%	0.003%
87	13.397	3747	3750	3754	rBV2	336	362	0.04%	0.005%
88	13.568	3801	3803	3806	rVB2	349	180	0.02%	0.002%
89	13.635	3821	3824	3828	rBV	247	240	0.03%	0.003%
90	13.915	3909	3911	3914	rVB3	348	181	0.02%	0.002%
91	13.944	3917	3920	3922	rBV2	287	197	0.02%	0.003%
92	14.008	3937	3940	3942	rVB	373	227	0.02%	0.003%
93	14.040	3948	3950	3955	rBV2	297	238	0.03%	0.003%
94	14.272	4018	4022	4025	rBV2	433	362	0.04%	0.005%
95	14.352	4045	4047	4051	rBV3	387	331	0.04%	0.004%
96	14.764	4173	4175	4183	rVB4	586	588	0.06%	0.008%
97	15.368	4360	4363	4367	rBV	482	343	0.04%	0.005%
98	15.564	4421	4424	4427	rBV3	590	531	0.06%	0.007%
99	15.632	4442	4445	4447	rBV2	737	439	0.05%	0.006%
100	15.773	4484	4489	4491	rBV2	957	869	0.09%	0.012%




Sum of corrected areas: 7514656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054029.D
Acq On : 01 May 2023 16:30
Operator : JC/MD
Sample : 02565-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

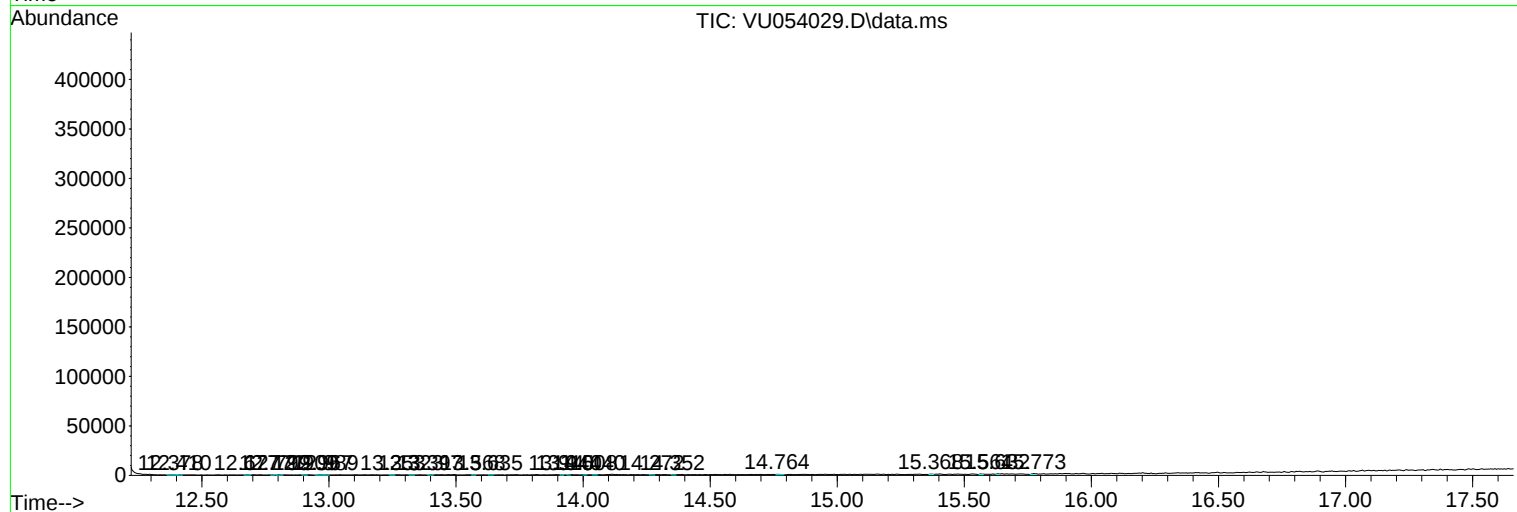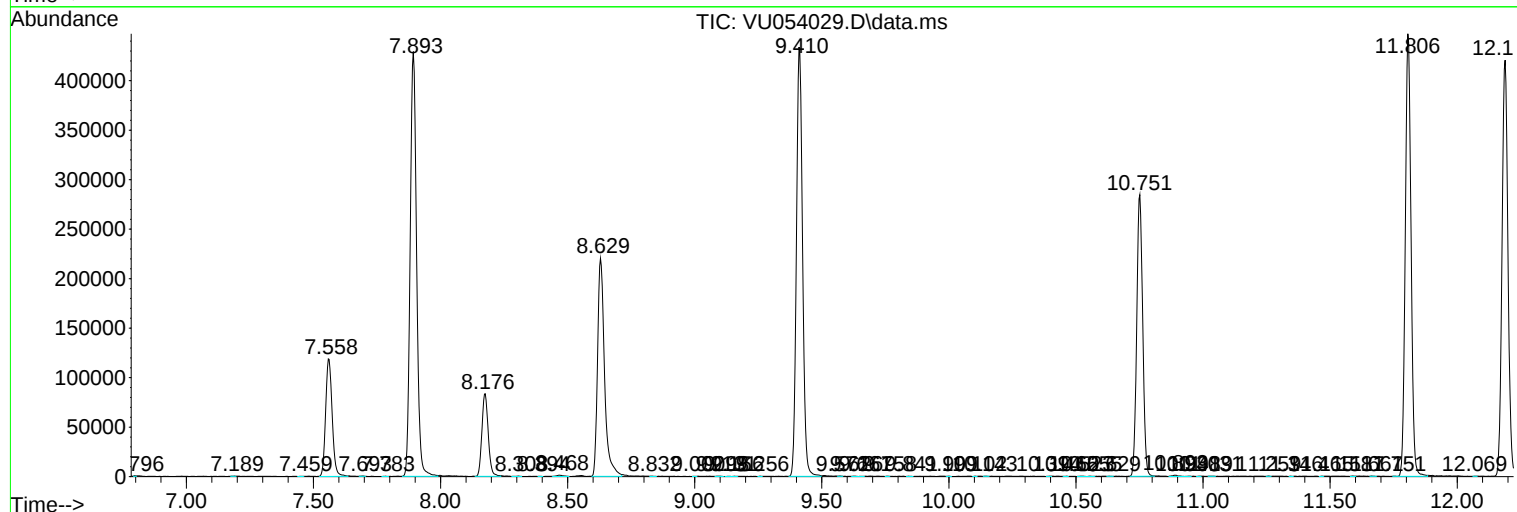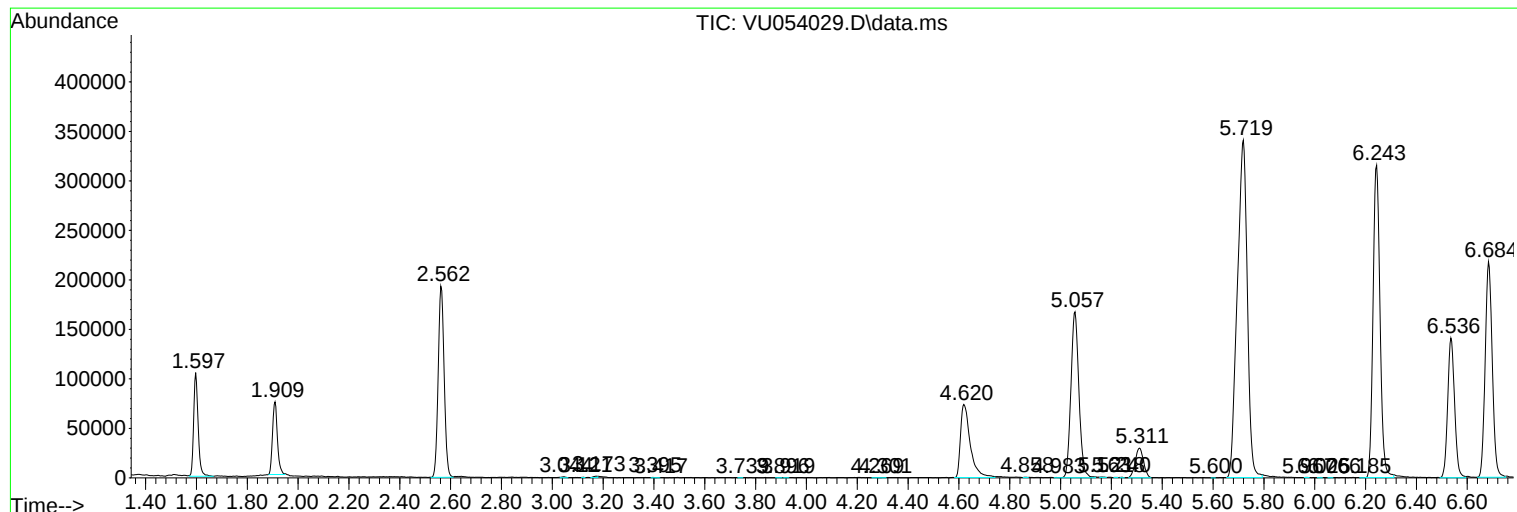

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054029.D
Acq On : 01 May 2023 16:30
Operator : JC/MD
Sample : 02565-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054029.D
Acq On : 01 May 2023 16:30
Operator : JC/MD
Sample : 02565-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------