

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054030.D
 Acq On : 01 May 2023 16:54
 Operator : JC/MD
 Sample : 02565-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	97	rVB	103055	125247	13.55%	1.727%
2	1.874	163	166	169	rBV3	1162	1093	0.12%	0.015%
3	1.909	169	177	194	rVB	71657	100441	10.87%	1.385%
4	2.372	317	321	322	rBV	723	566	0.06%	0.008%
5	2.562	367	380	396	rBV	190162	307095	33.23%	4.234%
6	2.732	429	433	437	rVB2	402	372	0.04%	0.005%
7	2.780	444	448	449	rBV	352	267	0.03%	0.004%
8	2.964	498	505	509	rVB2	312	453	0.05%	0.006%
9	2.996	511	515	519	rBV2	391	340	0.04%	0.005%
10	3.041	523	529	536	rBV3	778	1263	0.14%	0.017%
11	3.115	548	552	556	rBV2	355	346	0.04%	0.005%
12	3.150	560	563	564	rBV	381	211	0.02%	0.003%
13	3.372	625	632	636	rBV2	265	343	0.04%	0.005%
14	3.462	658	660	663	rVB	376	217	0.02%	0.003%
15	3.491	667	669	677	rVB2	199	238	0.03%	0.003%
16	3.533	677	682	684	rBV	320	298	0.03%	0.004%
17	3.575	690	695	698	rVB2	279	234	0.03%	0.003%
18	3.594	698	701	707	rBV2	369	325	0.04%	0.004%
19	4.147	870	873	878	rBV2	182	218	0.02%	0.003%
20	4.227	894	898	902	rBV2	237	238	0.03%	0.003%
21	4.253	902	906	909	rBV	295	233	0.03%	0.003%
22	4.465	967	972	977	rVB2	284	344	0.04%	0.005%
23	4.536	988	994	997	rBV	274	336	0.04%	0.005%
24	4.620	1008	1020	1055	rBV	73828	195719	21.18%	2.699%
25	5.057	1140	1156	1185	rBV	165338	364635	39.46%	5.028%
26	5.263	1216	1220	1223	rBV	245	218	0.02%	0.003%
27	5.620	1330	1331	1339	rVB	158	199	0.02%	0.003%
28	5.719	1340	1362	1391	rBV2	337852	924133	100.00%	12.742%
29	5.938	1428	1430	1435	rVB3	301	247	0.03%	0.003%
30	6.102	1479	1481	1483	rBV	387	220	0.02%	0.003%
31	6.243	1511	1525	1549	rBV	332657	627011	67.85%	8.645%
32	6.529	1603	1614	1627	rVB6	3349	6694	0.72%	0.092%
33	6.684	1648	1662	1683	rVV	214347	415503	44.96%	5.729%
34	6.973	1748	1752	1757	rBV2	246	208	0.02%	0.003%
35	7.083	1782	1786	1788	rBV	317	284	0.03%	0.004%
36	7.102	1788	1792	1796	rVV	258	314	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054030.D
 Acq On : 01 May 2023 16:54
 Operator : JC/MD
 Sample : 02565-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	7.301	1850	1854	1858	rBV2	222	258	0.03%	0.004%
38	7.491	1909	1913	1920	rBV2	210	265	0.03%	0.004%
39	7.558	1921	1934	1960	rBV	119827	209394	22.66%	2.887%
40	7.697	1974	1977	1982	rBV3	400	395	0.04%	0.005%
41	7.893	2022	2038	2063	rBV	416254	740202	80.10%	10.206%
42	8.131	2107	2112	2114	rBV2	246	252	0.03%	0.003%
43	8.172	2114	2125	2148	rVV	82993	143747	15.55%	1.982%
44	8.336	2173	2176	2180	rVB2	335	284	0.03%	0.004%
45	8.388	2187	2192	2195	rBV2	238	244	0.03%	0.003%
46	8.468	2206	2217	2223	rBV3	1567	2386	0.26%	0.033%
47	8.555	2235	2244	2254	rBV5	1643	2716	0.29%	0.037%
48	8.629	2256	2267	2303	rBV2	219893	420942	45.55%	5.804%
49	8.838	2330	2332	2336	rVB	360	253	0.03%	0.003%
50	8.867	2336	2341	2345	rBV3	313	328	0.04%	0.005%
51	8.970	2370	2373	2376	rBV2	229	198	0.02%	0.003%
52	9.012	2383	2386	2390	rVB	313	235	0.03%	0.003%
53	9.034	2390	2393	2399	rBV2	261	322	0.03%	0.004%
54	9.192	2438	2442	2445	rBV	200	208	0.02%	0.003%
55	9.410	2495	2510	2532	rBV	450423	748272	80.97%	10.317%
56	9.568	2557	2559	2563	rVB2	466	292	0.03%	0.004%
57	9.738	2609	2612	2617	rVB2	247	210	0.02%	0.003%
58	9.886	2654	2658	2662	rBV2	211	202	0.02%	0.003%
59	10.034	2701	2704	2710	rVB2	278	241	0.03%	0.003%
60	10.140	2734	2737	2744	rBV2	274	373	0.04%	0.005%
61	10.172	2744	2747	2752	rBV2	299	250	0.03%	0.003%
62	10.452	2830	2834	2840	rVB	239	224	0.02%	0.003%
63	10.523	2851	2856	2858	rBV	342	289	0.03%	0.004%
64	10.616	2882	2885	2890	rBV	287	234	0.03%	0.003%
65	10.751	2909	2927	2946	rBV	288769	465124	50.33%	6.413%
66	10.848	2953	2957	2963	rVB2	312	348	0.04%	0.005%
67	10.893	2963	2971	2978	rBV4	1537	2252	0.24%	0.031%
68	11.037	3012	3016	3020	rBV2	281	348	0.04%	0.005%
69	11.147	3046	3050	3054	rBV	216	198	0.02%	0.003%
70	11.420	3130	3135	3140	rBV	307	360	0.04%	0.005%
71	11.465	3146	3149	3152	rBV2	333	224	0.02%	0.003%
72	11.526	3162	3168	3171	rBV2	289	366	0.04%	0.005%
73	11.639	3197	3203	3206	rBV	231	308	0.03%	0.004%
74	11.722	3225	3229	3232	rBV2	269	246	0.03%	0.003%
75	11.806	3242	3255	3281	rBV	466494	735163	79.55%	10.136%
76	12.028	3318	3324	3328	rVB2	207	302	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054030.D
 Acq On : 01 May 2023 16:54
 Operator : JC/MD
 Sample : 02565-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	12.188	3359	3374	3395	rBV	427447	690340	74.70%	9.518%
78	12.359	3422	3427	3429	rBV2	213	231	0.02%	0.003%
79	12.433	3446	3450	3453	rBV2	251	232	0.03%	0.003%
80	12.452	3453	3456	3459	rBV2	213	198	0.02%	0.003%
81	12.639	3510	3514	3517	rBV2	285	261	0.03%	0.004%
82	12.796	3560	3563	3566	rVB2	388	270	0.03%	0.004%
83	13.204	3687	3690	3694	rVB2	390	343	0.04%	0.005%
84	13.266	3706	3709	3712	rVB2	336	236	0.03%	0.003%
85	13.346	3732	3734	3737	rBV	416	216	0.02%	0.003%
86	13.581	3804	3807	3810	rVB2	461	328	0.04%	0.005%
87	13.626	3818	3821	3827	rBV2	408	484	0.05%	0.007%
88	13.790	3868	3872	3877	rBV3	381	397	0.04%	0.005%
89	13.851	3889	3891	3895	rVB	481	247	0.03%	0.003%
90	13.873	3895	3898	3900	rBV2	458	252	0.03%	0.003%
91	14.095	3963	3967	3970	rBV2	447	462	0.05%	0.006%
92	14.163	3985	3988	3991	rBV3	383	222	0.02%	0.003%
93	14.243	4007	4013	4016	rBV2	400	477	0.05%	0.007%
94	14.272	4019	4022	4025	rBV2	423	388	0.04%	0.005%
95	14.709	4155	4158	4162	rBV2	499	446	0.05%	0.006%
96	14.995	4245	4247	4252	rBV	341	199	0.02%	0.003%
97	15.413	4374	4377	4381	rBV3	667	465	0.05%	0.006%
98	15.491	4393	4401	4404	rBV3	565	884	0.10%	0.012%
99	15.507	4404	4406	4409	rBV3	486	372	0.04%	0.005%
100	15.632	4443	4445	4447	rVB2	668	295	0.03%	0.004%

Sum of corrected areas: 7252803




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054030.D
Acq On : 01 May 2023 16:54
Operator : JC/MD
Sample : 02565-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

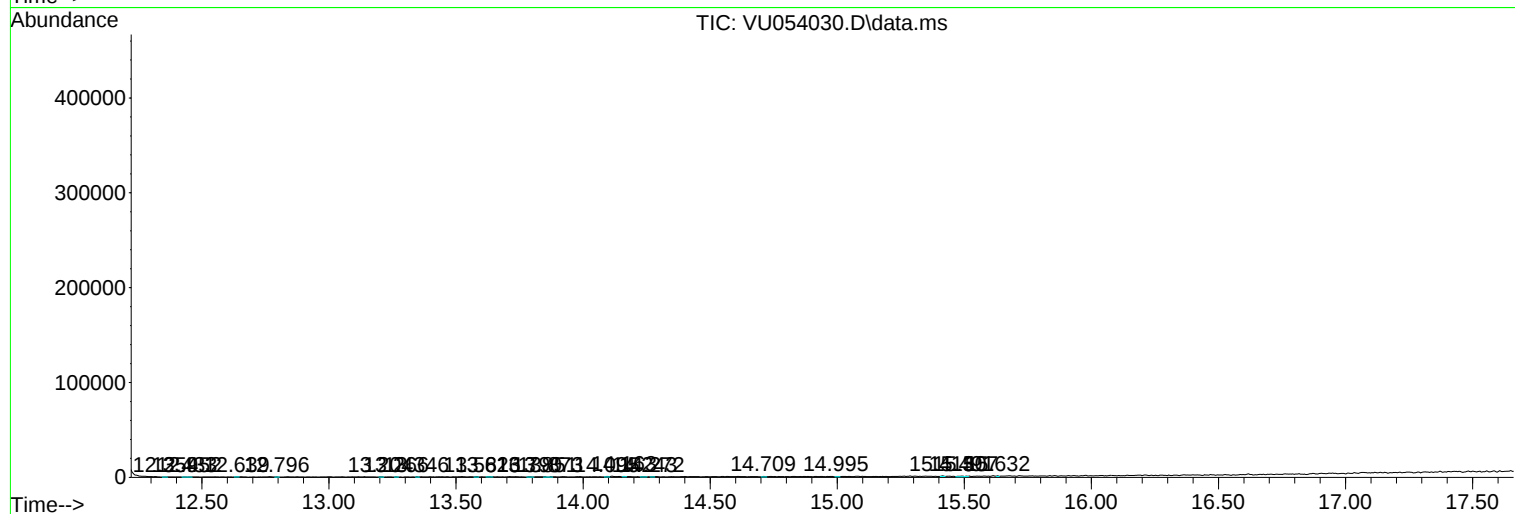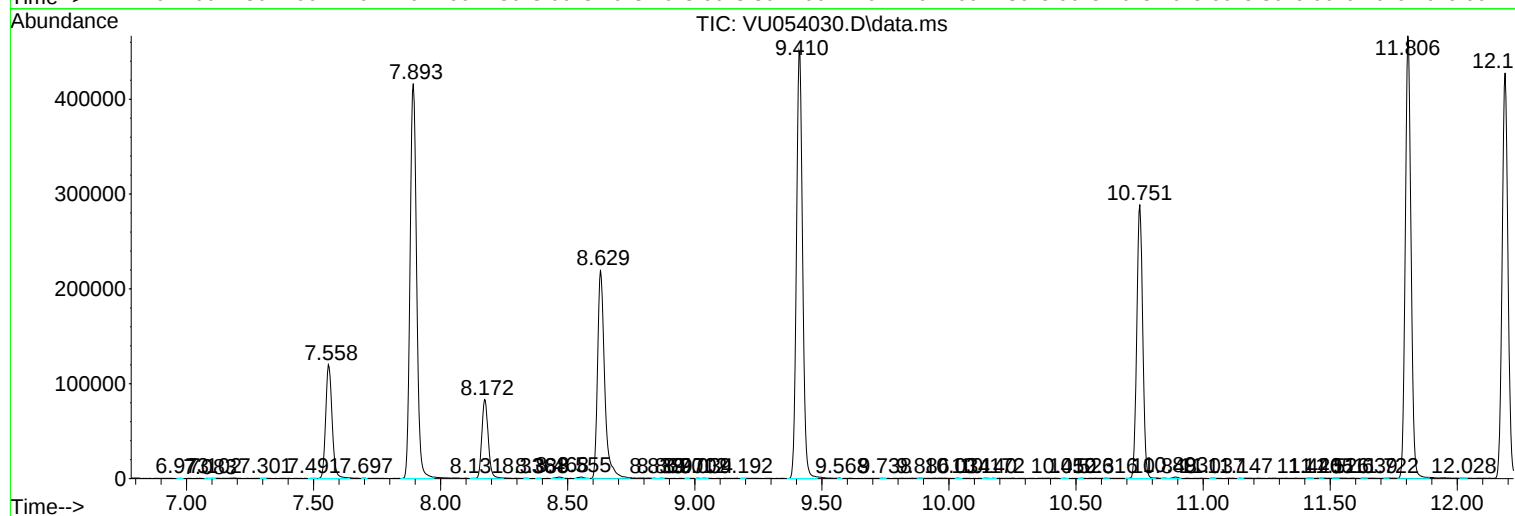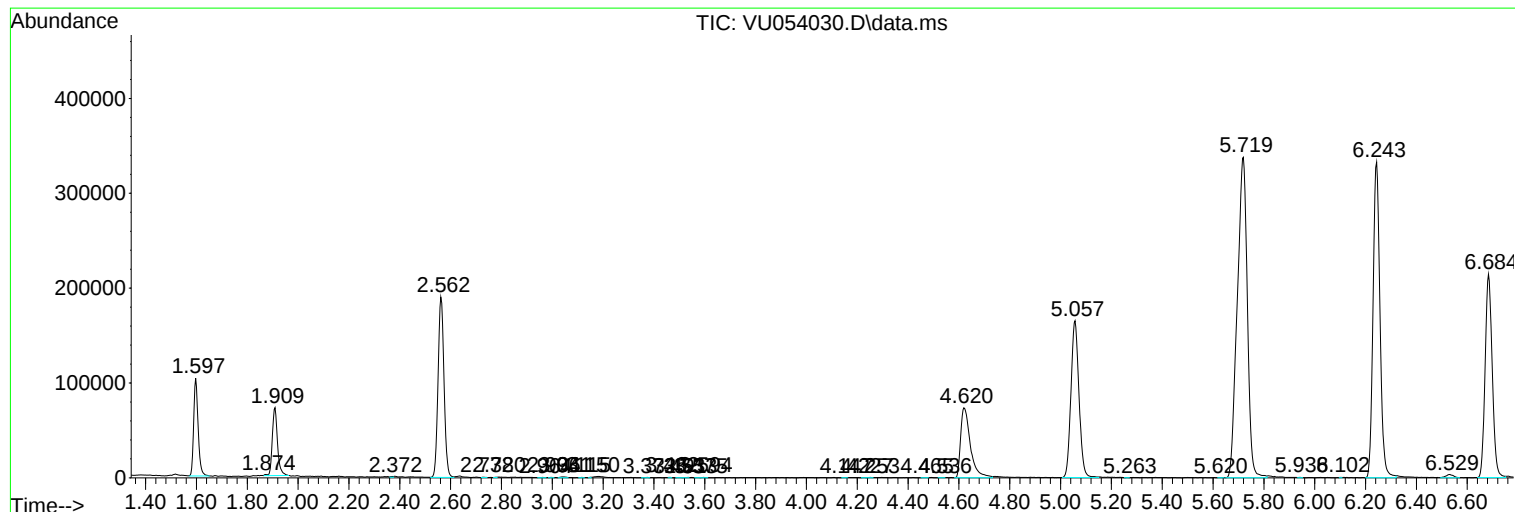

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054030.D
Acq On : 01 May 2023 16:54
Operator : JC/MD
Sample : 02565-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054030.D
Acq On : 01 May 2023 16:54
Operator : JC/MD
Sample : 02565-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------