

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054035.D
 Acq On : 01 May 2023 18:52
 Operator : JC/MD
 Sample : 02565-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054035.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.495	43	48	51	rBV4	1109	1457	0.17%	0.021%
2	1.597	72	80	98	rVB	96323	118220	13.60%	1.728%
3	1.906	168	176	196	rVB	74418	104753	12.05%	1.531%
4	2.234	275	278	280	rBV	691	541	0.06%	0.008%
5	2.562	368	380	397	rBV	178014	289816	33.35%	4.236%
6	2.630	397	401	406	rVB2	898	909	0.10%	0.013%
7	2.697	417	422	424	rBV3	562	477	0.05%	0.007%
8	2.745	433	437	441	rVV	237	221	0.03%	0.003%
9	2.855	469	471	477	rBV	401	271	0.03%	0.004%
10	2.912	486	489	492	rBV	291	207	0.02%	0.003%
11	3.038	524	528	537	rVB4	960	1344	0.15%	0.020%
12	3.176	562	571	574	rBV3	1158	1684	0.19%	0.025%
13	3.462	657	660	662	rBV	268	217	0.02%	0.003%
14	4.076	846	851	855	rBV2	344	465	0.05%	0.007%
15	4.147	868	873	876	rVB	238	241	0.03%	0.004%
16	4.392	944	949	952	rBV2	203	223	0.03%	0.003%
17	4.414	953	956	963	rVB	282	308	0.04%	0.005%
18	4.456	966	969	974	rBV2	312	307	0.04%	0.004%
19	4.498	979	982	985	rBV2	268	235	0.03%	0.003%
20	4.620	1008	1020	1051	rBV2	66998	171240	19.70%	2.503%
21	4.822	1078	1083	1086	rVB2	454	366	0.04%	0.005%
22	4.890	1101	1104	1109	rBV	334	287	0.03%	0.004%
23	4.951	1119	1123	1126	rBV3	286	240	0.03%	0.004%
24	5.057	1139	1156	1175	rVV	153349	344985	39.69%	5.043%
25	5.205	1200	1202	1208	rVB4	513	379	0.04%	0.006%
26	5.311	1229	1235	1241	rBV4	1064	1722	0.20%	0.025%
27	5.443	1273	1276	1281	rVB	331	235	0.03%	0.003%
28	5.485	1285	1289	1292	rBV2	228	211	0.02%	0.003%
29	5.719	1340	1362	1384	rBV2	321011	869101	100.00%	12.704%
30	5.945	1428	1432	1435	rVB	441	293	0.03%	0.004%
31	5.964	1435	1438	1440	rBV3	330	255	0.03%	0.004%
32	6.028	1456	1458	1463	rVB	300	198	0.02%	0.003%
33	6.182	1502	1506	1509	rBV2	254	287	0.03%	0.004%
34	6.244	1511	1525	1541	rBV	309158	589941	67.88%	8.623%
35	6.530	1608	1614	1622	rBV5	1865	2960	0.34%	0.043%
36	6.684	1648	1662	1686	rBV	201569	392681	45.18%	5.740%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054035.D
 Acq On : 01 May 2023 18:52
 Operator : JC/MD
 Sample : 02565-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.797	1693	1697	1698	rBV3	310	205	0.02%	0.003%
38	6.861	1715	1717	1723	rBV	323	308	0.04%	0.005%
39	7.044	1772	1774	1781	rVB2	175	235	0.03%	0.003%
40	7.089	1785	1788	1792	rVB2	289	251	0.03%	0.004%
41	7.125	1793	1799	1803	rBV2	398	481	0.06%	0.007%
42	7.179	1810	1816	1817	rBV3	363	315	0.04%	0.005%
43	7.305	1852	1855	1859	rBV2	214	200	0.02%	0.003%
44	7.334	1860	1864	1870	rVB2	292	344	0.04%	0.005%
45	7.559	1921	1934	1959	rBV	110529	197107	22.68%	2.881%
46	7.690	1973	1975	1981	rVB2	460	453	0.05%	0.007%
47	7.774	1995	2001	2003	rBV	185	234	0.03%	0.003%
48	7.893	2024	2038	2071	rBV	405327	706513	81.29%	10.327%
49	8.006	2071	2073	2077	rVB2	405	202	0.02%	0.003%
50	8.083	2095	2097	2102	rVB3	494	320	0.04%	0.005%
51	8.173	2112	2125	2142	rBV2	79366	134582	15.49%	1.967%
52	8.353	2176	2181	2185	rBV2	248	276	0.03%	0.004%
53	8.465	2206	2216	2226	rVV2	2151	3758	0.43%	0.055%
54	8.542	2237	2240	2243	rBV3	1085	825	0.09%	0.012%
55	8.629	2255	2267	2298	rBV2	202907	383596	44.14%	5.607%
56	8.790	2315	2317	2322	rVB2	412	267	0.03%	0.004%
57	8.922	2356	2358	2364	rBV	305	286	0.03%	0.004%
58	8.967	2369	2372	2380	rBV2	229	362	0.04%	0.005%
59	9.163	2431	2433	2440	rVB	218	228	0.03%	0.003%
60	9.221	2443	2451	2455	rVB2	307	444	0.05%	0.006%
61	9.260	2458	2463	2465	rBV	195	210	0.02%	0.003%
62	9.411	2494	2510	2534	rBV	421085	703242	80.92%	10.279%
63	9.571	2556	2560	2562	rBV3	404	332	0.04%	0.005%
64	9.626	2570	2577	2585	rVB2	276	535	0.06%	0.008%
65	10.095	2721	2723	2726	rVV	421	240	0.03%	0.004%
66	10.478	2839	2842	2844	rBV	425	312	0.04%	0.005%
67	10.751	2914	2927	2946	rVV	273914	439540	50.57%	6.425%
68	10.886	2959	2969	2980	rBV3	2789	4649	0.53%	0.068%
69	10.973	2992	2996	3001	rVB2	226	257	0.03%	0.004%
70	11.185	3059	3062	3067	rBV2	237	251	0.03%	0.004%
71	11.218	3067	3072	3077	rVB2	297	280	0.03%	0.004%
72	11.292	3088	3095	3101	rVV2	195	324	0.04%	0.005%
73	11.362	3114	3117	3122	rVB	349	202	0.02%	0.003%
74	11.491	3154	3157	3164	rVB	334	309	0.04%	0.005%
75	11.726	3225	3230	3233	rBV2	273	233	0.03%	0.003%
76	11.806	3243	3255	3282	rBV	438005	696065	80.09%	10.174%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054035.D
 Acq On : 01 May 2023 18:52
 Operator : JC/MD
 Sample : 02565-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AY7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	11.960	3299	3303	3307	rBV4	437	430	0.05%	0.006%
78	12.189	3360	3374	3391	rBV	407588	658220	75.74%	9.621%
79	12.394	3435	3438	3443	rBV	200	233	0.03%	0.003%
80	12.529	3477	3480	3483	rBV2	265	212	0.02%	0.003%
81	12.584	3494	3497	3499	rBV2	283	221	0.03%	0.003%
82	12.632	3510	3512	3516	rVB2	285	200	0.02%	0.003%
83	12.658	3516	3520	3523	rBV	319	355	0.04%	0.005%
84	12.764	3551	3553	3556	rBV	725	452	0.05%	0.007%
85	13.076	3646	3650	3653	rBV2	199	221	0.03%	0.003%
86	13.327	3723	3728	3731	rBV2	367	368	0.04%	0.005%
87	13.382	3742	3745	3748	rVB2	295	197	0.02%	0.003%
88	13.549	3794	3797	3800	rBV2	241	205	0.02%	0.003%
89	13.796	3871	3874	3876	rBV2	265	190	0.02%	0.003%
90	13.845	3885	3889	3890	rBV2	474	281	0.03%	0.004%
91	13.896	3903	3905	3909	rVB2	298	190	0.02%	0.003%
92	14.021	3942	3944	3948	rBV2	242	193	0.02%	0.003%
93	14.269	4016	4021	4023	rVV3	249	228	0.03%	0.003%
94	14.340	4037	4043	4046	rBV2	425	460	0.05%	0.007%
95	14.533	4102	4103	4108	rVB	361	211	0.02%	0.003%
96	14.690	4147	4152	4155	rBV2	638	648	0.07%	0.009%
97	14.983	4240	4243	4246	rBV	518	421	0.05%	0.006%
98	15.150	4292	4295	4301	rBB3	356	377	0.04%	0.006%
99	15.250	4324	4326	4331	rBV2	396	293	0.03%	0.004%
100	15.770	4485	4488	4490	rBV2	783	495	0.06%	0.007%




Sum of corrected areas: 6841351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054035.D
Acq On : 01 May 2023 18:52
Operator : JC/MD
Sample : 02565-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

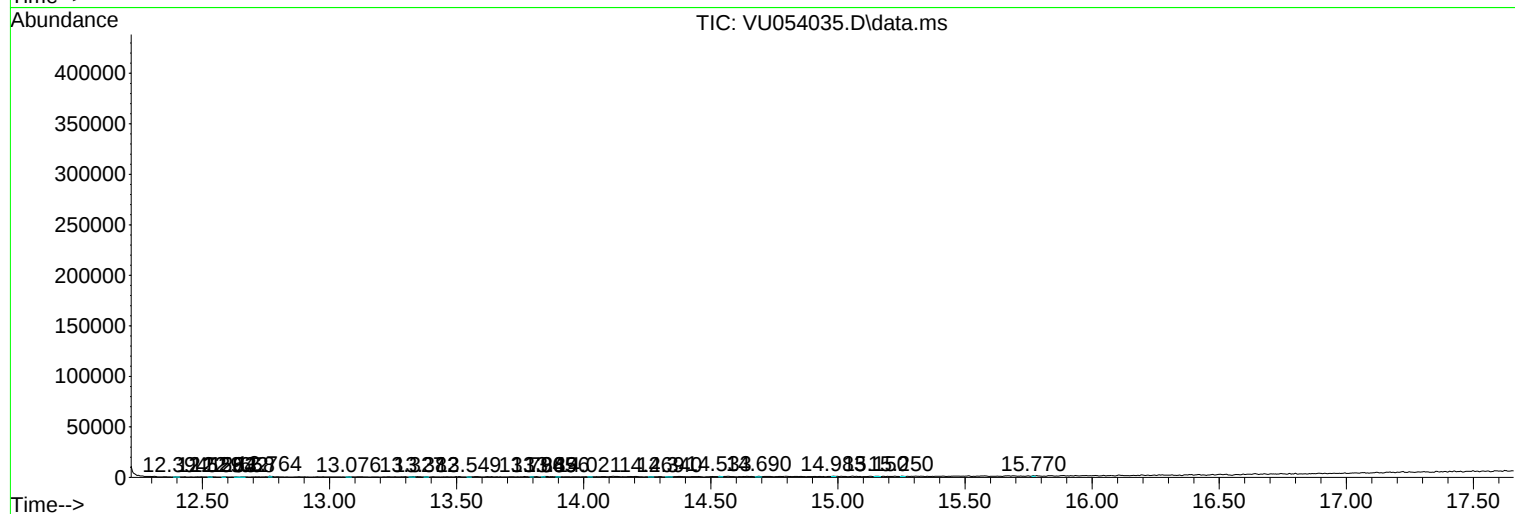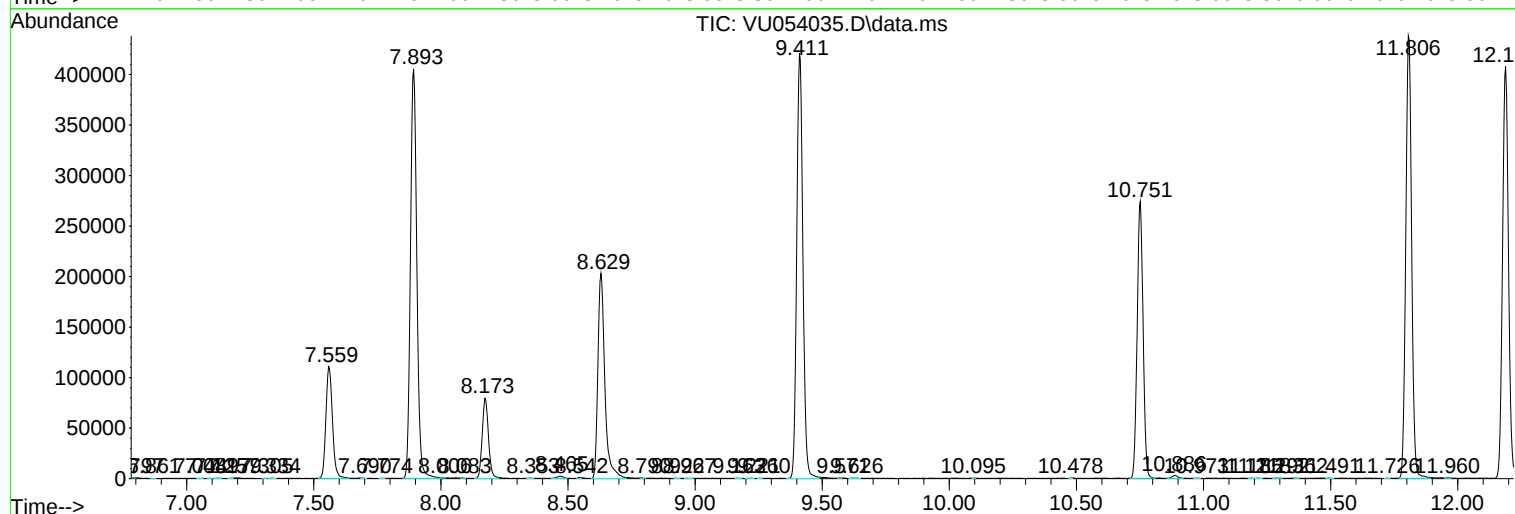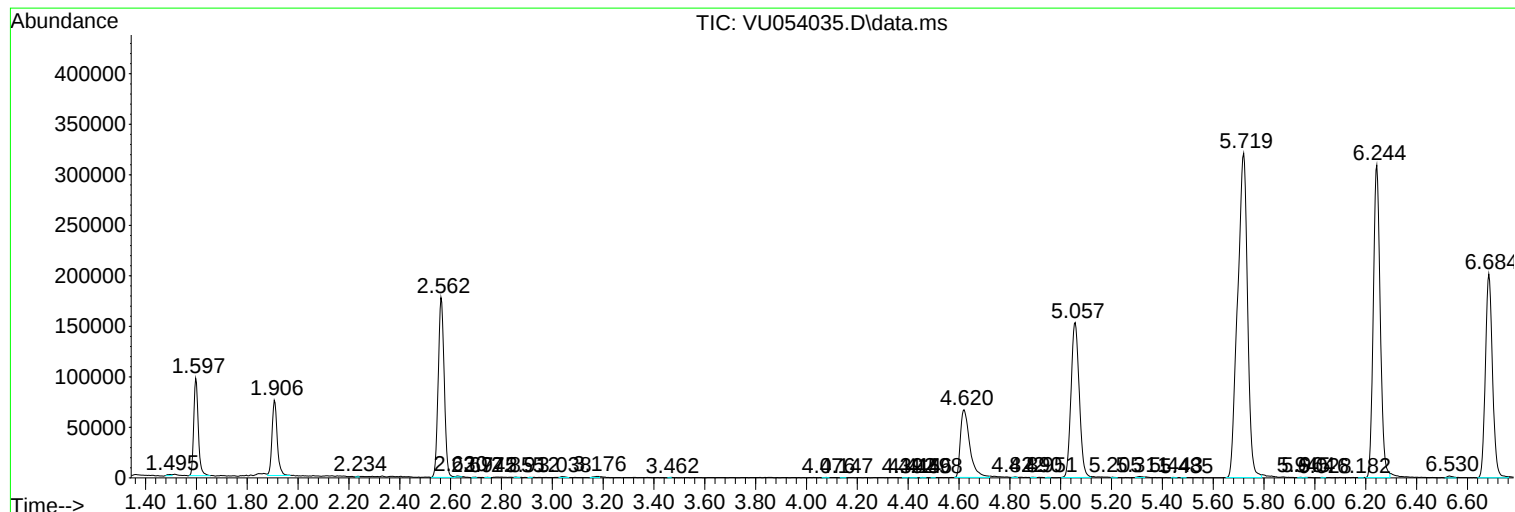

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054035.D
Acq On : 01 May 2023 18:52
Operator : JC/MD
Sample : 02565-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054035.D
Acq On : 01 May 2023 18:52
Operator : JC/MD
Sample : 02565-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AY7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------