

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054038.D
 Acq On : 01 May 2023 20:02
 Operator : JC/MD
 Sample : 02548-31ME
 Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCR1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

Signal : TIC: VU054038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	100920	122888	13.19%	1.728%
2	1.906	169	176	192	rVB	79627	108034	11.59%	1.520%
3	2.562	368	380	397	rBV	185540	303872	32.61%	4.274%
4	2.694	418	421	425	rBV2	370	296	0.03%	0.004%
5	2.954	496	502	506	rBV2	250	310	0.03%	0.004%
6	3.041	520	529	540	rBV4	4024	7133	0.77%	0.100%
7	3.263	597	598	599	rBV	202	68	0.01%	0.001%
8	3.308	610	612	615	rVB	210	101	0.01%	0.001%
9	3.327	616	618	622	rVV2	195	126	0.01%	0.002%
10	3.501	668	672	675	rBV2	276	218	0.02%	0.003%
11	3.543	680	685	688	rBV2	273	263	0.03%	0.004%
12	3.729	741	743	744	rBV	206	108	0.01%	0.002%
13	3.809	766	768	771	rBV	221	160	0.02%	0.002%
14	3.864	782	785	788	rBV2	193	116	0.01%	0.002%
15	3.935	804	807	809	rBV2	316	213	0.02%	0.003%
16	3.948	809	811	814	rVV	253	169	0.02%	0.002%
17	3.964	814	816	819	rVB2	282	177	0.02%	0.002%
18	3.989	819	824	828	rBV2	449	564	0.06%	0.008%
19	4.198	886	889	890	rBV	219	114	0.01%	0.002%
20	4.224	896	897	898	rBV	296	94	0.01%	0.001%
21	4.301	918	921	923	rBV2	222	134	0.01%	0.002%
22	4.317	923	926	931	rVB2	213	198	0.02%	0.003%
23	4.401	950	952	955	rBV	156	128	0.01%	0.002%
24	4.507	981	985	987	rBV	236	212	0.02%	0.003%
25	4.620	1009	1020	1045	rBV2	70178	174120	18.68%	2.449%
26	4.960	1124	1126	1128	rBV	210	127	0.01%	0.002%
27	5.057	1135	1156	1180	rBV	168070	370422	39.75%	5.210%
28	5.272	1221	1223	1224	rBV	252	96	0.01%	0.001%
29	5.546	1306	1308	1310	rBV2	176	105	0.01%	0.001%
30	5.719	1341	1362	1391	rBV2	340159	931918	100.00%	13.108%
31	6.063	1467	1469	1470	rBV	167	45	0.00%	0.001%
32	6.099	1477	1480	1482	rBV	252	120	0.01%	0.002%
33	6.169	1499	1502	1508	rBV2	256	294	0.03%	0.004%
34	6.243	1511	1525	1553	rBV	306077	590241	63.34%	8.302%
35	6.440	1583	1586	1590	rVB2	319	184	0.02%	0.003%
36	6.456	1590	1591	1594	rVB2	299	109	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054038.D
 Acq On : 01 May 2023 20:02
 Operator : JC/MD
 Sample : 02548-31ME
 Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCR1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.472	1594	1596	1599	rBV	213	129	0.01%	0.002%
38	6.526	1605	1613	1625	rVB5	2701	4401	0.47%	0.062%
39	6.616	1638	1641	1645	rVB2	209	160	0.02%	0.002%
40	6.639	1645	1648	1649	rBV	254	161	0.02%	0.002%
41	6.684	1649	1662	1682	rBV2	215414	418667	44.93%	5.889%
42	7.115	1792	1796	1798	rBV	245	201	0.02%	0.003%
43	7.224	1827	1830	1834	rBV	185	110	0.01%	0.002%
44	7.558	1923	1934	1962	rBV	115662	205905	22.09%	2.896%
45	7.722	1982	1985	1988	rBV2	239	169	0.02%	0.002%
46	7.742	1988	1991	1994	rVV	222	124	0.01%	0.002%
47	7.893	2025	2038	2073	rBV	423462	740838	79.50%	10.420%
48	8.076	2093	2095	2099	rVB2	436	234	0.03%	0.003%
49	8.099	2099	2102	2108	rBV2	350	405	0.04%	0.006%
50	8.173	2115	2125	2146	rBV	84056	140294	15.05%	1.973%
51	8.365	2183	2185	2186	rBV	135	55	0.01%	0.001%
52	8.546	2237	2241	2243	rBV3	770	653	0.07%	0.009%
53	8.568	2245	2248	2251	rVB	317	199	0.02%	0.003%
54	8.629	2253	2267	2293	rBV2	216344	400521	42.98%	5.633%
55	8.780	2311	2314	2321	rVB2	721	621	0.07%	0.009%
56	8.829	2326	2329	2333	rVB	443	327	0.04%	0.005%
57	8.996	2377	2381	2383	rBV	195	135	0.01%	0.002%
58	9.163	2431	2433	2434	rBV	173	76	0.01%	0.001%
59	9.192	2440	2442	2444	rBV	192	86	0.01%	0.001%
60	9.237	2451	2456	2458	rBV	232	232	0.02%	0.003%
61	9.410	2498	2510	2536	rBV	424870	712955	76.50%	10.028%
62	9.594	2566	2567	2568	rBV	129	39	0.00%	0.001%
63	9.603	2568	2570	2575	rVB	255	165	0.02%	0.002%
64	9.706	2599	2602	2608	rBV2	341	262	0.03%	0.004%
65	9.845	2642	2645	2647	rBV	246	128	0.01%	0.002%
66	9.925	2667	2670	2674	rBV	247	201	0.02%	0.003%
67	10.121	2728	2731	2734	rBV	262	225	0.02%	0.003%
68	10.269	2774	2777	2779	rBV	219	150	0.02%	0.002%
69	10.552	2863	2865	2867	rBV	175	76	0.01%	0.001%
70	10.706	2910	2913	2914	rBV	300	164	0.02%	0.002%
71	10.751	2914	2927	2949	rVB	285013	463559	49.74%	6.520%
72	11.034	3012	3015	3016	rBV	217	122	0.01%	0.002%
73	11.578	3179	3184	3188	rBV2	231	296	0.03%	0.004%
74	11.687	3215	3218	3222	rBV	238	175	0.02%	0.002%
75	11.806	3243	3255	3281	rBV	448428	707959	75.97%	9.958%
76	11.992	3310	3313	3315	rBV	429	232	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054038.D
Acq On : 01 May 2023 20:02
Operator : JC/MD
Sample : 02548-31ME
Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCR1ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M

Title : VOC Analysis

77	12.012	3315	3319	3321	rBV2	318	250	0.03%	0.004%
78	12.188	3361	3374	3393	rBV	433650	694664	74.54%	9.771%


Sum of corrected areas: 7109802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054038.D
Acq On : 01 May 2023 20:02
Operator : JC/MD
Sample : 02548-31ME
Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCR1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

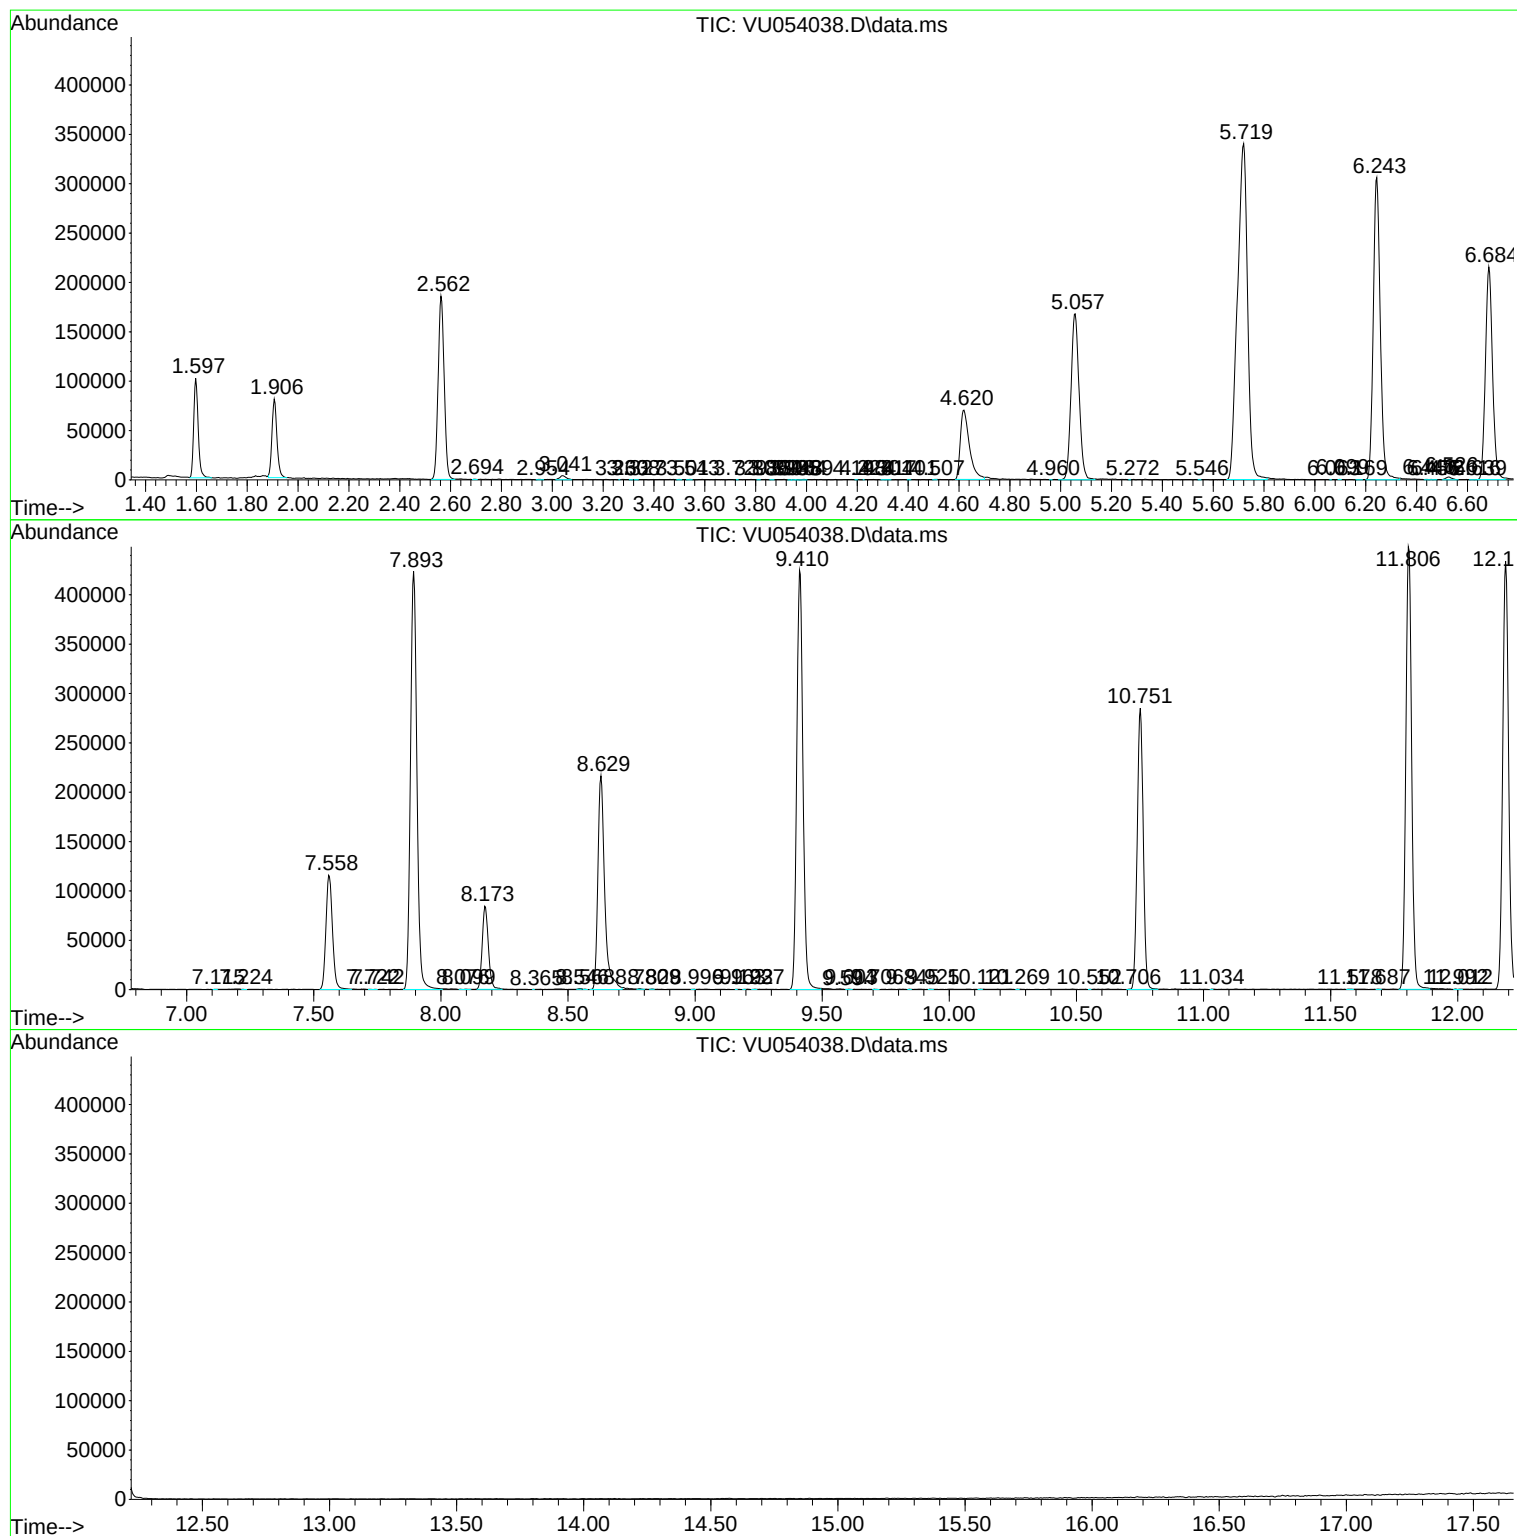

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054038.D
Acq On : 01 May 2023 20:02
Operator : JC/MD
Sample : 02548-31ME
Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCR1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054038.D
Acq On : 01 May 2023 20:02
Operator : JC/MD
Sample : 02548-31ME
Misc : 6.27g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCR1ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------