

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054039.D
 Acq On : 01 May 2023 20:26
 Operator : JC/MD
 Sample : 02565-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	107	rVB	99607	123662	13.43%	1.747%
2	1.903	169	175	193	rVB	73009	103800	11.28%	1.466%
3	2.562	368	380	397	rBV	186693	299652	32.55%	4.233%
4	2.790	447	451	455	rBV3	353	368	0.04%	0.005%
5	2.960	501	504	506	rBV2	184	117	0.01%	0.002%
6	2.993	511	514	516	rVV2	191	131	0.01%	0.002%
7	3.041	520	529	542	rVB4	3577	6738	0.73%	0.095%
8	3.160	561	566	568	rBV	226	186	0.02%	0.003%
9	3.324	614	617	619	rBV	230	165	0.02%	0.002%
10	3.504	671	673	676	rBV	238	142	0.02%	0.002%
11	3.825	769	773	777	rVB	283	233	0.03%	0.003%
12	3.851	777	781	784	rBV2	225	232	0.03%	0.003%
13	3.932	803	806	808	rBV	193	126	0.01%	0.002%
14	3.977	817	820	822	rBV2	224	158	0.02%	0.002%
15	4.118	860	864	866	rBV2	128	111	0.01%	0.002%
16	4.147	871	873	876	rBV	205	119	0.01%	0.002%
17	4.202	887	890	892	rBV	217	122	0.01%	0.002%
18	4.288	913	917	919	rBV	244	195	0.02%	0.003%
19	4.346	928	935	937	rBV2	204	278	0.03%	0.004%
20	4.468	969	973	980	rBV2	257	325	0.04%	0.005%
21	4.620	1008	1020	1048	rBV	74744	186675	20.28%	2.637%
22	4.980	1129	1132	1133	rBV2	371	228	0.02%	0.003%
23	5.057	1141	1156	1178	rBV	163226	360058	39.11%	5.087%
24	5.259	1216	1219	1223	rBV2	238	187	0.02%	0.003%
25	5.327	1235	1240	1242	rBV3	341	374	0.04%	0.005%
26	5.430	1269	1272	1273	rBV	171	116	0.01%	0.002%
27	5.501	1289	1294	1297	rVV2	231	192	0.02%	0.003%
28	5.607	1324	1327	1331	rBV2	216	200	0.02%	0.003%
29	5.719	1340	1362	1393	rBV2	333545	920594	100.00%	13.006%
30	5.954	1431	1435	1442	rBV2	308	436	0.05%	0.006%
31	5.999	1446	1449	1453	rBV	329	318	0.03%	0.004%
32	6.128	1485	1489	1492	rBV2	328	212	0.02%	0.003%
33	6.144	1492	1494	1499	rVB2	224	173	0.02%	0.002%
34	6.243	1509	1525	1549	rBV	307448	591405	64.24%	8.355%
35	6.462	1590	1593	1595	rBV	238	134	0.01%	0.002%
36	6.523	1605	1612	1624	rVB4	2670	4477	0.49%	0.063%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054039.D
 Acq On : 01 May 2023 20:26
 Operator : JC/MD
 Sample : 02565-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.594	1630	1634	1636	rBV2	339	197	0.02%	0.003%
38	6.684	1647	1662	1690	rBV	214186	419278	45.54%	5.923%
39	6.835	1706	1709	1714	rBV	281	249	0.03%	0.004%
40	7.015	1763	1765	1768	rBV	184	134	0.01%	0.002%
41	7.047	1772	1775	1778	rBV2	287	202	0.02%	0.003%
42	7.269	1840	1844	1850	rVB2	193	188	0.02%	0.003%
43	7.327	1860	1862	1865	rBV	193	135	0.01%	0.002%
44	7.433	1892	1895	1897	rBV	176	141	0.02%	0.002%
45	7.562	1922	1935	1961	rBV	114974	205011	22.27%	2.896%
46	7.809	2010	2012	2015	rBV	275	142	0.02%	0.002%
47	7.893	2025	2038	2066	rVV	417820	735246	79.87%	10.387%
48	8.131	2109	2112	2114	rBV2	222	157	0.02%	0.002%
49	8.172	2114	2125	2141	rBV	83610	139295	15.13%	1.968%
50	8.304	2165	2166	2171	rVB2	220	128	0.01%	0.002%
51	8.353	2178	2181	2183	rBV	179	128	0.01%	0.002%
52	8.375	2183	2188	2191	rVV	224	227	0.02%	0.003%
53	8.436	2201	2207	2211	rBV2	364	444	0.05%	0.006%
54	8.468	2211	2217	2224	rVB2	459	635	0.07%	0.009%
55	8.549	2237	2242	2249	rBV4	1058	1372	0.15%	0.019%
56	8.629	2255	2267	2292	rBV	225054	412616	44.82%	5.829%
57	9.012	2380	2386	2389	rVV2	250	250	0.03%	0.004%
58	9.108	2414	2416	2422	rVB	268	241	0.03%	0.003%
59	9.140	2423	2426	2428	rBV	192	141	0.02%	0.002%
60	9.198	2441	2444	2446	rBV	230	125	0.01%	0.002%
61	9.243	2455	2458	2462	rBV2	258	251	0.03%	0.004%
62	9.285	2466	2471	2474	rBV	192	199	0.02%	0.003%
63	9.307	2476	2478	2481	rVB	296	123	0.01%	0.002%
64	9.330	2481	2485	2488	rBV	125	115	0.01%	0.002%
65	9.410	2498	2510	2532	rBV	425218	703786	76.45%	9.943%
66	9.594	2564	2567	2570	rBV	349	285	0.03%	0.004%
67	9.658	2583	2587	2590	rBV2	265	229	0.02%	0.003%
68	9.770	2618	2622	2628	rBV2	231	312	0.03%	0.004%
69	9.825	2636	2639	2641	rBV	237	164	0.02%	0.002%
70	9.973	2682	2685	2688	rBV	152	129	0.01%	0.002%
71	10.028	2699	2702	2706	rVB	217	173	0.02%	0.002%
72	10.057	2706	2711	2715	rBV2	205	190	0.02%	0.003%
73	10.115	2725	2729	2735	rBV2	244	371	0.04%	0.005%
74	10.176	2746	2748	2751	rBV2	186	112	0.01%	0.002%
75	10.230	2762	2765	2769	rVB	218	183	0.02%	0.003%
76	10.250	2769	2771	2775	rBV	162	132	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
 Data File : VU054039.D
 Acq On : 01 May 2023 20:26
 Operator : JC/MD
 Sample : 02565-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	10.452	2828	2834	2837	rBV2	218	299	0.03%	0.004%
78	10.533	2856	2859	2862	rBV	193	165	0.02%	0.002%
79	10.571	2868	2871	2873	rBV	257	149	0.02%	0.002%
80	10.751	2915	2927	2944	rBV	288415	466058	50.63%	6.584%
81	10.928	2979	2982	2985	rBV2	276	213	0.02%	0.003%
82	10.970	2989	2995	2997	rBV	185	209	0.02%	0.003%
83	11.082	3027	3030	3032	rBV	169	114	0.01%	0.002%
84	11.465	3146	3149	3152	rVB2	169	146	0.02%	0.002%
85	11.623	3195	3198	3202	rVB	324	223	0.02%	0.003%
86	11.690	3216	3219	3220	rBV	169	120	0.01%	0.002%
87	11.806	3242	3255	3279	rBV	434305	696196	75.62%	9.836%
88	12.073	3335	3338	3342	rBV2	311	321	0.03%	0.005%
89	12.114	3348	3351	3354	rBV	292	220	0.02%	0.003%
90	12.188	3361	3374	3391	rBV	424458	685469	74.46%	9.684%
91	12.613	3503	3506	3509	rBV	330	230	0.02%	0.003%
92	12.809	3563	3567	3570	rVB2	394	296	0.03%	0.004%
93	12.828	3570	3573	3577	rBV	313	320	0.03%	0.005%
94	12.873	3584	3587	3589	rBV	312	245	0.03%	0.003%
95	12.967	3613	3616	3618	rBV	386	312	0.03%	0.004%
96	13.185	3680	3684	3685	rBV	260	159	0.02%	0.002%
97	13.430	3758	3760	3762	rBV	300	142	0.02%	0.002%
98	13.745	3855	3858	3860	rBV2	312	195	0.02%	0.003%
99	13.999	3933	3937	3938	rBV	297	223	0.02%	0.003%
100	14.220	4004	4006	4009	rBV	385	271	0.03%	0.004%




Sum of corrected areas: 7078370

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054039.D
Acq On : 01 May 2023 20:26
Operator : JC/MD
Sample : 02565-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

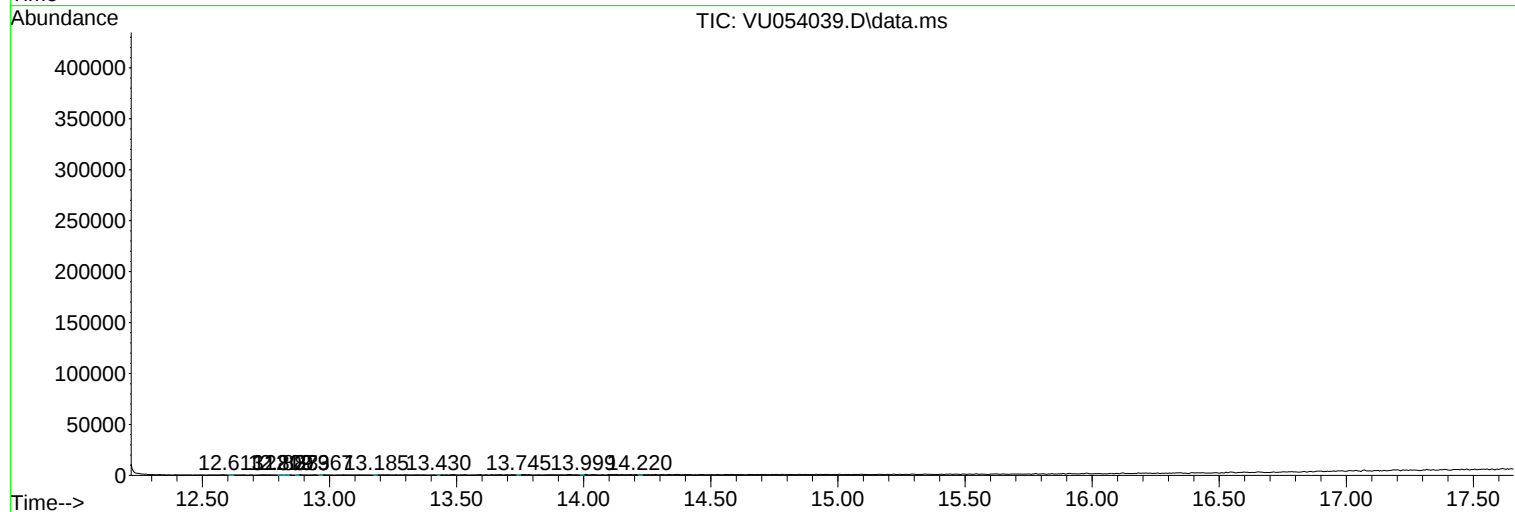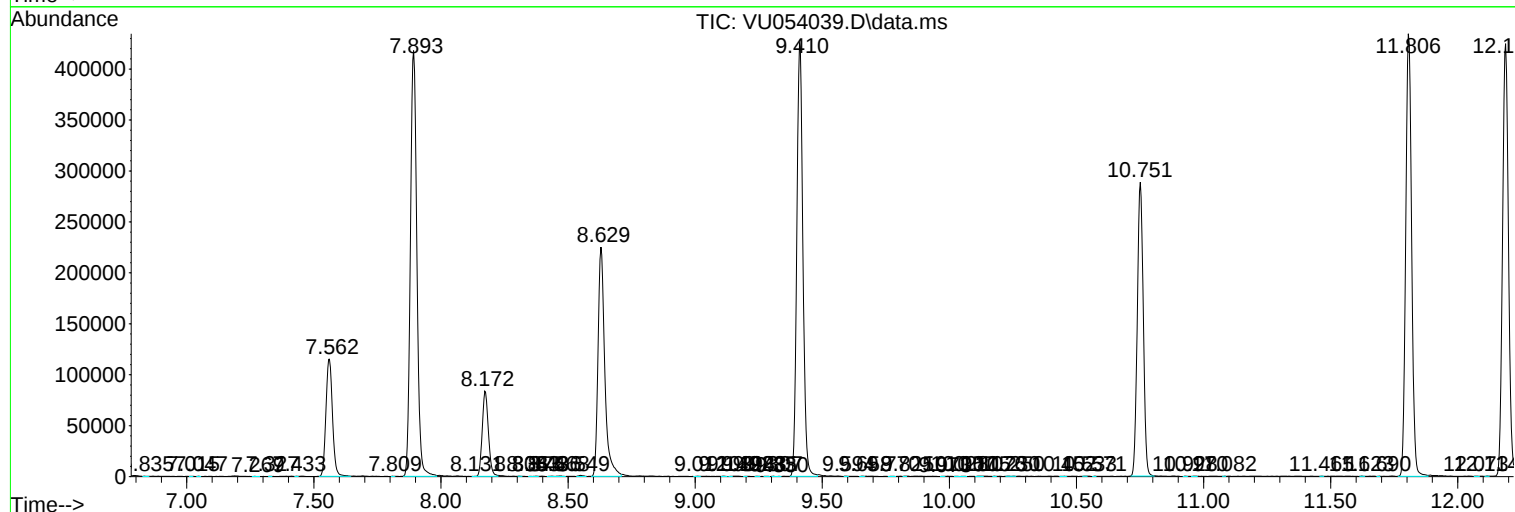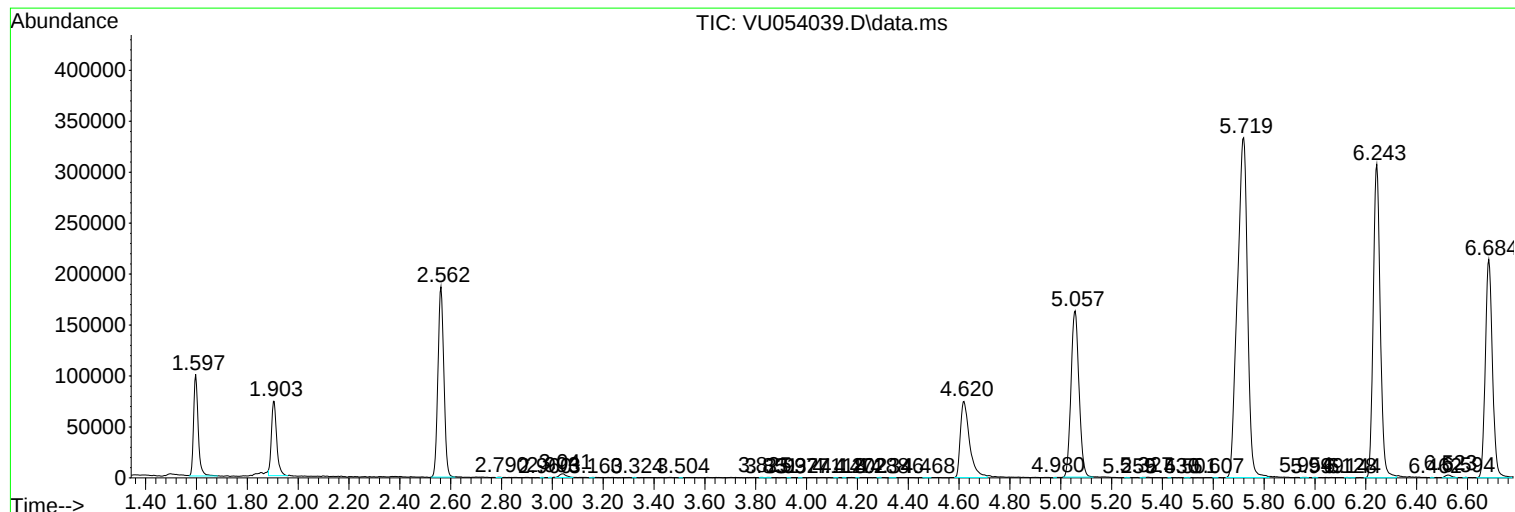

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054039.D
Acq On : 01 May 2023 20:26
Operator : JC/MD
Sample : 02565-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054039.D
Acq On : 01 May 2023 20:26
Operator : JC/MD
Sample : 02565-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------