
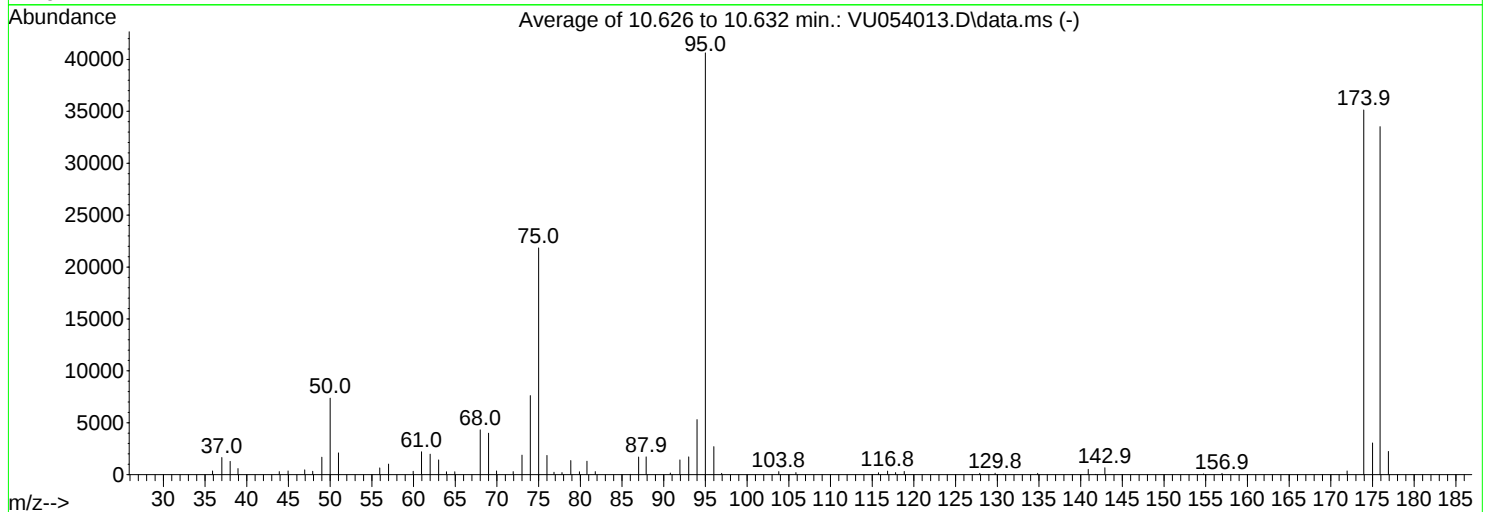


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050123\
Data File : VU054013.D
Acq On : 01 May 2023 09:16
Operator : JC/MD
Sample : BFB183
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB183

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis
Last Update : Tue May 02 05:29:54 2023

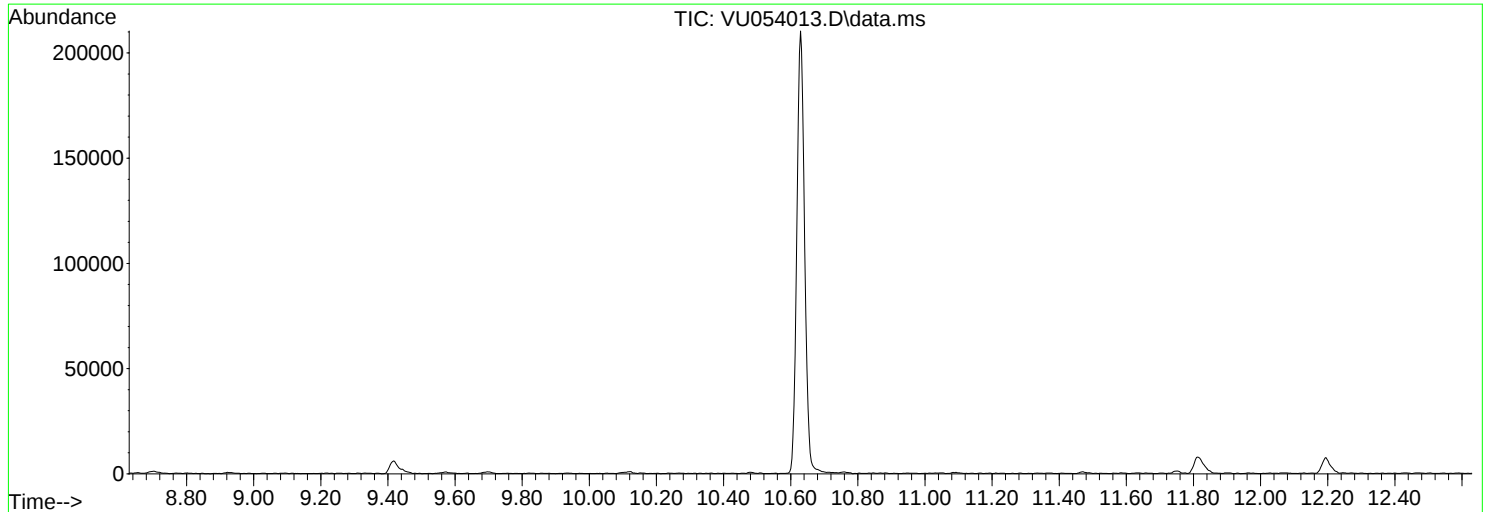

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	7374	PASS
75	95	30	80	53.8	21845	PASS
95	95	100	100	100.0	40635	PASS
96	95	5	9	6.6	2701	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.5	35133	PASS
175	174	5	9	8.7	3057	PASS
176	174	95	101	95.4	33528	PASS
177	176	5	9	6.7	2239	PASS

m/z	Abundance
39.90	136.0
43.90	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	336.0
37.00	1603.0
38.00	1264.0
39.00	551.0
39.90	119.0
43.90	463.0
44.90	379.0
47.00	389.0
47.90	281.0
49.00	1599.0
50.00	7336.0
51.00	2088.0
56.00	696.0
57.00	1021.0
60.00	318.0
60.90	2214.0
62.00	1899.0
63.00	1405.0
63.90	269.0
64.90	244.0
68.00	4385.0
69.00	3982.0
70.00	346.0
72.00	257.0
73.00	1729.0
74.00	7477.0
75.00	21872.0
76.00	1900.0
76.90	250.0
77.80	174.0
78.80	1463.0
79.90	267.0
80.80	1231.0
81.80	293.0
87.00	1730.0
87.90	1665.0
90.80	181.0
91.90	1436.0
93.00	1824.0
94.00	5324.0
95.00	40240.0
96.00	2660.0
96.90	126.0
103.80	292.0
105.80	233.0
115.80	166.0
116.90	338.0
117.80	162.0
118.90	337.0
128.90	106.0
129.80	144.0
130.80	116.0
134.80	110.0
140.90	494.0
142.90	697.0
154.80	109.0
156.90	124.0
171.90	321.0
174.00	33880.0
175.00	2940.0
175.90	31688.0
176.90	2121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	355.0
37.00	1694.0
38.00	1308.0
39.00	589.0
39.90	137.0
43.90	474.0
45.00	385.0
47.00	473.0
47.90	347.0
49.00	1743.0
50.00	7592.0
51.00	2182.0
56.00	661.0
57.00	1058.0
59.90	312.0
61.00	2278.0
62.00	2041.0
63.00	1454.0
64.00	297.0
64.90	298.0
68.00	4447.0
69.00	4104.0
70.00	356.0
71.90	289.0
73.00	1963.0
74.00	7885.0
75.00	22712.0
76.00	1889.0
76.80	230.0
77.80	229.0
78.90	1355.0
79.90	276.0
80.80	1355.0
81.80	314.0
87.00	1756.0
87.90	1769.0
90.80	151.0
91.90	1502.0
93.00	1775.0
94.00	5494.0
95.00	41824.0
96.00	2802.0
96.90	133.0
103.80	311.0
105.80	209.0
115.70	192.0
116.90	354.0
117.80	204.0
118.80	320.0
127.90	159.0
129.80	139.0
134.80	144.0
140.90	533.0
142.90	677.0
154.70	118.0
156.90	121.0
172.00	368.0
174.00	36192.0
175.00	3211.0
175.90	34552.0
176.90	2314.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	359.0
37.00	1638.0
38.00	1284.0
38.90	620.0
39.90	123.0
43.90	433.0
45.00	325.0
46.90	526.0
47.90	333.0
49.00	1689.0
50.00	7195.0
51.00	2017.0
55.90	583.0
57.00	960.0
59.90	327.0
61.00	2135.0
62.00	1965.0
63.00	1401.0
64.00	273.0
65.00	310.0
68.00	4113.0
69.00	3902.0
69.90	382.0
71.90	321.0
73.00	1929.0
74.00	7474.0
75.00	20952.0
76.00	1779.0
76.90	201.0
77.80	220.0
78.90	1257.0
79.90	299.0
80.80	1282.0
81.80	282.0
86.00	102.0
87.00	1598.0
87.90	1722.0
90.80	114.0
92.00	1303.0
93.00	1533.0
94.00	5103.0
95.00	39840.0
96.00	2642.0
97.00	129.0
103.80	281.0
105.90	183.0
115.70	210.0
116.80	332.0
117.80	240.0
118.90	284.0
127.90	218.0
129.70	131.0
134.90	126.0
140.90	481.0
141.80	115.0
142.90	612.0
157.00	115.0
172.00	371.0
173.90	35328.0
175.00	3021.0
175.90	34344.0
176.90	2282.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183