

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
 Data File : VU023576.D
 Acq On : 02 May 2018 13:54
 Operator : MD/SY
 Sample : J2660-13
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 03 06:45:25 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 03 05:16:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	210849	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	203401	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	98089	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	87430	58.50	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	117.00%
7) Chloroethane-d5	1.68	69	71416	62.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	125.40%
11) 1,1-Dichloroethene-d2	2.27	63	135052	46.35	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.70%
21) 2-Butanone-d5	4.18	46	174166	168.69	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	168.69%#
24) Chloroform-d	4.65	84	171133	69.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	138.50%#
26) 1,2-Dichloroethane-d4	5.31	65	115408	67.14	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	134.28%#
32) Benzene-d6	5.35	84	353378	64.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	129.50%#
36) 1,2-Dichloropropane-d6	6.34	67	123787	67.72	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	135.44%#
41) Toluene-d8	7.57	98	315397	62.69	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	125.38%#
43) trans-1,3-Dichloropropene-	7.85	79	50528	64.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	128.42%#
47) 2-Hexanone-d5	8.31	63	117640	169.47	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	169.47%#
57) 1,1,2,2-Tetrachloroethane-	10.44	84	166770	70.53	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	141.06%#
64) 1,2-Dichlorobenzene-d4	11.87	152	130353	68.12	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	136.24%#


Target Compounds					Ovalue
13) Acetone	2.32	43	10283	6.70 ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
Data File : VU023576.D
Acq On : 02 May 2018 13:54
Operator : MD/SY
Sample : J2660-13
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: May 03 06:45:25 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 03 05:16:38 2018
Response via : Initial Calibration

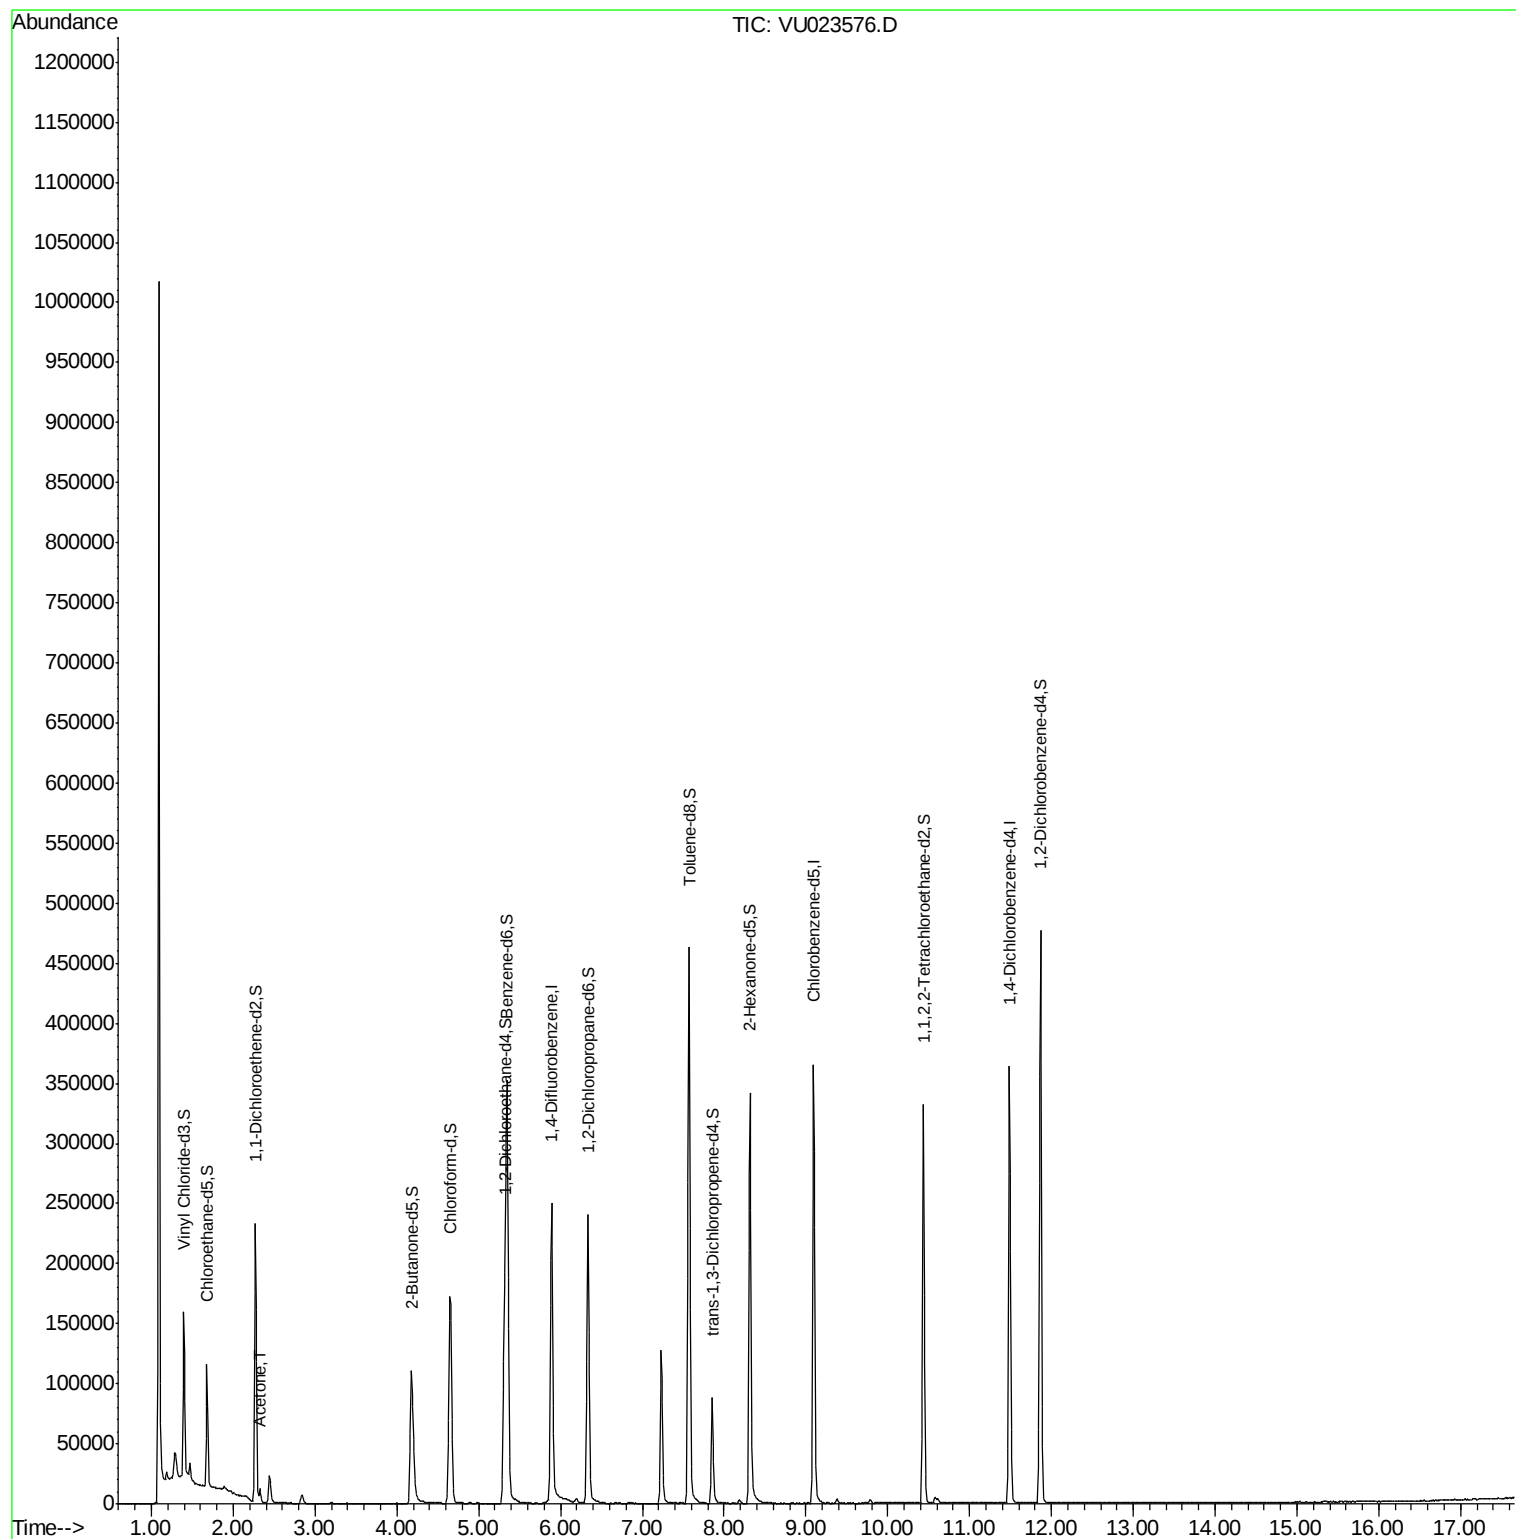

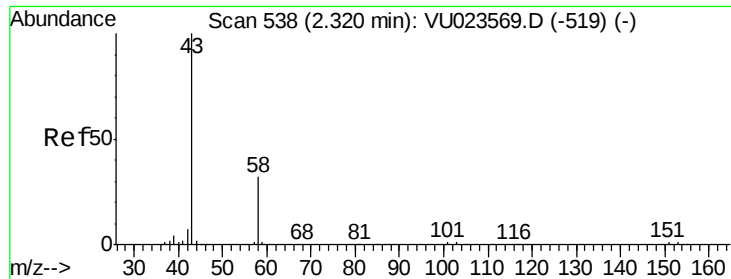

#13

Acetone

Concen: 6.70 ug/L

RT: 2.32 min Scan# 539

Delta R.T. 0.00 min

Lab File: VU023576.D

Acq: 02 May 2018 13:54

Tot Ion: 43 Resp: 10283

Ion Ratio Lower Upper

43 100

58 32.7 0.0 64.8

