

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
 Data File : VU023579.D
 Acq On : 02 May 2018 15:14
 Operator : MD/SY
 Sample : J2661-20
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Quant Time: May 03 06:49:01 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 03 05:16:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	329161	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	321425	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	151609	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	94639	40.57	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	81.14%
7) Chloroethane-d5	1.68	69	76409	42.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.94%
11) 1,1-Dichloroethene-d2	2.27	63	141961	31.21	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	62.42%
21) 2-Butanone-d5	4.18	46	195205	121.11	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	121.11%
24) Chloroform-d	4.65	84	189283	49.06	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.12%
26) 1,2-Dichloroethane-d4	5.31	65	128106	47.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.48%
32) Benzene-d6	5.35	84	385832	44.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.48%
36) 1,2-Dichloropropane-d6	6.34	67	136270	47.18	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.36%
41) Toluene-d8	7.57	98	346495	43.58	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.16%
43) trans-1,3-Dichloropropene-	7.85	79	57336	46.11	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.22%
47) 2-Hexanone-d5	8.31	63	134962	123.03	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	123.03%
57) 1,1,2,2-Tetrachloroethane-	10.44	84	187581	50.20	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.40%
64) 1,2-Dichlorobenzene-d4	11.86	152	144088	48.72	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.44%


Target Compounds					Ovalue
13) Acetone	2.32	43	12614	5.27 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
Data File : VU023579.D
Acq On : 02 May 2018 15:14
Operator : MD/SY
Sample : J2661-20
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Quant Time: May 03 06:49:01 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 03 05:16:38 2018
Response via : Initial Calibration

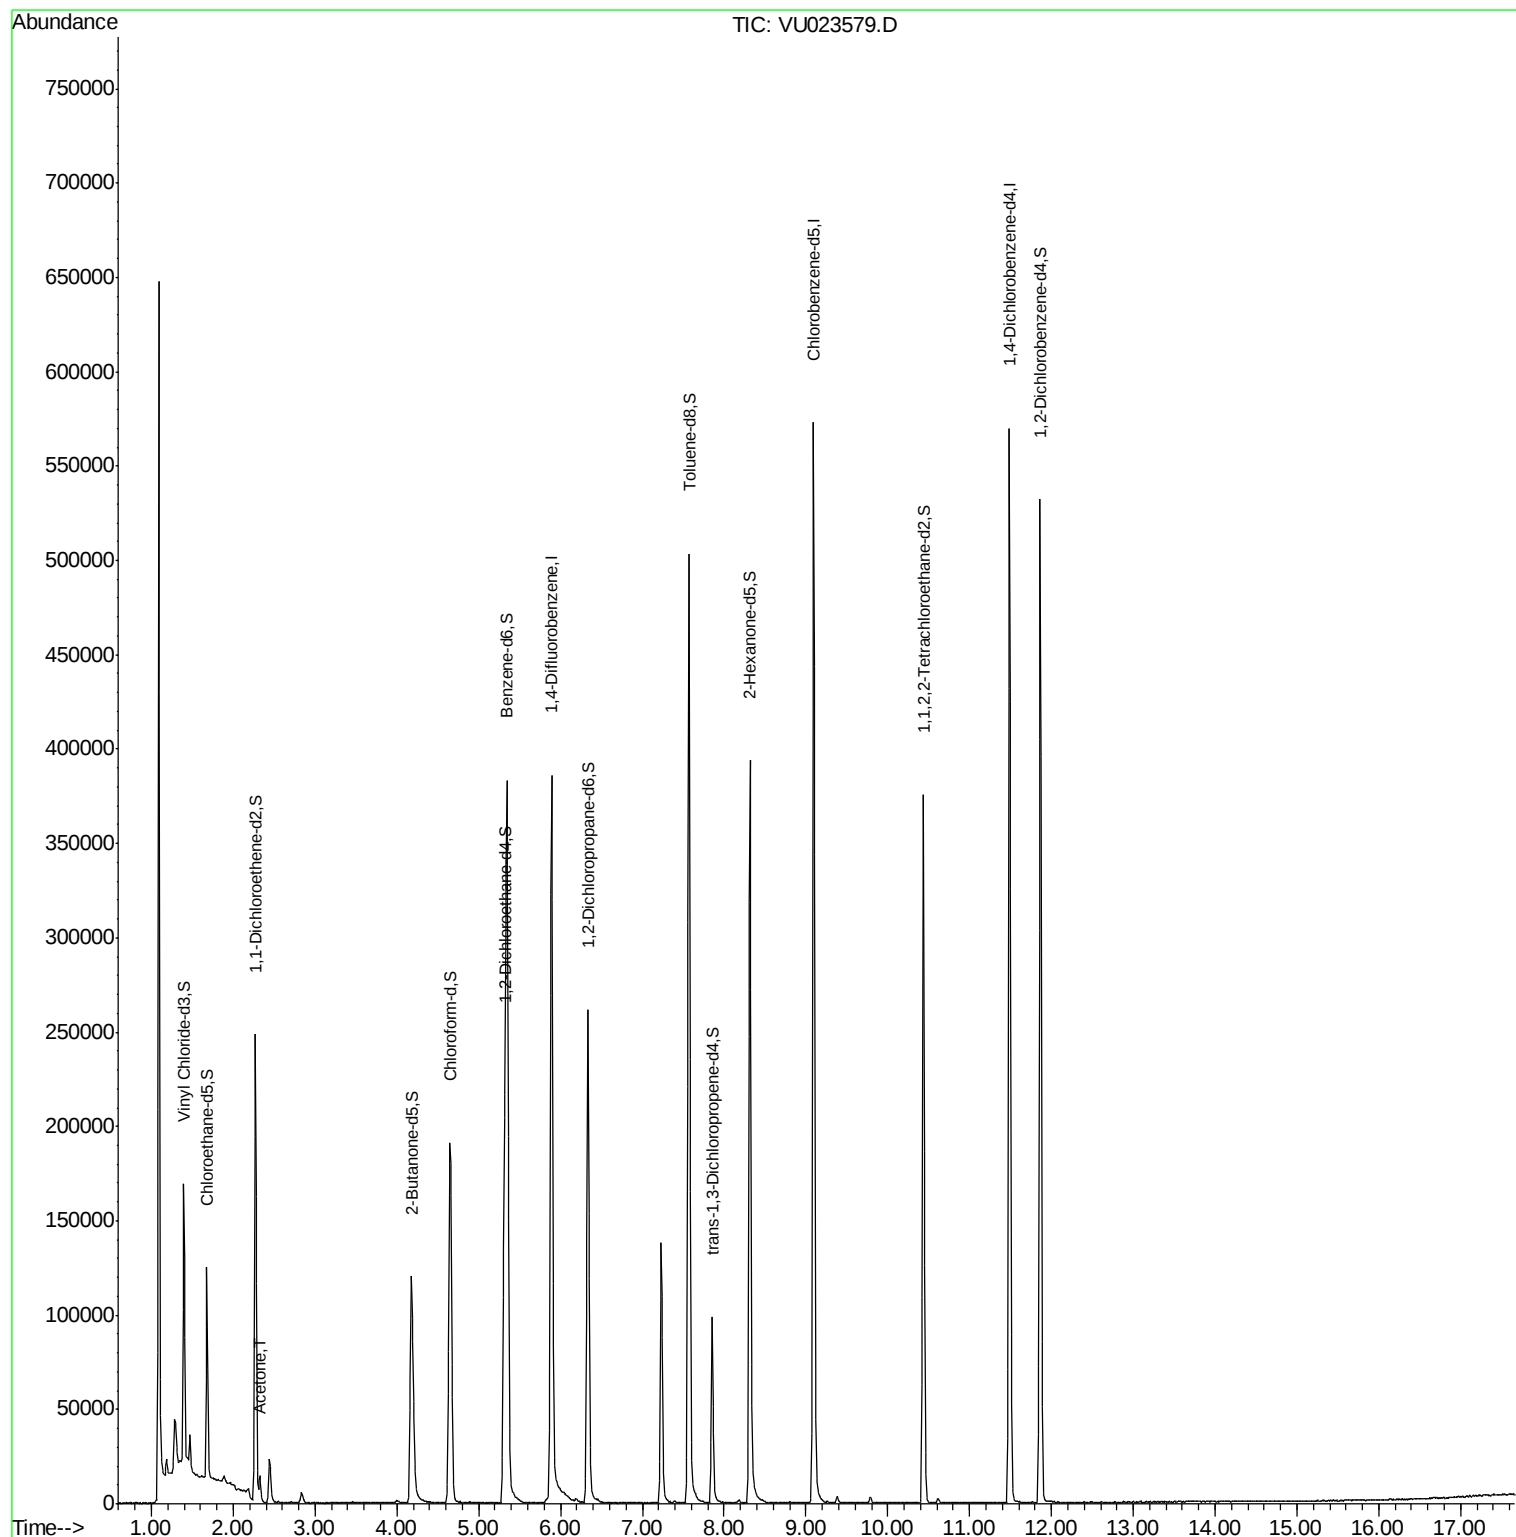

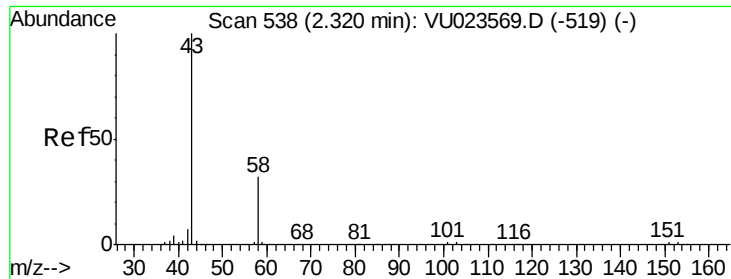

#13

Acetone

Concen: 5.27 ug/L

RT: 2.32 min Scan# 539

Delta R.T. 0.00 min

Lab File: VU023579.D

Acq: 02 May 2018 15:14

Tot Ion: 43 Resp: 12614

Ion Ratio Lower Upper

43 100

58 31.8 0.0 64.8

