

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
 Data File : VU023582.D
 Acq On : 02 May 2018 16:33
 Operator : MD/SY
 Sample : J2621-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: May 03 06:53:41 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu May 03 05:16:38 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	337641	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	306157	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	147714	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	94028	39.29	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	78.58%
7) Chloroethane-d5	1.68	69	77871	42.69	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.38%
11) 1,1-Dichloroethene-d2	2.27	63	133963	28.71	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	57.42%#
21) 2-Butanone-d5	4.18	46	215317	130.23	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	130.23%#
24) Chloroform-d	4.65	84	191979	48.51	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.02%
26) 1,2-Dichloroethane-d4	5.31	65	134501	48.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.74%
32) Benzene-d6	5.35	84	390390	47.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.06%
36) 1,2-Dichloropropane-d6	6.34	67	140310	51.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.00%
41) Toluene-d8	7.57	98	329417	43.50	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.00%
43) trans-1,3-Dichloropropene-	7.85	79	55097	46.52	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.04%
47) 2-Hexanone-d5	8.31	63	155421	148.75	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	148.75%#
57) 1,1,2,2-Tetrachloroethane-	10.44	84	198379	55.74	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	111.48%
64) 1,2-Dichlorobenzene-d4	11.87	152	136761	47.46	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.92%


Target Compounds


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.32	43	26050	10.60	ug/L	100
15) Methyl Acetate	2.62	43	21939	6.74	ug/L	97
16) Methylene chloride	2.70	84	181521	59.02	ug/L	99
20) cis-1,2-Dichloroethene	4.23	96	8106	2.71	ug/L	97
22) 2-Butanone	4.27	43	34441	12.61	ug/L	99
30) 1,1,1-Trichloroethane	4.92	97	808865	208.59	ug/L	100
34) Trichloroethene	6.19	95	3126848	1131.17	ug/L	98
40) 4-Methyl-2-pentanone	7.46	43	19927	5.28	ug/L	94
42) Toluene	7.64	91	188163	16.83	ug/L	99
45) 1,1,2-Trichloroethane	8.07	97	28565	10.87	ug/L	99
52) Ethylbenzene	9.26	91	521630	43.03	ug/L	100
53) m,p-Xylene	9.38	106	855904	185.13	ug/L	99
54) o-xylene	9.78	106	441665	100.83	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
Data File : VU023582.D
Acq On : 02 May 2018 16:33
Operator : MD/SY
Sample : J2621-08
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Quant Time: May 03 06:53:41 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Quant Title : VOC Analysis
QLast Update : Thu May 03 05:16:38 2018
Response via : Initial Calibration

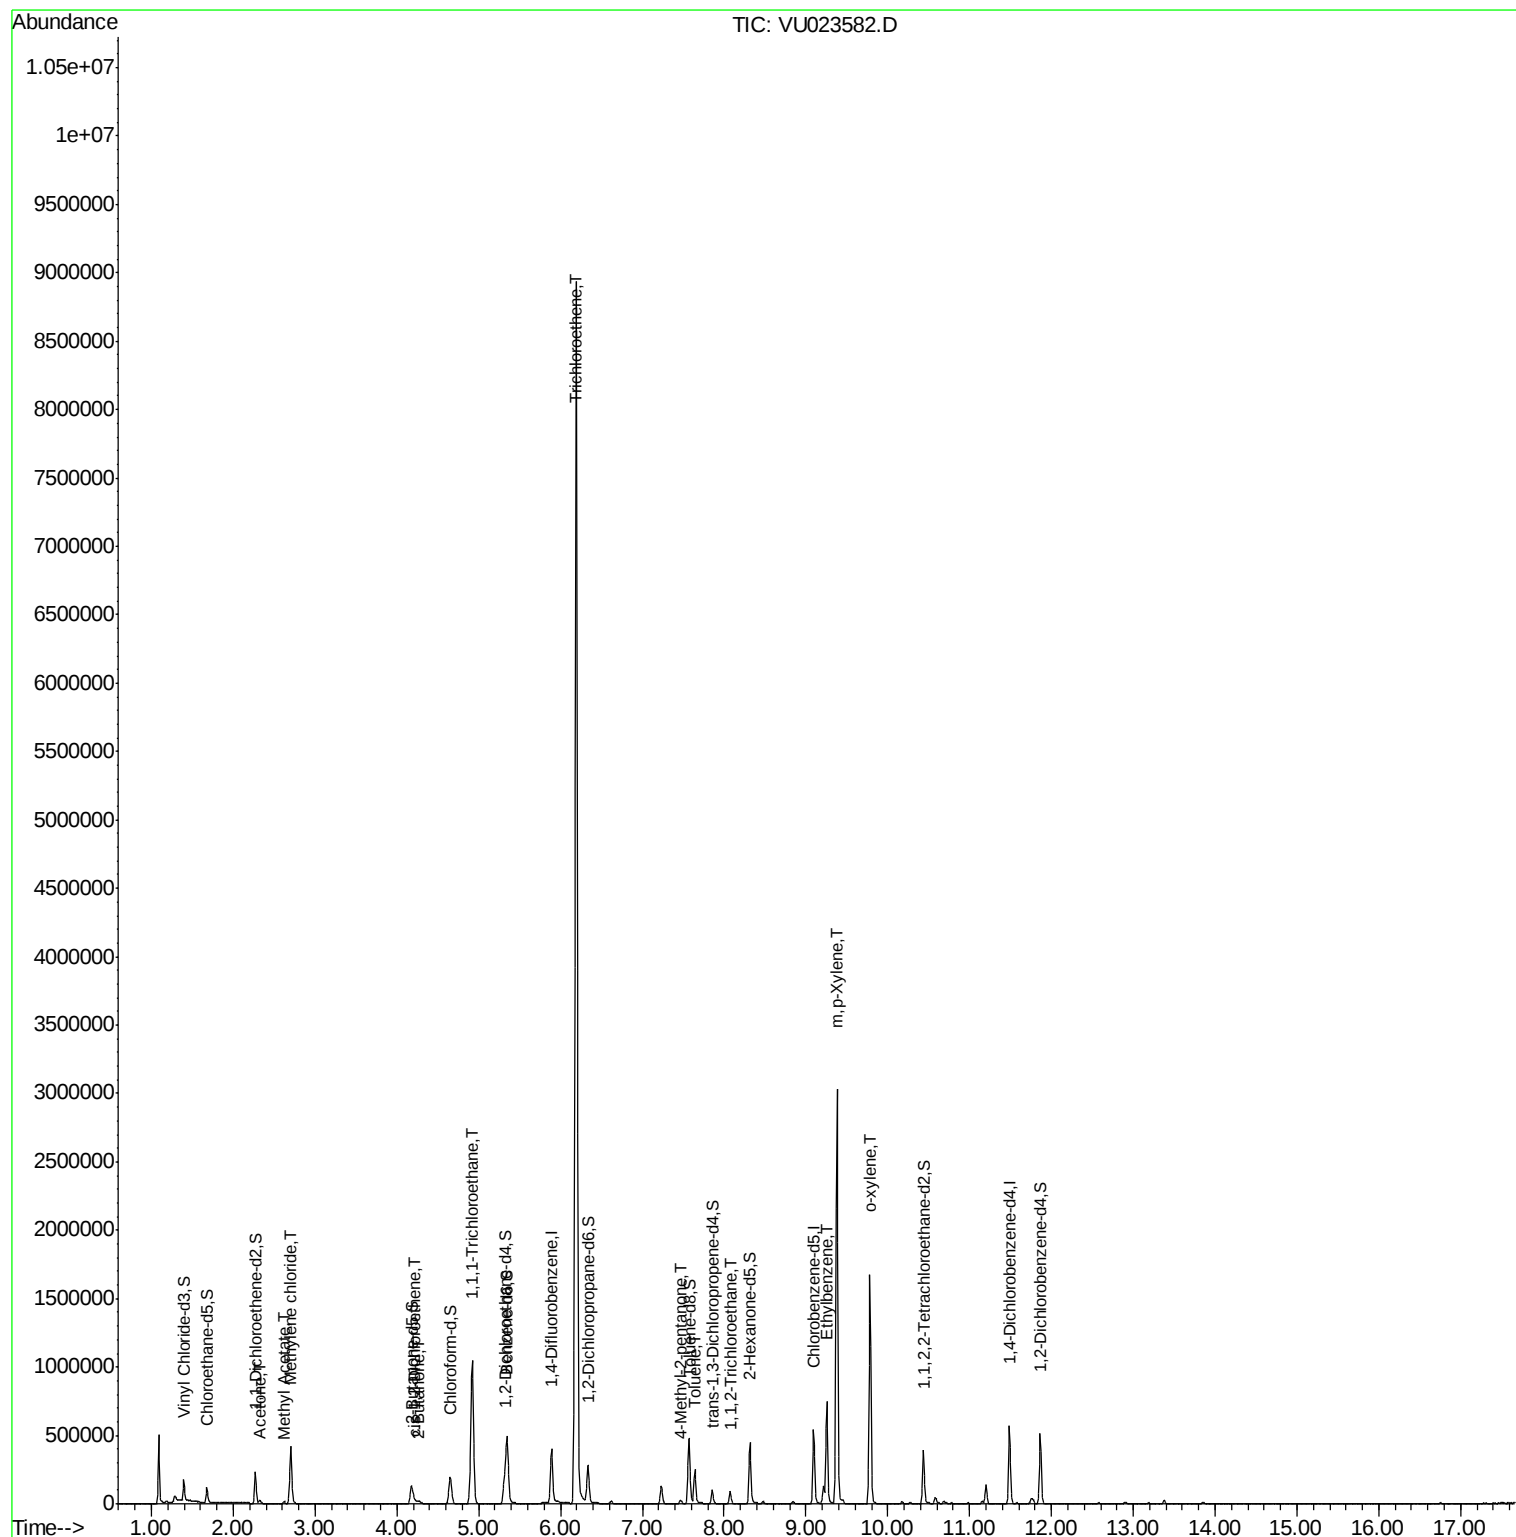

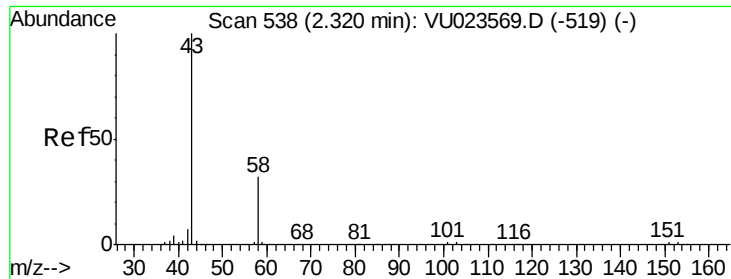

#13

Acetone

Concen: 10.60 ug/L

RT: 2.32 min Scan# 539

Delta R.T. 0.00 min

Lab File: VU023582.D


Acq: 02 May 2018 16:33

Tot Ion: 43 Resp: 26050

Ion Ratio Lower Upper




43 100

58 32.1 0.0 64.8

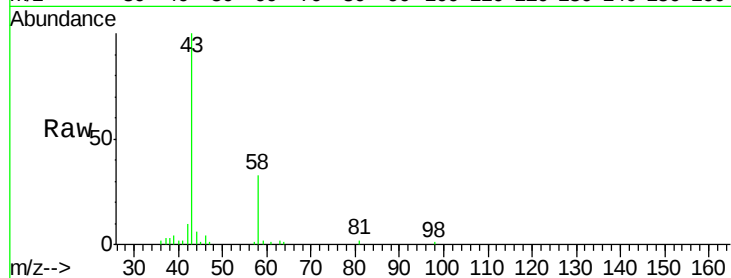

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 58.00 (57.70 to 58.70): VU0

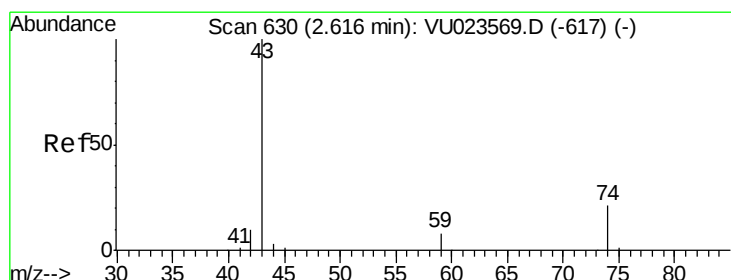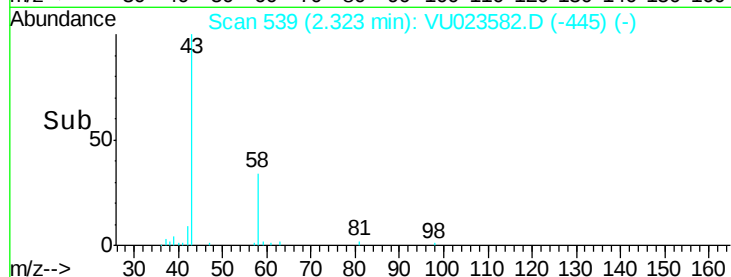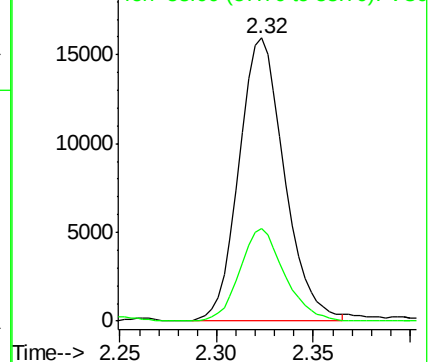

#15

Methyl Acetate

Concen: 6.74 ug/L

RT: 2.62 min Scan# 631

Delta R.T. 0.00 min

Lab File: VU023582.D


Acq: 02 May 2018 16:33

Tgt Ion: 43 Resp: 21939

Ion Ratio Lower Upper



43 100


74 20.5 17.5 26.3

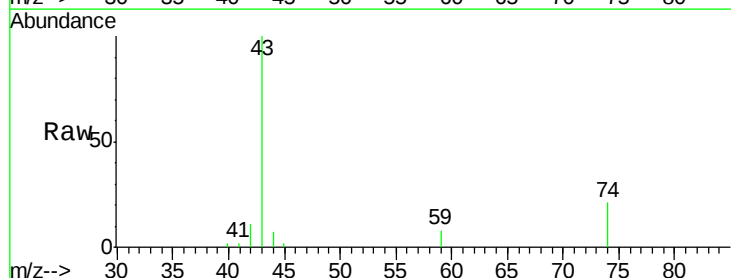

Abundance Ion 43.00 (42.70 to 43.70): VU0


Ion 74.00 (73.70 to 74.70): VU0

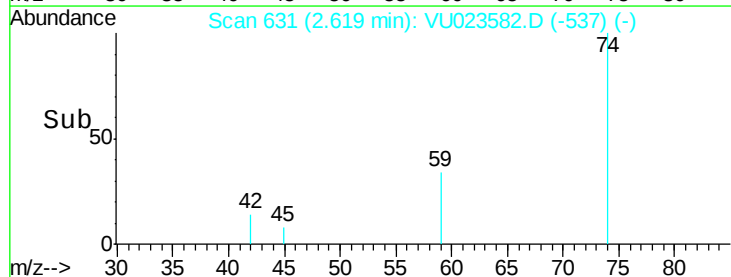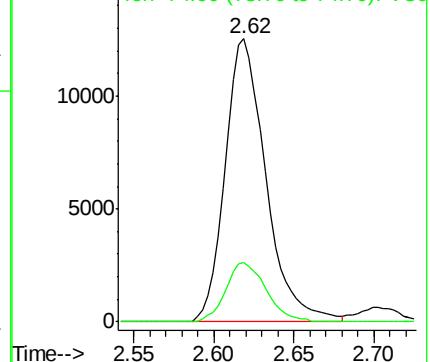



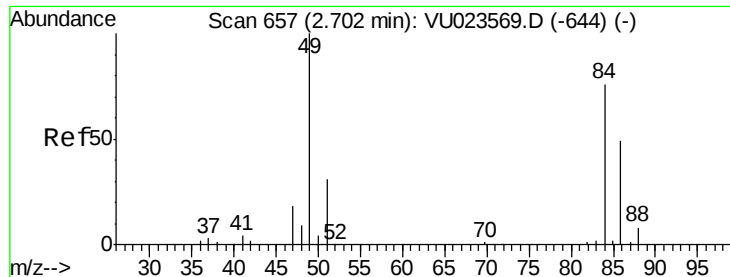


#16
Methvlene chloride
Concen: 59.02 ug/L
RT: 2.70 min Scan# 657
Delta R.T. 0.00 min
Lab File: VU023582.D
Acq: 02 May 2018 16:33

Tot Ion: 84 Resp: 181521
Ion Ratio Lower Upper
84 100
86 65.8 45.6 84.8
49 133.0 91.9 170.7

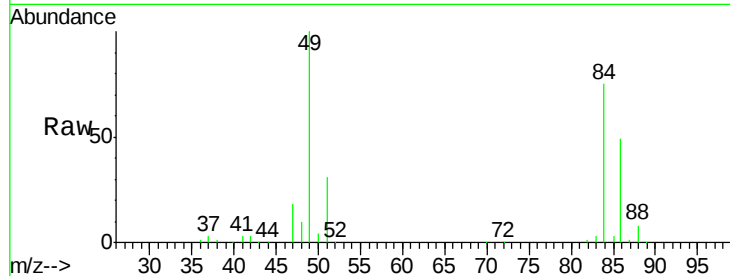


Abundance Ion 84.00 (83.70 to 84.70): VU0
Ion 86.00 (85.70 to 86.70): VU0
Ion 49.00 (48.70 to 49.70): VU0

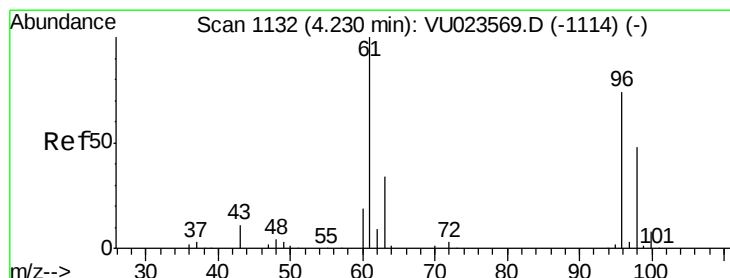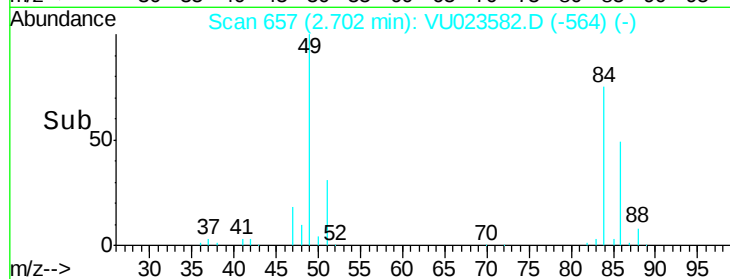
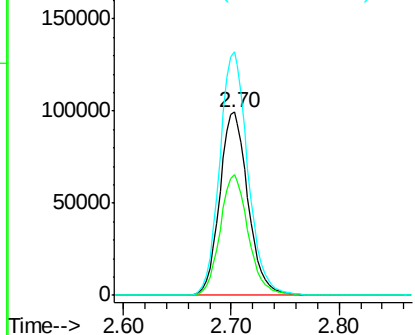



#20
cis-1,2-Dichloroethene
Concen: 2.71 ug/L
RT: 4.23 min Scan# 1132
Delta R.T. 0.00 min
Lab File: VU023582.D
Acq: 02 May 2018 16:33

Tgt Ion: 96 Resp: 8106
Ion Ratio Lower Upper
96 100
61 133.0 95.3 177.1
68 0.0 0.0 0.0

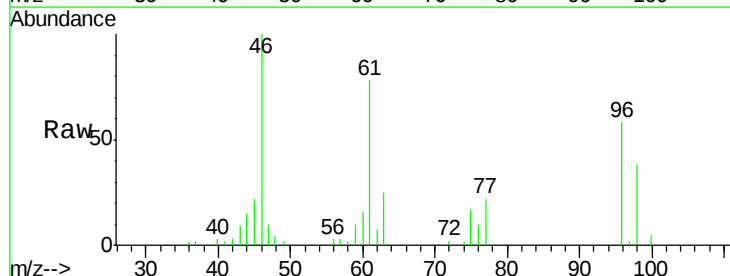

Abundance Ion 96.00 (95.70 to 96.70): VU0
Ion 61.00 (60.70 to 61.70): VU0
Ion 68.00 (67.70 to 68.70): VU0

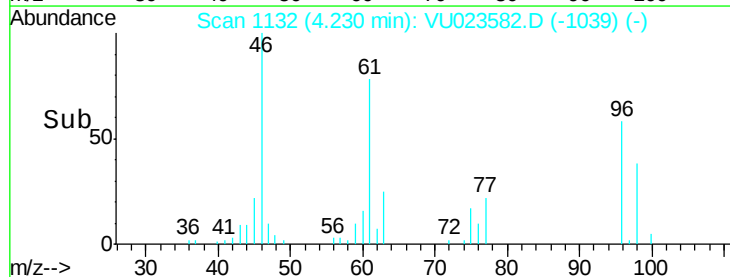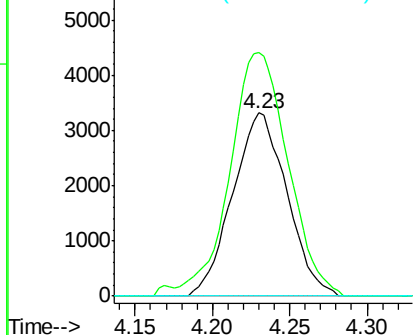

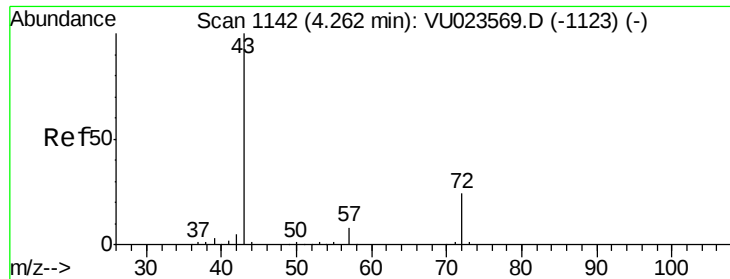

#22

2-Butanone

Concen: 12.61 ug/L

RT: 4.27 min Scan# 1145

Delta R.T. 0.01 min

Lab File: VU023582.D


Acq: 02 May 2018 16:33

Tot Ion: 43 Resp: 34441

Ion Ratio Lower Upper




43 100

72 23.8 12.3 36.8

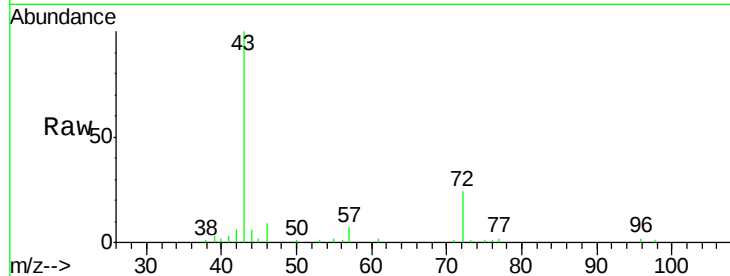

Abundance Ion 43.00 (42.70 to 43.70): VU0

Ion 72.00 (71.70 to 72.70): VU0

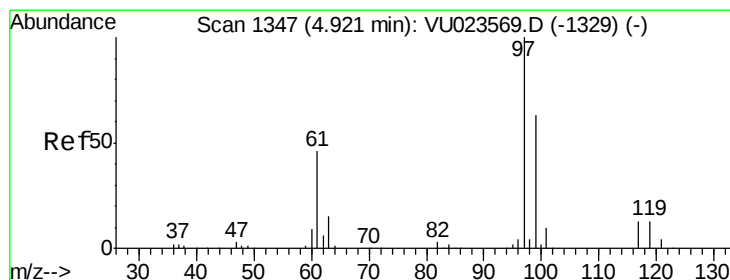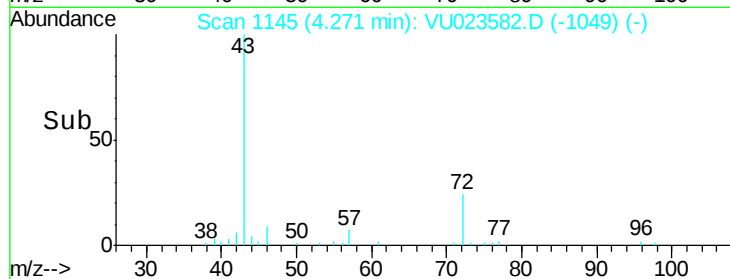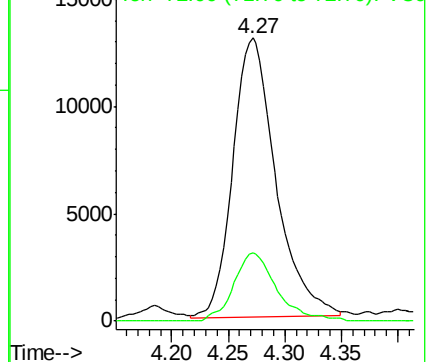

#30

1,1,1-Trichloroethane

Concen: 208.59 ug/L

RT: 4.92 min Scan# 1347

Delta R.T. -0.00 min

Lab File: VU023582.D

Acq: 02 May 2018 16:33


Tgt Ion: 97 Resp: 808865

Ion Ratio Lower Upper

97 100

99 64.3 51.8 77.6



61 47.2 37.7 56.5

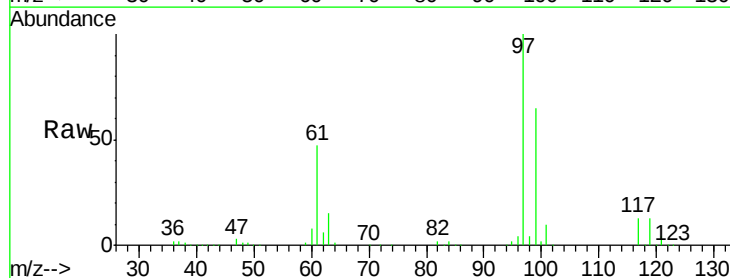


Abundance Ion 97.00 (96.70 to 97.70): VU0

Ion 99.00 (98.70 to 99.70): VU0

Ion 61.05 (60.75 to 61.75): VU0

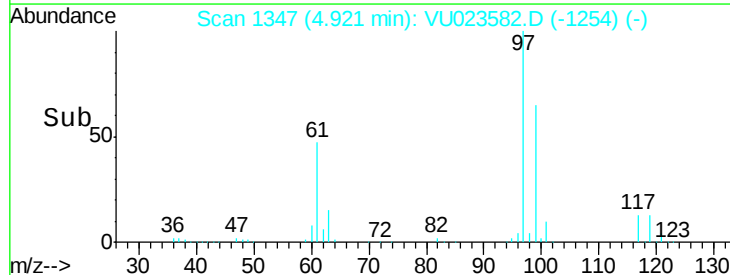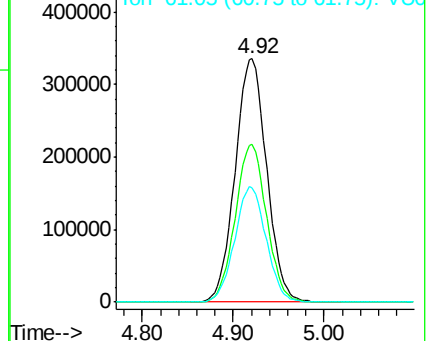


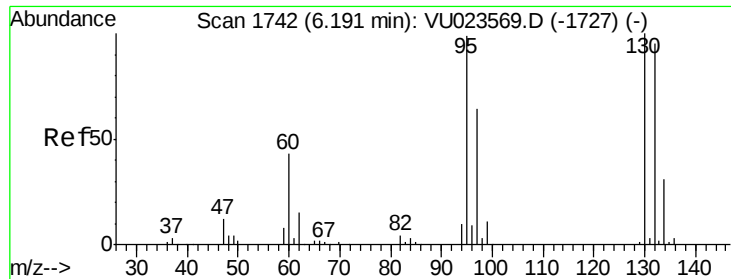




#34
 Trichloroethene
 Concen: 1131.17 ug/L
 RT: 6.19 min Scan# 1742
 Delta R.T. 0.00 min
 Lab File: VU023582.D
 Acq: 02 May 2018 16:33

Tot Ion: 95 Resp: 3126848

Ion	Ratio	Lower	Upper
95	100		
97	64.7	46.3	85.9
132	95.2	68.5	127.1
130	98.9	70.8	131.4

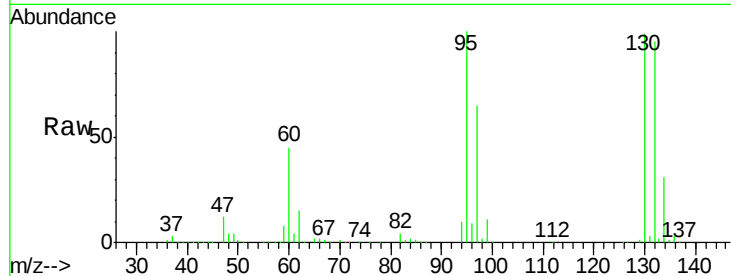


Abundance Ion 95.00 (94.70 to 95.70): VU0
 Ion 97.00 (96.70 to 97.70): VU0
 Ion 132.00 (131.70 to 132.70): V
 Ion 130.00 (129.70 to 130.70): V

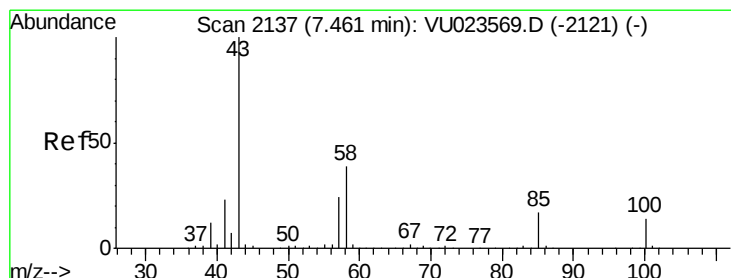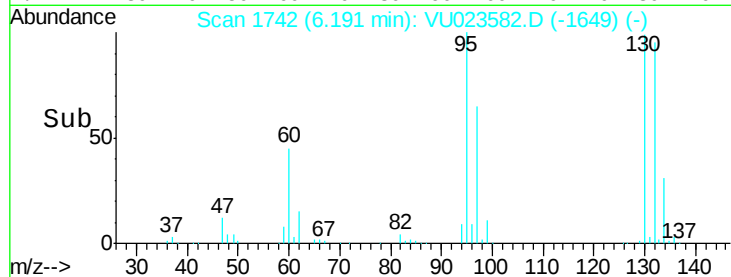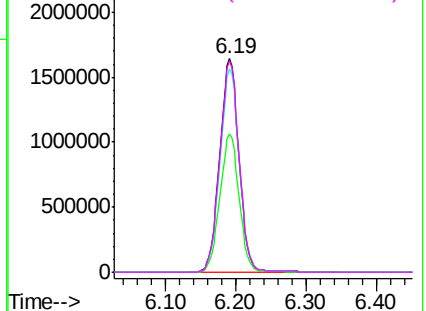



#40
 4-Methyl-2-pentanone
 Concen: 5.28 ug/L
 RT: 7.46 min Scan# 2138
 Delta R.T. 0.00 min
 Lab File: VU023582.D
 Acq: 02 May 2018 16:33


Tgt Ion: 43 Resp: 19927

Ion	Ratio	Lower	Upper
43	100		
58	34.1	30.8	46.2
100	13.0	10.7	16.1

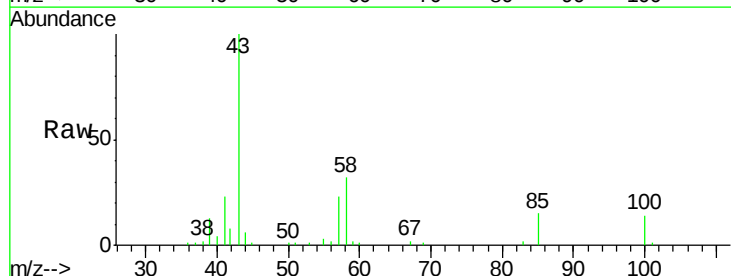

Abundance Ion 43.00 (42.70 to 43.70): VU0
 Ion 58.00 (57.70 to 58.70): VU0
 Ion 100.00 (99.70 to 100.70): VU

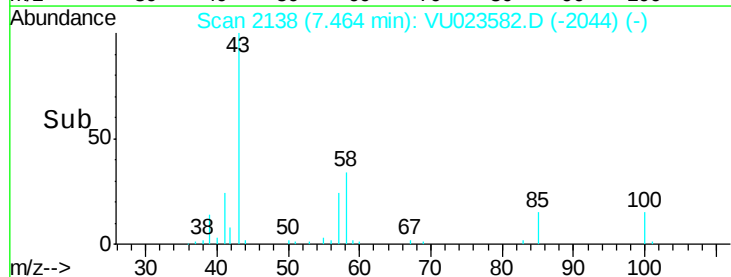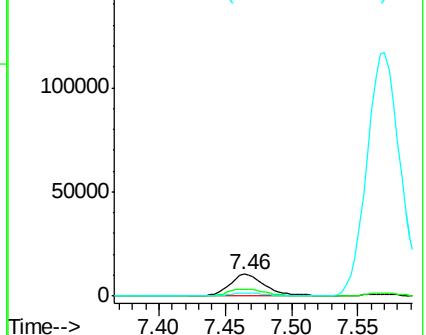

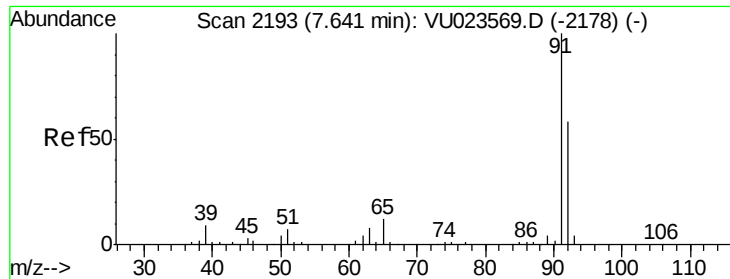

#42

Toluene

Concen: 16.83 ug/L

RT: 7.64 min Scan# 2193

Delta R.T. 0.00 min

Lab File: VU023582.D


Acq: 02 May 2018 16:33

Tot Ion: 91 Resp: 188163

Ion Ratio Lower Upper

91 100

92 57.0 40.3 74.9

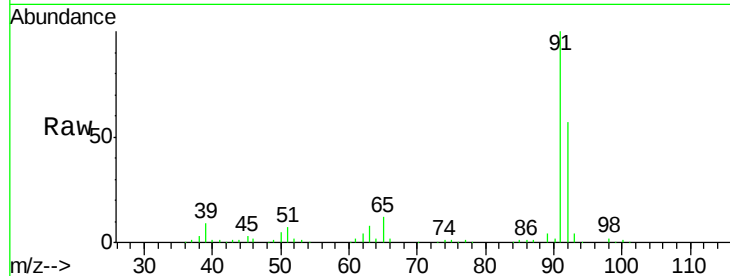

Abundance Ion 91.00 (90.70 to 91.70): VU023569.D (-2178) (-)

Ion 92.00 (91.70 to 92.70): VU023569.D (-2178) (-)

7.64

100000

80000



60000

40000

20000

0

Time-->

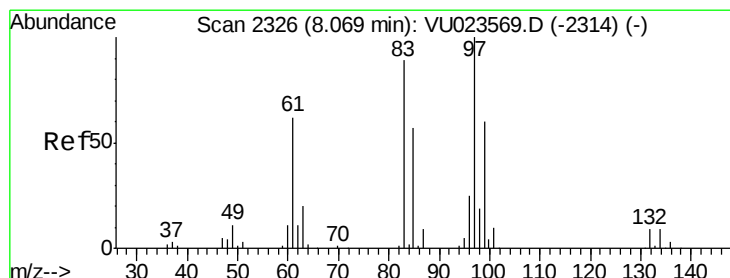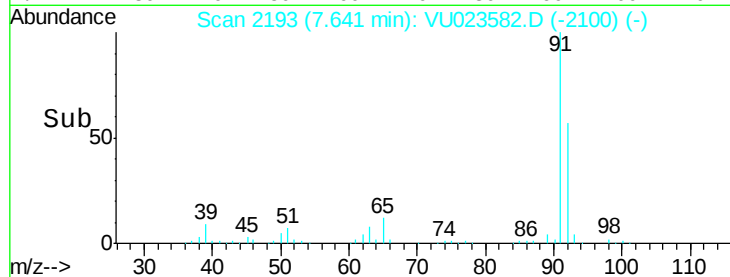

#45

1,1,2-Trichloroethane

Concen: 10.87 ug/L

RT: 8.07 min Scan# 2327

Delta R.T. 0.00 min

Lab File: VU023582.D

Acq: 02 May 2018 16:33

Tgt Ion: 97 Resp: 28565


Ion Ratio Lower Upper

97 100

99 63.1 44.2 82.2

83 88.9 63.1 117.1

85 59.6 40.3 74.8

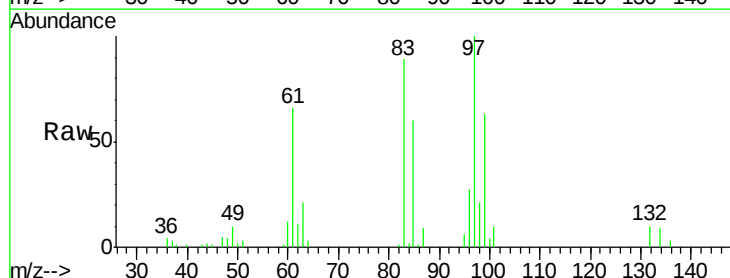

Abundance Ion 97.00 (96.70 to 97.70): VU023569.D (-2314) (-)

Ion 99.00 (98.70 to 99.70): VU023569.D (-2314) (-)

Ion 83.00 (82.70 to 83.70): VU023569.D (-2314) (-)

Ion 85.00 (84.70 to 85.70): VU023569.D (-2314) (-)

8.07

25000

20000


15000


10000

5000

0

Time-->

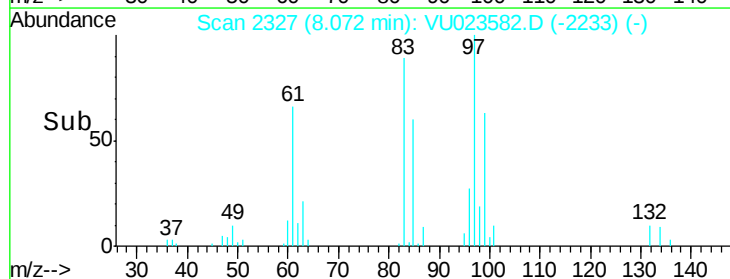

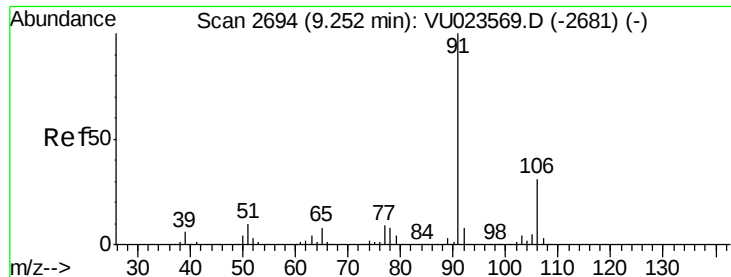

#52

Ethylbenzene

Concen: 43.03 ug/L

RT: 9.26 min Scan# 2695

Delta R.T. 0.00 min

Lab File: VU023582.D


Acq: 02 May 2018 16:33

Tot Ion: 91 Resp: 521630

Ion Ratio Lower Upper

91 100

106 30.8 21.6 40.0

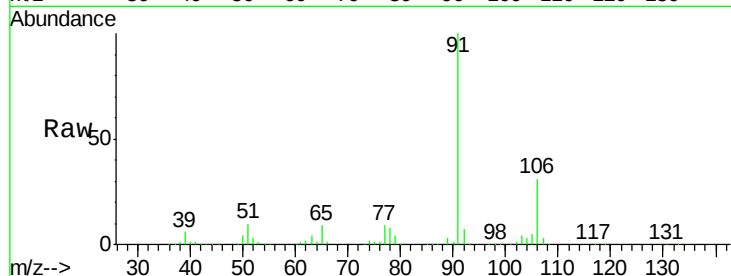

Abundance Ion 91.00 (90.70 to 91.70): VU023569.D (-2681) (-)

Ion 106.00 (105.70 to 106.70): VU023569.D (-2681) (-)

1200000

1000000

800000

600000



400000

200000

0

9.15 9.20 9.25 9.30 9.35

Time-->

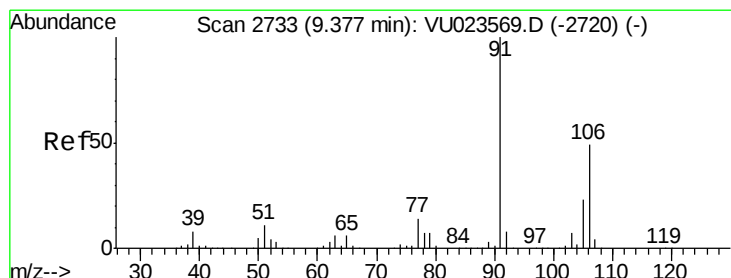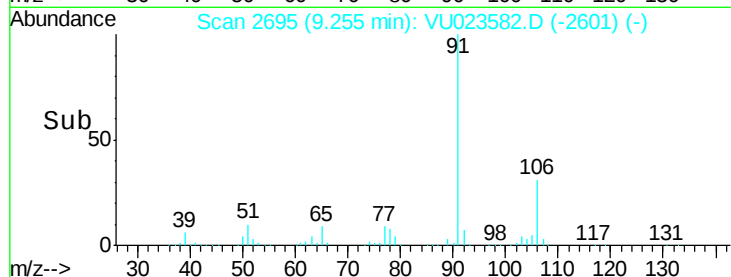

#53

m,p-Xylene

Concen: 185.13 ug/L

RT: 9.38 min Scan# 2733

Delta R.T. 0.00 min

Lab File: VU023582.D


Acq: 02 May 2018 16:33

Tgt Ion: 106 Resp: 855904

Ion Ratio Lower Upper

106 100

91 204.8 144.1 267.5

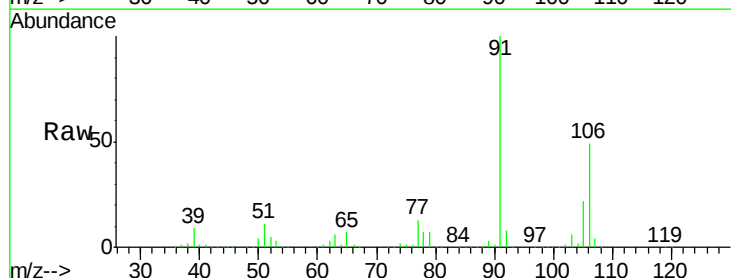

Abundance Ion 106.00 (105.70 to 106.70): VU023569.D (-2720) (-)

Ion 91.00 (90.70 to 91.70): VU023569.D (-2720) (-)

1200000

1000000

800000

600000


400000


200000

0

9.30 9.40 9.50

Time-->

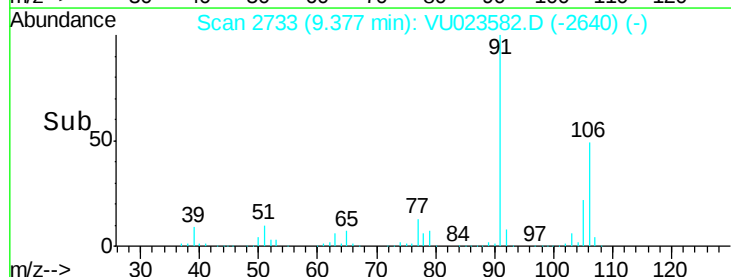

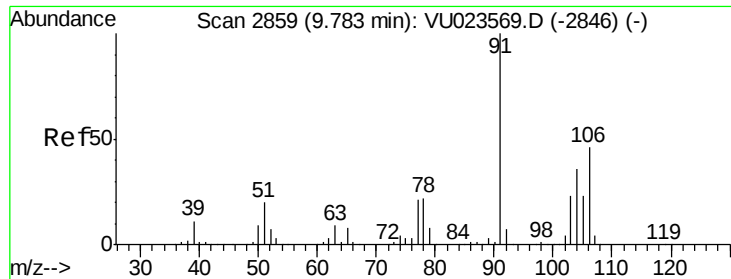

#54
 o-xylene
 Concen: 100.83 ug/L
 RT: 9.78 min Scan# 2859
 Delta R.T. 0.00 min
 Lab File: VU023582.D
 Acq: 02 May 2018 16:33

Tot Ion:106 Resp: 441665
 Ion Ratio Lower Upper
 106 100
 91 215.6 148.9 276.5

