


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050218\
 Data File : VU023568.D
 Acq On : 02 May 2018 09:59
 Operator : MD/SY
 Sample : BFB46
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Title : VOC Analysis
 Last Update : Thu May 03 05:16:38 2018

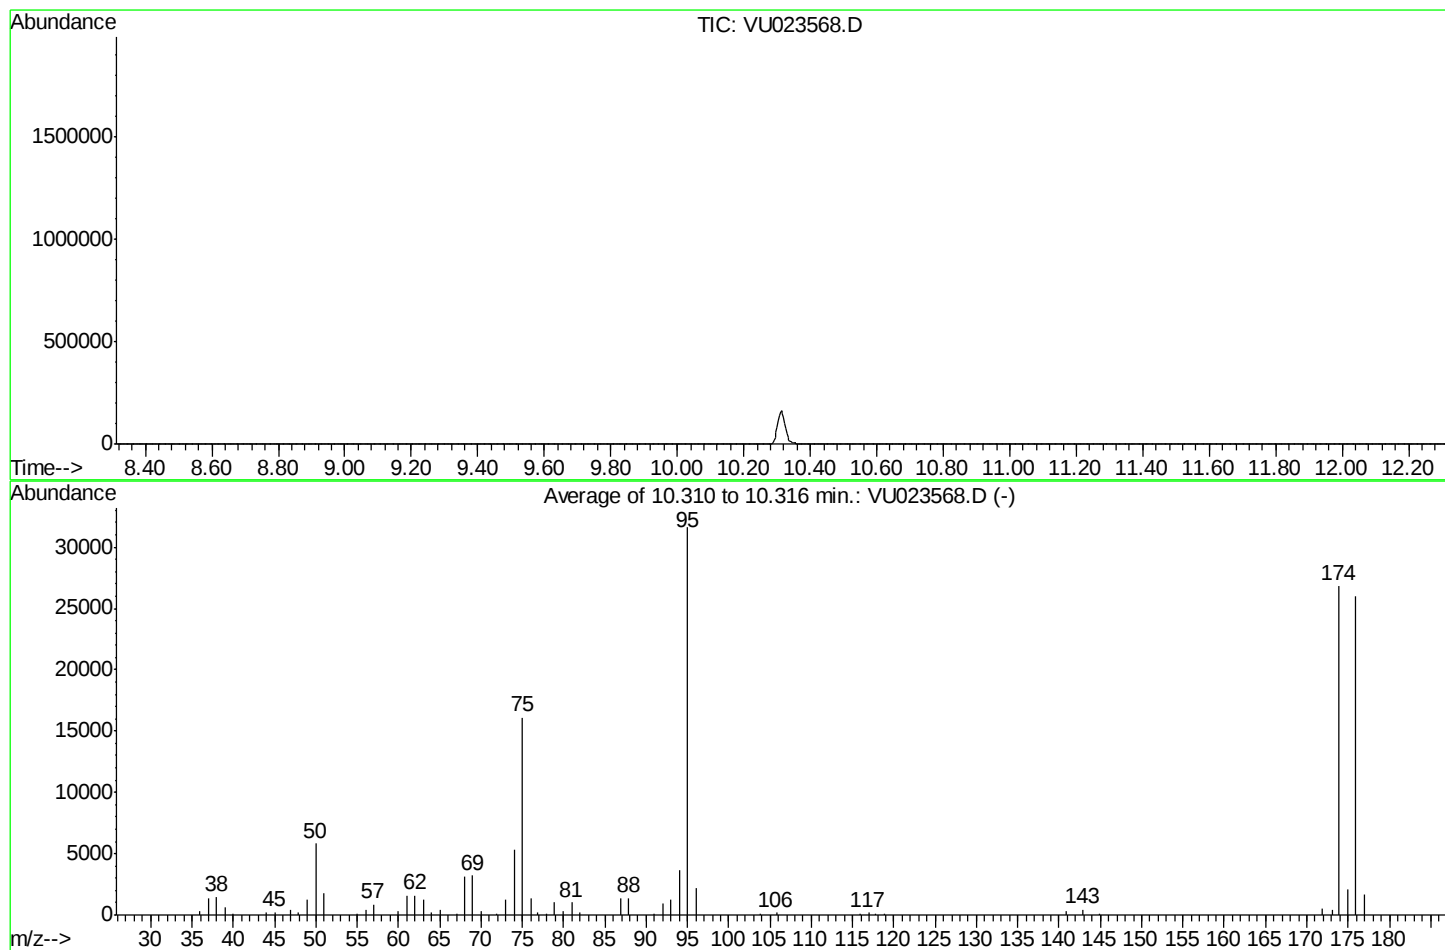

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3012

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5839	PASS
75	95	30	80	51.0	16121	PASS
95	95	100	100	100.0	31610	PASS
96	95	5	9	7.0	2223	PASS
173	174	0.00	2	1.4	380	PASS
174	95	50	120	84.9	26824	PASS
175	174	5	9	7.8	2080	PASS
176	174	95	101	96.9	25984	PASS
177	176	5	9	6.4	1656	PASS

Scan 3012 (10.275 min): VU023568.D
BFB46

m/z	Abundance
40.00	160.0
44.00	395.0

m/z	Abundance
35.90	288.0
37.00	1485.0
38.00	1457.0
39.00	691.0
40.00	219.0
44.10	665.0
45.00	237.0
47.00	504.0
47.80	207.0
49.00	1218.0
50.00	6149.0
51.00	1850.0
55.00	138.0
56.00	509.0
57.00	901.0
60.00	369.0
61.00	1542.0
62.00	1643.0
63.00	1326.0
64.00	241.0
65.10	379.0
67.00	113.0
68.00	3214.0
69.00	3204.0
69.90	290.0
71.80	140.0
73.00	1222.0
74.00	5497.0
75.00	16362.0
76.10	1481.0
76.90	272.0
78.00	134.0
78.90	1037.0
79.90	320.0
80.90	1009.0
81.90	233.0
86.90	1413.0
87.90	1291.0
92.00	1004.0
93.00	1312.0
94.00	3645.0
95.00	31784.0
96.00	2238.0
103.80	158.0
105.80	150.0
116.90	187.0
118.80	132.0
140.80	256.0
142.90	456.0
144.90	134.0
171.90	443.0
173.00	357.0
174.00	26520.0
175.00	2028.0
175.90	25664.0
176.90	1716.0

m/z	Abundance
35.90	309.0
37.00	1397.0
38.00	1552.0
39.00	628.0
40.00	232.0
44.10	636.0
45.00	259.0
47.00	427.0
47.80	195.0
49.00	1271.0
50.00	6021.0
51.00	1846.0
55.00	170.0
56.00	477.0
57.00	913.0
60.00	333.0
61.00	1604.0
62.00	1655.0
63.00	1255.0
64.00	268.0
65.00	440.0
67.00	116.0
68.00	3287.0
69.00	3348.0
70.00	284.0
71.80	128.0
73.00	1316.0
74.00	5508.0
75.00	16656.0
76.10	1452.0
76.90	266.0
77.90	145.0
78.90	1070.0
79.90	319.0
80.90	1070.0
81.90	261.0
87.00	1440.0
87.90	1432.0
91.00	123.0
92.00	981.0
93.00	1321.0
94.00	3843.0
95.00	32648.0
96.00	2319.0
103.80	152.0
105.80	175.0
115.90	110.0
116.90	192.0
117.80	109.0
118.90	140.0
140.80	294.0
142.90	462.0
144.80	138.0
171.90	480.0
173.10	403.0
174.00	27664.0
175.00	2115.0
175.90	26776.0
176.90	1700.0

m/z	Abundance
35.00	284.0
37.00	1179.0
38.00	1396.0
39.00	553.0
39.00	235.0
44.00	601.0
45.00	278.0
47.00	316.0
47.80	166.0
49.00	1260.0
50.00	5348.0
51.00	1704.0
55.00	148.0
56.00	400.0
57.00	825.0
59.90	308.0
61.00	1486.0
62.00	1410.0
63.00	1148.0
63.90	256.0
65.00	455.0
68.00	3046.0
69.00	3136.0
70.00	240.0
71.90	143.0
73.00	1307.0
74.00	4970.0
75.00	15345.0
76.00	1245.0
76.90	236.0
77.90	157.0
78.90	977.0
80.00	296.0
81.00	1011.0
81.90	262.0
87.00	1328.0
87.90	1479.0
91.00	102.0
92.00	890.0
93.00	1270.0
94.00	3625.0
95.00	30400.0
96.00	2114.0
103.80	113.0
105.80	174.0
115.80	116.0
117.00	185.0
117.80	111.0
118.90	156.0
140.80	287.0
142.90	420.0
144.80	129.0
171.90	507.0
173.00	381.0
173.90	26288.0
174.90	2098.0
175.90	25512.0
176.90	1554.0