

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031718.D
 Acq On : 02 May 2019 17:38
 Operator : JC/SP
 Sample : K2661-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	87	94	108	rVB	544072	597368	15.86%	1.978%
2	1.678	175	183	199	rBV	417144	529207	14.05%	1.752%
3	2.267	355	366	379	rVB	898449	1362118	36.15%	4.510%
4	2.418	409	413	418	rVB3	2190	2158	0.06%	0.007%
5	2.447	418	422	424	rBV3	2204	1696	0.05%	0.006%
6	2.672	488	492	494	rBV2	1235	1020	0.03%	0.003%
7	2.694	496	499	505	rVB5	2914	2635	0.07%	0.009%
8	2.820	534	538	539	rBV3	2016	1279	0.03%	0.004%
9	2.829	539	541	544	rVV3	2040	1421	0.04%	0.005%
10	2.846	544	546	550	rVB	1833	1262	0.03%	0.004%
11	2.868	550	553	556	rBV3	1680	992	0.03%	0.003%
12	2.887	556	559	562	rBV4	971	873	0.02%	0.003%
13	2.981	583	588	592	rVV6	2870	3497	0.09%	0.012%
14	3.042	603	607	610	rVV3	990	864	0.02%	0.003%
15	3.151	637	641	645	rBV5	1190	1200	0.03%	0.004%
16	3.209	652	659	661	rBV4	1637	1830	0.05%	0.006%
17	3.309	685	690	694	rVB4	1907	1691	0.04%	0.006%
18	3.473	738	741	746	rVV3	1914	1472	0.04%	0.005%
19	3.498	746	749	753	rVB3	1583	1043	0.03%	0.003%
20	3.543	758	763	766	rBV3	2068	1461	0.04%	0.005%
21	3.633	787	791	795	rVB4	1623	1489	0.04%	0.005%
22	3.807	840	845	848	rBV5	1669	1326	0.04%	0.004%
23	4.112	938	940	944	rVB2	1666	1178	0.03%	0.004%
24	4.141	944	949	950	rBV2	1486	1258	0.03%	0.004%
25	4.190	950	964	1003	rBV	352939	1238951	32.88%	4.102%
26	4.643	1086	1105	1131	rBV	588264	1416277	37.59%	4.689%
27	4.878	1175	1178	1179	rBV3	1960	1242	0.03%	0.004%
28	4.974	1203	1208	1210	rBV4	2094	1988	0.05%	0.007%
29	5.074	1236	1239	1244	rVB2	1410	1092	0.03%	0.004%
30	5.170	1266	1269	1272	rVB2	1877	1167	0.03%	0.004%
31	5.193	1272	1276	1279	rBV3	1015	854	0.02%	0.003%
32	5.218	1280	1284	1289	rBV3	1401	1028	0.03%	0.003%
33	5.334	1296	1320	1347	rBV2	1284221	3767684	100.00%	12.475%
34	5.736	1441	1445	1448	rBV3	1467	1139	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031718.D
 Acq On : 02 May 2019 17:38
 Operator : JC/SP
 Sample : K2661-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.881	1473	1490	1513	rBV	1117807	2294546	60.90%	7.597%
36	6.183	1570	1584	1603	rBV3	285336	594282	15.77%	1.968%
37	6.324	1614	1628	1663	rBV	825125	1702167	45.18%	5.636%
38	6.572	1703	1705	1708	rBV2	1414	926	0.02%	0.003%
39	6.791	1769	1773	1780	rVB4	1788	1840	0.05%	0.006%
40	6.926	1812	1815	1818	rVB2	1876	1155	0.03%	0.004%
41	6.945	1818	1821	1826	rBV3	1785	1990	0.05%	0.007%
42	7.013	1838	1842	1847	rBV6	1658	1158	0.03%	0.004%
43	7.077	1858	1862	1866	rBV3	1593	1145	0.03%	0.004%
44	7.112	1870	1873	1877	rBV4	1160	955	0.03%	0.003%
45	7.225	1894	1908	1933	rBV	465714	868669	23.06%	2.876%
46	7.424	1966	1970	1973	rBV3	1864	1607	0.04%	0.005%
47	7.562	1999	2013	2045	rBV	1574139	2925169	77.64%	9.685%
48	7.849	2089	2102	2134	rBV	306962	575677	15.28%	1.906%
49	8.103	2178	2181	2190	rVB7	2342	3101	0.08%	0.010%
50	8.151	2190	2196	2198	rBV4	1800	1864	0.05%	0.006%
51	8.225	2207	2219	2235	rBV	338931	595629	15.81%	1.972%
52	8.312	2235	2246	2279	rVV	1245227	2321121	61.61%	7.685%
53	8.726	2373	2375	2381	rVB3	2357	1746	0.05%	0.006%
54	8.758	2381	2385	2388	rBV2	1527	1042	0.03%	0.003%
55	8.784	2388	2393	2396	rBV4	1756	1620	0.04%	0.005%
56	8.807	2396	2400	2403	rBV5	1654	1449	0.04%	0.005%
57	8.897	2423	2428	2431	rBV4	2062	1628	0.04%	0.005%
58	8.935	2435	2440	2443	rBV5	2150	1810	0.05%	0.006%
59	9.016	2462	2465	2466	rBV2	1628	975	0.03%	0.003%
60	9.086	2474	2487	2527	rBV	1586889	2764637	73.38%	9.154%
61	9.302	2550	2554	2555	rBV3	1431	1023	0.03%	0.003%
62	9.357	2565	2571	2572	rBV4	2262	1985	0.05%	0.007%
63	9.463	2602	2604	2610	rVV7	1095	1123	0.03%	0.004%
64	9.675	2667	2670	2676	rVB5	1987	1924	0.05%	0.006%
65	9.707	2676	2680	2685	rBV3	2057	2178	0.06%	0.007%
66	9.948	2752	2755	2758	rVB3	1155	866	0.02%	0.003%
67	10.022	2774	2778	2780	rBV3	1520	1241	0.03%	0.004%
68	10.109	2800	2805	2810	rBV4	1252	1669	0.04%	0.006%
69	10.135	2810	2813	2815	rVV2	1958	1213	0.03%	0.004%
70	10.180	2824	2827	2829	rVB3	1487	861	0.02%	0.003%
71	10.427	2892	2904	2934	rVV	1050824	1706065	45.28%	5.649%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031718.D
 Acq On : 02 May 2019 17:38
 Operator : JC/SP
 Sample : K2661-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.533	2934	2937	2941	rVB3	1747	1534	0.04%	0.005%
73	10.594	2951	2956	2959	rBV6	1664	1866	0.05%	0.006%
74	10.681	2980	2983	2986	rVB2	1591	1242	0.03%	0.004%
75	10.729	2993	2998	3000	rBV3	1854	1417	0.04%	0.005%
76	10.771	3005	3011	3013	rBV6	1551	1293	0.03%	0.004%
77	10.893	3045	3049	3053	rBV5	1887	1503	0.04%	0.005%
78	10.948	3062	3066	3070	rBV5	1350	1110	0.03%	0.004%
79	11.073	3102	3105	3107	rBV3	1872	1434	0.04%	0.005%
80	11.154	3124	3130	3133	rBV6	1212	1519	0.04%	0.005%
81	11.218	3146	3150	3152	rBV5	1434	1117	0.03%	0.004%
82	11.353	3189	3192	3196	rVB2	1174	975	0.03%	0.003%
83	11.482	3219	3232	3250	rBV	1442537	2344633	62.23%	7.763%
84	11.855	3336	3348	3376	rBV	1347404	2248284	59.67%	7.444%
85	12.369	3505	3508	3509	rBV2	2176	1167	0.03%	0.004%
86	12.517	3551	3554	3557	rBV3	1469	1077	0.03%	0.004%
87	12.559	3565	3567	3573	rBV4	1929	1787	0.05%	0.006%
88	12.649	3593	3595	3598	rBV3	1833	1100	0.03%	0.004%
89	12.710	3612	3614	3618	rVB2	2567	1483	0.04%	0.005%
90	12.729	3618	3620	3622	rBV2	2505	1622	0.04%	0.005%
91	13.096	3732	3734	3739	rVB4	1511	1135	0.03%	0.004%
92	13.295	3794	3796	3799	rBV4	1297	1037	0.03%	0.003%
93	13.424	3833	3836	3843	rVB6	2288	1716	0.05%	0.006%
94	13.482	3849	3854	3855	rBV2	1441	1316	0.03%	0.004%
95	13.520	3864	3866	3869	rBV3	1531	849	0.02%	0.003%
96	13.765	3930	3942	3957	rVV	31978	94048	2.50%	0.311%
97	14.057	4030	4033	4037	rVB3	2817	2134	0.06%	0.007%
98	14.112	4048	4050	4053	rBV3	2125	1284	0.03%	0.004%
99	14.897	4284	4294	4314	rBV3	41109	103856	2.76%	0.344%
100	15.070	4343	4348	4365	rVB4	17922	39471	1.05%	0.131%


Sum of corrected areas: 30202825

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050219\
Data File : VU031718.D
Acq On : 02 May 2019 17:38
Operator : JC/SP
Sample : K2661-05 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

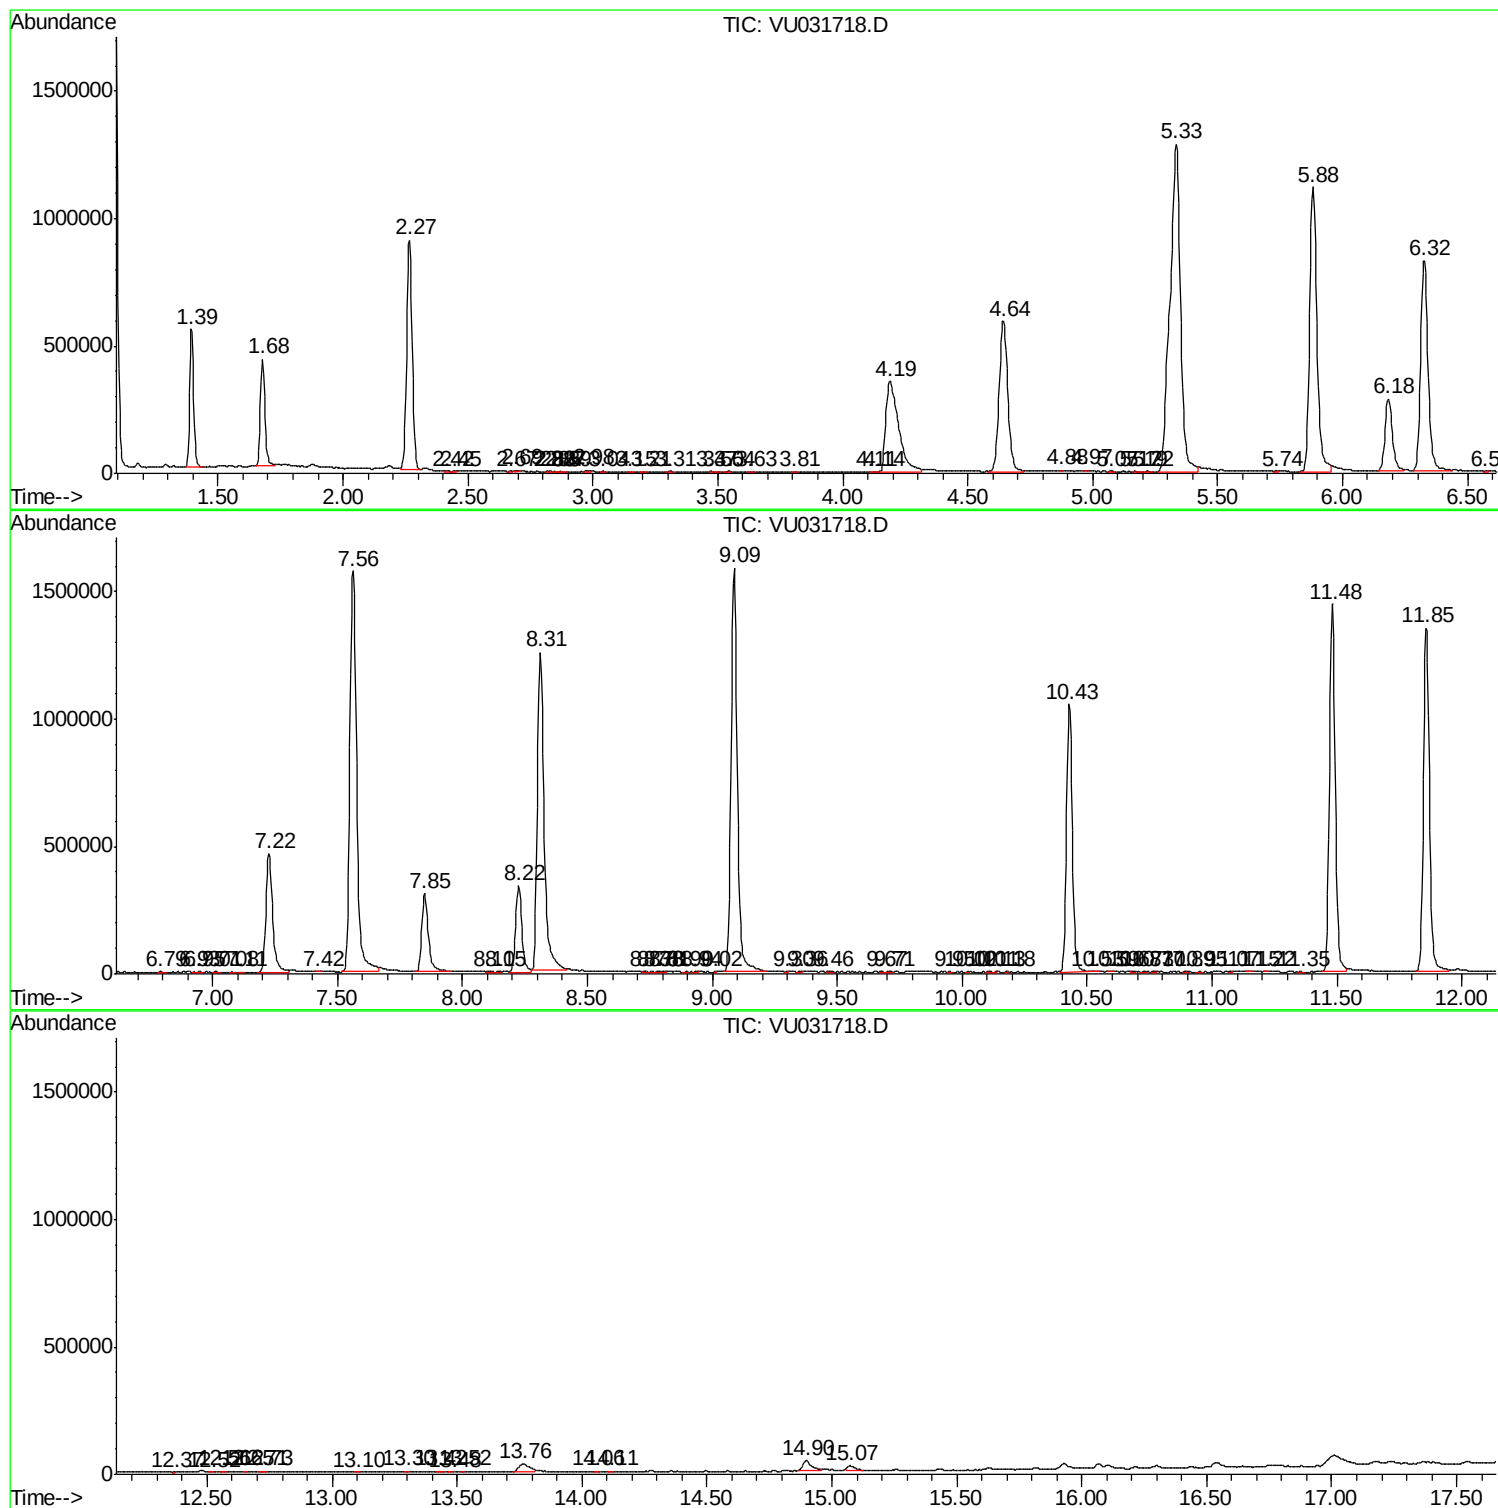

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031718.D
Acq On : 02 May 2019 17:38
Operator : JC/SP
Sample : K2661-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031718.D
Acq On : 02 May 2019 17:38
Operator : JC/SP
Sample : K2661-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
