

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031719.D
 Acq On : 02 May 2019 18:02
 Operator : JC/SP
 Sample : K2661-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rBV3	15096	14263	0.35%	0.046%
2	1.392	87	94	108	rBV	586540	642106	15.77%	2.079%
3	1.675	175	182	199	rVB	460191	563475	13.84%	1.824%
4	2.267	355	366	379	rBV	963281	1460821	35.89%	4.730%
5	2.444	418	421	425	rBV5	1606	1670	0.04%	0.005%
6	2.518	440	444	450	rVB4	1886	1938	0.05%	0.006%
7	2.691	494	498	500	rBV3	2895	2479	0.06%	0.008%
8	2.913	563	567	573	rBV2	1431	1501	0.04%	0.005%
9	2.987	586	590	594	rBV4	1905	1459	0.04%	0.005%
10	3.013	594	598	601	rBV3	708	748	0.02%	0.002%
11	3.109	626	628	631	rVB3	1607	770	0.02%	0.002%
12	3.293	682	685	688	rBV2	1068	827	0.02%	0.003%
13	3.350	699	703	706	rBV2	1681	1395	0.03%	0.005%
14	3.376	708	711	713	rBV3	1336	959	0.02%	0.003%
15	3.469	733	740	745	rBV3	1621	2149	0.05%	0.007%
16	3.569	767	771	774	rBV3	988	739	0.02%	0.002%
17	3.736	820	823	829	rVV6	1588	1470	0.04%	0.005%
18	3.903	872	875	881	rBV5	967	804	0.02%	0.003%
19	3.993	899	903	908	rVB3	1390	1378	0.03%	0.004%
20	4.038	913	917	918	rBV2	1326	908	0.02%	0.003%
21	4.119	939	942	950	rVB4	1539	1715	0.04%	0.006%
22	4.183	950	962	994	rBV	389211	1132272	27.82%	3.666%
23	4.643	1088	1105	1127	rBV	637375	1510158	37.10%	4.889%
24	4.955	1198	1202	1205	rBV4	1098	1037	0.03%	0.003%
25	4.984	1205	1211	1224	rVV4	3857	8269	0.20%	0.027%
26	5.119	1250	1253	1254	rBV	1558	740	0.02%	0.002%
27	5.132	1254	1257	1260	rVB4	2135	1402	0.03%	0.005%
28	5.161	1260	1266	1269	rBV3	1357	1521	0.04%	0.005%
29	5.247	1286	1293	1296	rBV5	2472	2339	0.06%	0.008%
30	5.334	1296	1320	1352	rBV2	1368036	4070544	100.00%	13.179%
31	5.881	1474	1490	1515	rBV	1155921	2371103	58.25%	7.677%
32	6.186	1574	1585	1598	rBV6	22368	46123	1.13%	0.149%
33	6.325	1614	1628	1655	rBV	888174	1830371	44.97%	5.926%
34	6.681	1735	1739	1743	rVB4	2228	1816	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031719.D
 Acq On : 02 May 2019 18:02
 Operator : JC/SP
 Sample : K2661-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.723	1749	1752	1755	rVB3	1139	740	0.02%	0.002%
36	6.768	1760	1766	1770	rBV6	1264	1534	0.04%	0.005%
37	6.810	1775	1779	1784	rBV5	1665	1641	0.04%	0.005%
38	6.858	1792	1794	1801	rVB6	1003	836	0.02%	0.003%
39	6.894	1801	1805	1809	rBV4	1974	2186	0.05%	0.007%
40	6.935	1815	1818	1822	rVB4	1559	1255	0.03%	0.004%
41	6.987	1830	1834	1838	rBV5	2155	2139	0.05%	0.007%
42	7.067	1856	1859	1866	rVB5	1286	1324	0.03%	0.004%
43	7.116	1869	1874	1877	rBV3	958	964	0.02%	0.003%
44	7.225	1895	1908	1942	rBV	496803	936795	23.01%	3.033%
45	7.453	1976	1979	1983	rVB3	1803	1333	0.03%	0.004%
46	7.562	1999	2013	2061	rBV	1697512	3177139	78.05%	10.286%
47	7.849	2090	2102	2122	rBV	331019	606272	14.89%	1.963%
48	8.128	2184	2189	2191	rVB3	1257	1073	0.03%	0.003%
49	8.144	2191	2194	2197	rBV2	1365	826	0.02%	0.003%
50	8.170	2197	2202	2205	rBV6	2012	1979	0.05%	0.006%
51	8.225	2207	2219	2233	rBV2	206693	368229	9.05%	1.192%
52	8.308	2235	2245	2282	rVV	1331522	2461354	60.47%	7.969%
53	8.607	2335	2338	2344	rBV5	1209	1325	0.03%	0.004%
54	8.826	2401	2406	2410	rBV3	2159	2008	0.05%	0.007%
55	9.087	2474	2487	2532	rBV	1622600	2850625	70.03%	9.229%
56	9.254	2537	2539	2542	rBV3	1720	1257	0.03%	0.004%
57	9.344	2562	2567	2570	rBV4	1603	1517	0.04%	0.005%
58	9.366	2571	2574	2577	rVV4	1892	1445	0.04%	0.005%
59	9.389	2577	2581	2586	rVV6	2003	2309	0.06%	0.007%
60	9.414	2586	2589	2594	rVV4	1947	1668	0.04%	0.005%
61	9.440	2594	2597	2601	rVV4	1294	925	0.02%	0.003%
62	9.463	2601	2604	2609	rVB6	2096	1602	0.04%	0.005%
63	9.514	2616	2620	2623	rBV5	1448	1204	0.03%	0.004%
64	9.659	2661	2665	2668	rBV4	1569	1537	0.04%	0.005%
65	9.701	2674	2678	2681	rBV5	1700	1500	0.04%	0.005%
66	9.736	2686	2689	2691	rBV3	1290	915	0.02%	0.003%
67	9.781	2697	2703	2705	rBV4	2000	2147	0.05%	0.007%
68	9.820	2712	2715	2720	rBV5	1836	1443	0.04%	0.005%
69	9.913	2740	2744	2747	rBV3	1432	1236	0.03%	0.004%
70	9.996	2767	2770	2773	rBV	1780	1401	0.03%	0.005%
71	10.080	2793	2796	2798	rBV2	1120	784	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031719.D
 Acq On : 02 May 2019 18:02
 Operator : JC/SP
 Sample : K2661-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.103	2800	2803	2805	rVB	1416	778	0.02%	0.003%
73	10.141	2810	2815	2821	rBV3	2102	2728	0.07%	0.009%
74	10.238	2842	2845	2848	rVV2	1439	880	0.02%	0.003%
75	10.318	2867	2870	2875	rBV2	1340	1005	0.02%	0.003%
76	10.427	2892	2904	2927	rBV	1109239	1813996	44.56%	5.873%
77	10.591	2953	2955	2962	rBV4	1349	1171	0.03%	0.004%
78	10.640	2967	2970	2974	rBV3	1920	1140	0.03%	0.004%
79	10.775	3010	3012	3017	rVB6	1526	1135	0.03%	0.004%
80	10.810	3017	3023	3027	rBV4	2285	2128	0.05%	0.007%
81	10.832	3027	3030	3034	rVB4	1923	1351	0.03%	0.004%
82	10.865	3037	3040	3044	rBV2	1356	1310	0.03%	0.004%
83	10.935	3059	3062	3066	rVB2	1172	853	0.02%	0.003%
84	11.176	3132	3137	3140	rBV4	1421	1337	0.03%	0.004%
85	11.231	3149	3154	3159	rBV4	2254	3067	0.08%	0.010%
86	11.366	3193	3196	3201	rBV4	1755	1423	0.03%	0.005%
87	11.395	3201	3205	3207	rBV3	1895	1543	0.04%	0.005%
88	11.479	3219	3231	3257	rBV	1461068	2405833	59.10%	7.789%
89	11.746	3311	3314	3318	rBV3	1572	1096	0.03%	0.004%
90	11.855	3337	3348	3373	rBV	1433588	2386975	58.64%	7.728%
91	12.221	3457	3462	3466	rBV4	2023	2383	0.06%	0.008%
92	12.479	3536	3542	3551	rVV4	4835	7420	0.18%	0.024%
93	12.530	3554	3558	3561	rVB5	1623	1356	0.03%	0.004%
94	12.643	3591	3593	3596	rVB3	2005	967	0.02%	0.003%
95	12.955	3688	3690	3692	rBV	1717	886	0.02%	0.003%
96	13.366	3815	3818	3821	rBV2	2161	1400	0.03%	0.005%
97	13.475	3849	3852	3857	rBV5	2006	2311	0.06%	0.007%
98	13.688	3916	3918	3921	rVB	1548	751	0.02%	0.002%
99	13.765	3934	3942	3961	rBV2	20427	57777	1.42%	0.187%
100	14.900	4287	4295	4306	rBV4	24774	56455	1.39%	0.183%


Sum of corrected areas: 30887191

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050219\
Data File : VU031719.D
Acq On : 02 May 2019 18:02
Operator : JC/SP
Sample : K2661-06 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

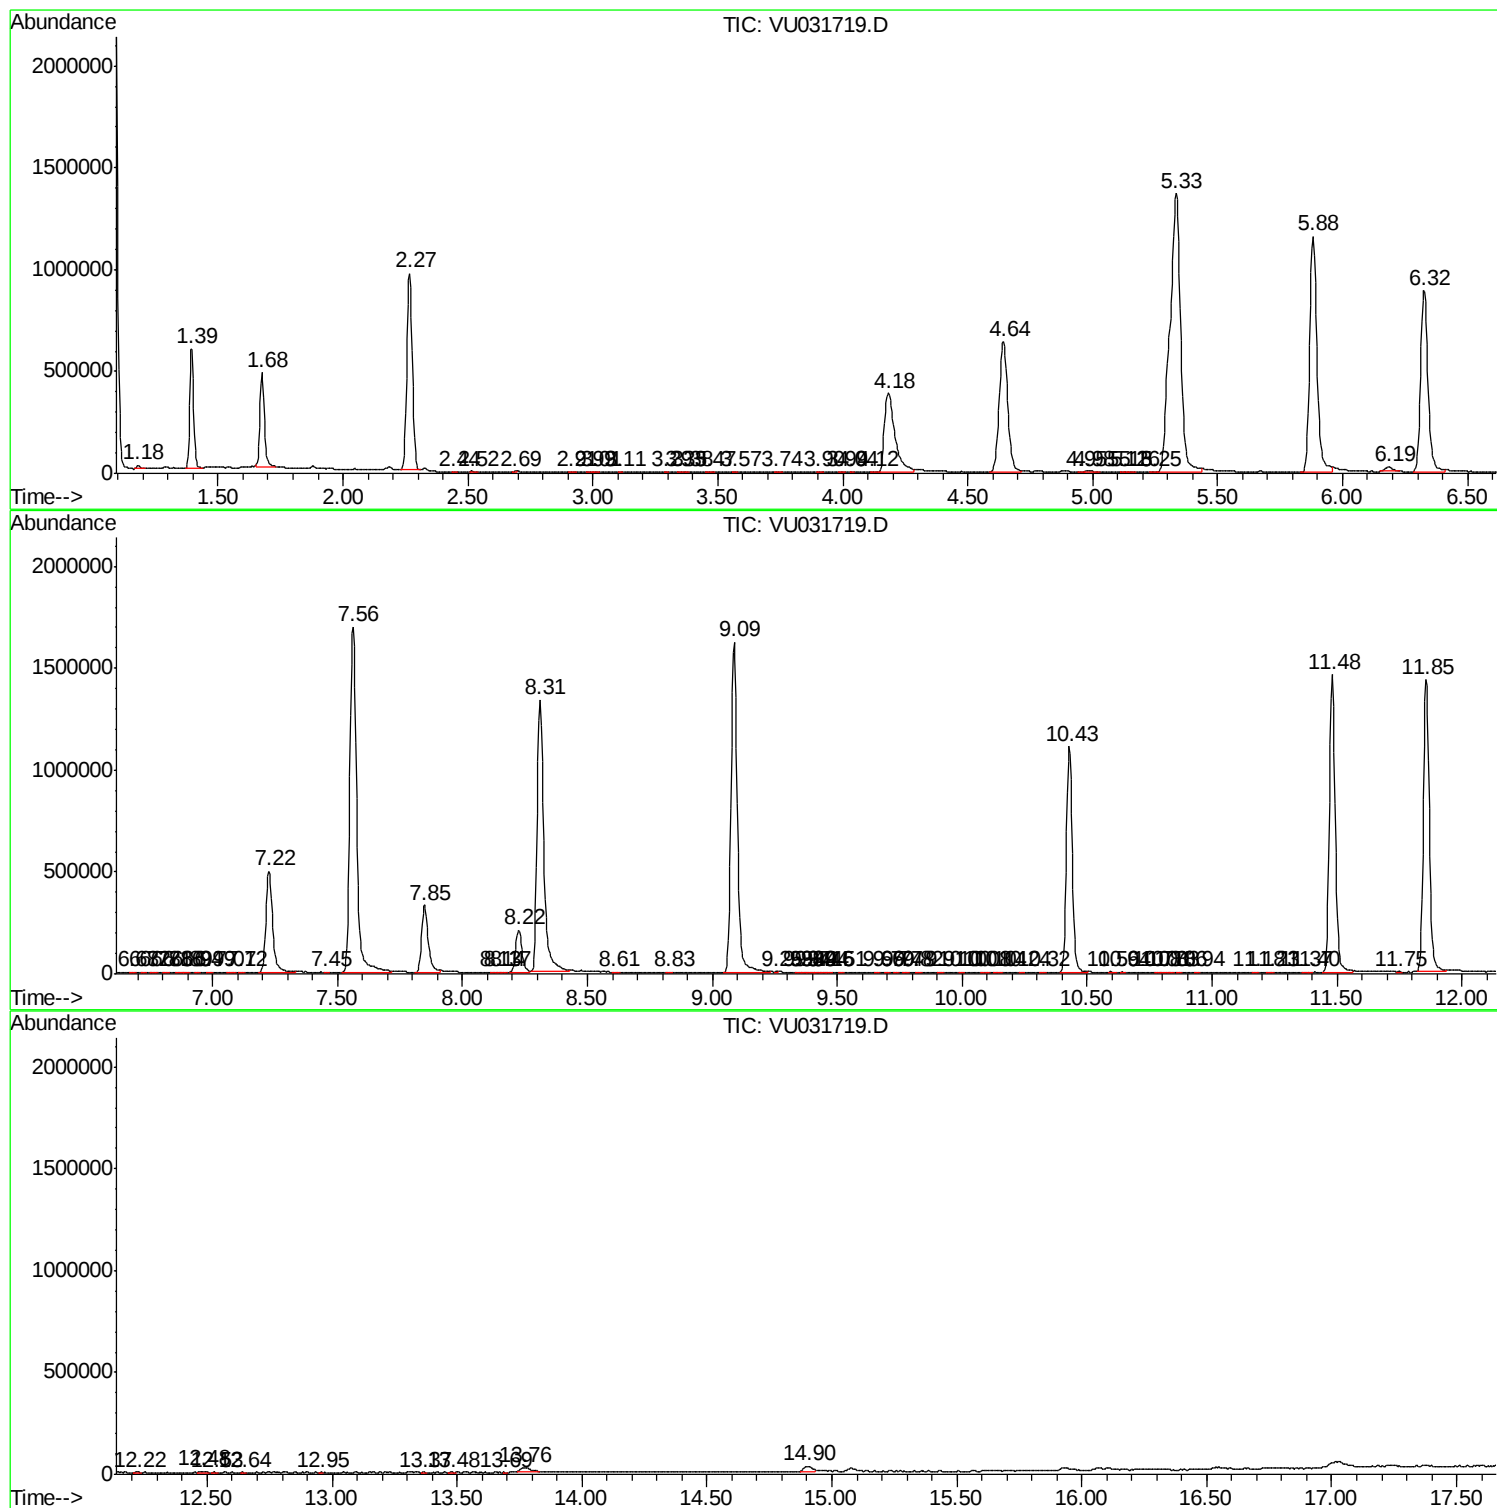

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031719.D
Acq On : 02 May 2019 18:02
Operator : JC/SP
Sample : K2661-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031719.D
Acq On : 02 May 2019 18:02
Operator : JC/SP
Sample : K2661-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc