

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031724.D
 Acq On : 02 May 2019 19:59
 Operator : JC/SP
 Sample : K2661-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB4	18039	18646	0.46%	0.062%
2	1.396	87	95	110	rVB	585689	639551	15.87%	2.128%
3	1.679	175	183	194	rBV	445306	559373	13.88%	1.861%
4	2.267	355	366	380	rVB	956696	1437156	35.67%	4.782%
5	2.537	448	450	455	rBV3	1922	1873	0.05%	0.006%
6	2.563	455	458	460	rBV2	2031	1136	0.03%	0.004%
7	2.659	483	488	491	rBV2	2221	2022	0.05%	0.007%
8	2.675	491	493	497	rBV4	1731	1497	0.04%	0.005%
9	2.965	579	583	589	rVB4	1888	1950	0.05%	0.006%
10	3.039	604	606	609	rVB2	1624	970	0.02%	0.003%
11	3.058	609	612	613	rBV2	1541	737	0.02%	0.002%
12	3.132	630	635	639	rVB2	1543	1455	0.04%	0.005%
13	3.151	639	641	646	rBV3	896	875	0.02%	0.003%
14	3.193	650	654	656	rBV3	1392	929	0.02%	0.003%
15	3.219	657	662	664	rBV3	942	929	0.02%	0.003%
16	3.389	707	715	718	rBV3	2704	3270	0.08%	0.011%
17	3.437	727	730	733	rVB2	1309	799	0.02%	0.003%
18	3.457	733	736	738	rBV	1374	795	0.02%	0.003%
19	3.524	753	757	761	rBV2	1500	1205	0.03%	0.004%
20	3.601	778	781	785	rVB3	933	746	0.02%	0.002%
21	3.621	785	787	791	rBV3	1052	790	0.02%	0.003%
22	3.707	809	814	818	rVB2	1283	865	0.02%	0.003%
23	3.749	823	827	829	rBV3	1131	1057	0.03%	0.004%
24	3.810	841	846	852	rBV	998	1349	0.03%	0.004%
25	3.994	898	903	905	rBV5	1146	915	0.02%	0.003%
26	4.032	912	915	917	rBV2	1291	898	0.02%	0.003%
27	4.090	930	933	935	rVV3	1246	860	0.02%	0.003%
28	4.186	950	963	1002	rBV	359575	1122986	27.87%	3.737%
29	4.643	1088	1105	1128	rBV	624437	1492664	37.05%	4.967%
30	4.971	1204	1207	1209	rBV3	1822	1154	0.03%	0.004%
31	4.987	1210	1212	1217	rVB3	2199	1722	0.04%	0.006%
32	5.096	1242	1246	1249	rBV4	2643	2149	0.05%	0.007%
33	5.334	1297	1320	1352	rBV2	1356279	4028802	100.00%	13.406%
34	5.653	1415	1419	1423	rBV2	2369	2347	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031724.D
 Acq On : 02 May 2019 19:59
 Operator : JC/SP
 Sample : K2661-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.810	1465	1468	1472	rVB3	1425	1087	0.03%	0.004%
36	5.881	1476	1490	1521	rBV	1138975	2344748	58.20%	7.802%
37	6.180	1574	1583	1594	rBV7	12571	25494	0.63%	0.085%
38	6.325	1614	1628	1663	rBV	876107	1817537	45.11%	6.048%
39	6.547	1693	1697	1699	rBV3	1406	891	0.02%	0.003%
40	6.662	1730	1733	1738	rVB5	1757	1370	0.03%	0.005%
41	6.784	1765	1771	1772	rBV3	1116	930	0.02%	0.003%
42	6.874	1794	1799	1800	rBV3	1200	810	0.02%	0.003%
43	6.919	1808	1813	1815	rBV5	1713	1549	0.04%	0.005%
44	6.952	1820	1823	1825	rVB4	1549	991	0.02%	0.003%
45	7.042	1848	1851	1854	rVB2	1319	885	0.02%	0.003%
46	7.225	1894	1908	1934	rBV	473804	907272	22.52%	3.019%
47	7.444	1973	1976	1978	rBV3	1430	981	0.02%	0.003%
48	7.514	1994	1998	2000	rBV3	1810	1454	0.04%	0.005%
49	7.563	2000	2013	2056	rVV	1649649	3103048	77.02%	10.325%
50	7.849	2091	2102	2129	rBV	313454	583791	14.49%	1.943%
51	8.122	2186	2187	2193	rVB3	1331	1001	0.02%	0.003%
52	8.177	2198	2204	2207	rBV7	2151	1856	0.05%	0.006%
53	8.228	2212	2220	2228	rVB7	4844	7983	0.20%	0.027%
54	8.263	2228	2231	2232	rBV2	1396	880	0.02%	0.003%
55	8.312	2234	2246	2292	rBV	1301647	2489743	61.80%	8.285%
56	8.771	2385	2389	2390	rBV4	1193	1053	0.03%	0.004%
57	8.826	2402	2406	2410	rBV5	1006	892	0.02%	0.003%
58	8.894	2420	2427	2428	rBV5	1526	1418	0.04%	0.005%
59	8.964	2446	2449	2454	rBV5	971	910	0.02%	0.003%
60	9.087	2474	2487	2517	rBV	1620732	2822555	70.06%	9.392%
61	9.408	2584	2587	2590	rBV3	2083	1470	0.04%	0.005%
62	9.521	2616	2622	2625	rBV6	1388	1101	0.03%	0.004%
63	9.540	2625	2628	2632	rBV3	1354	923	0.02%	0.003%
64	9.562	2632	2635	2643	rVB6	1804	2416	0.06%	0.008%
65	9.598	2643	2646	2649	rBV2	1383	984	0.02%	0.003%
66	9.620	2649	2653	2656	rBV2	1264	1227	0.03%	0.004%
67	9.752	2691	2694	2699	rBV6	1718	1201	0.03%	0.004%
68	9.788	2702	2705	2708	rVV3	1464	1007	0.02%	0.003%
69	9.858	2722	2727	2730	rBV5	1124	933	0.02%	0.003%
70	9.881	2732	2734	2737	rVV3	1127	737	0.02%	0.002%
71	10.032	2775	2781	2782	rBV2	2206	1904	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031724.D
 Acq On : 02 May 2019 19:59
 Operator : JC/SP
 Sample : K2661-12 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B32

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.132	2808	2812	2814	rBV3	1707	1271	0.03%	0.004%
73	10.164	2819	2822	2826	rBV2	1371	1333	0.03%	0.004%
74	10.260	2848	2852	2861	rVB3	2028	2412	0.06%	0.008%
75	10.299	2861	2864	2872	rBV3	1823	1830	0.05%	0.006%
76	10.337	2872	2876	2880	rVB3	1202	1013	0.03%	0.003%
77	10.360	2880	2883	2888	rVB2	1195	751	0.02%	0.002%
78	10.427	2888	2904	2933	rBV	1113666	1825674	45.32%	6.075%
79	10.585	2951	2953	2961	rVV4	1945	2278	0.06%	0.008%
80	10.694	2983	2987	2990	rBV5	1543	1045	0.03%	0.003%
81	10.823	3022	3027	3035	rVB6	1652	2400	0.06%	0.008%
82	10.871	3038	3042	3048	rVB5	1681	1629	0.04%	0.005%
83	10.903	3048	3052	3053	rBV	1338	1059	0.03%	0.004%
84	11.016	3082	3087	3094	rBV3	1847	2463	0.06%	0.008%
85	11.238	3152	3156	3158	rBV2	904	804	0.02%	0.003%
86	11.302	3174	3176	3180	rVB3	1258	826	0.02%	0.003%
87	11.363	3191	3195	3197	rBV5	1164	998	0.02%	0.003%
88	11.424	3209	3214	3217	rBV5	1915	1841	0.05%	0.006%
89	11.479	3219	3231	3257	rBV	1450600	2364921	58.70%	7.869%
90	11.855	3336	3348	3373	rBV	1375372	2332758	57.90%	7.762%
91	12.331	3493	3496	3498	rBV3	1125	959	0.02%	0.003%
92	12.392	3511	3515	3517	rBV4	1001	831	0.02%	0.003%
93	12.688	3605	3607	3610	rBV2	1726	747	0.02%	0.002%
94	12.958	3687	3691	3695	rBV3	2691	2170	0.05%	0.007%
95	13.029	3711	3713	3718	rVB4	1521	1201	0.03%	0.004%
96	13.562	3876	3879	3883	rBV2	1532	1179	0.03%	0.004%
97	13.781	3937	3947	3955	rBV6	10354	24032	0.60%	0.080%
98	14.074	4035	4038	4041	rVB2	3492	1918	0.05%	0.006%
99	14.093	4041	4044	4047	rBV3	2320	1746	0.04%	0.006%
100	14.331	4116	4118	4121	rBV4	1715	1150	0.03%	0.004%


Sum of corrected areas: 30052743

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050219\
Data File : VU031724.D
Acq On : 02 May 2019 19:59
Operator : JC/SP
Sample : K2661-12 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B32

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

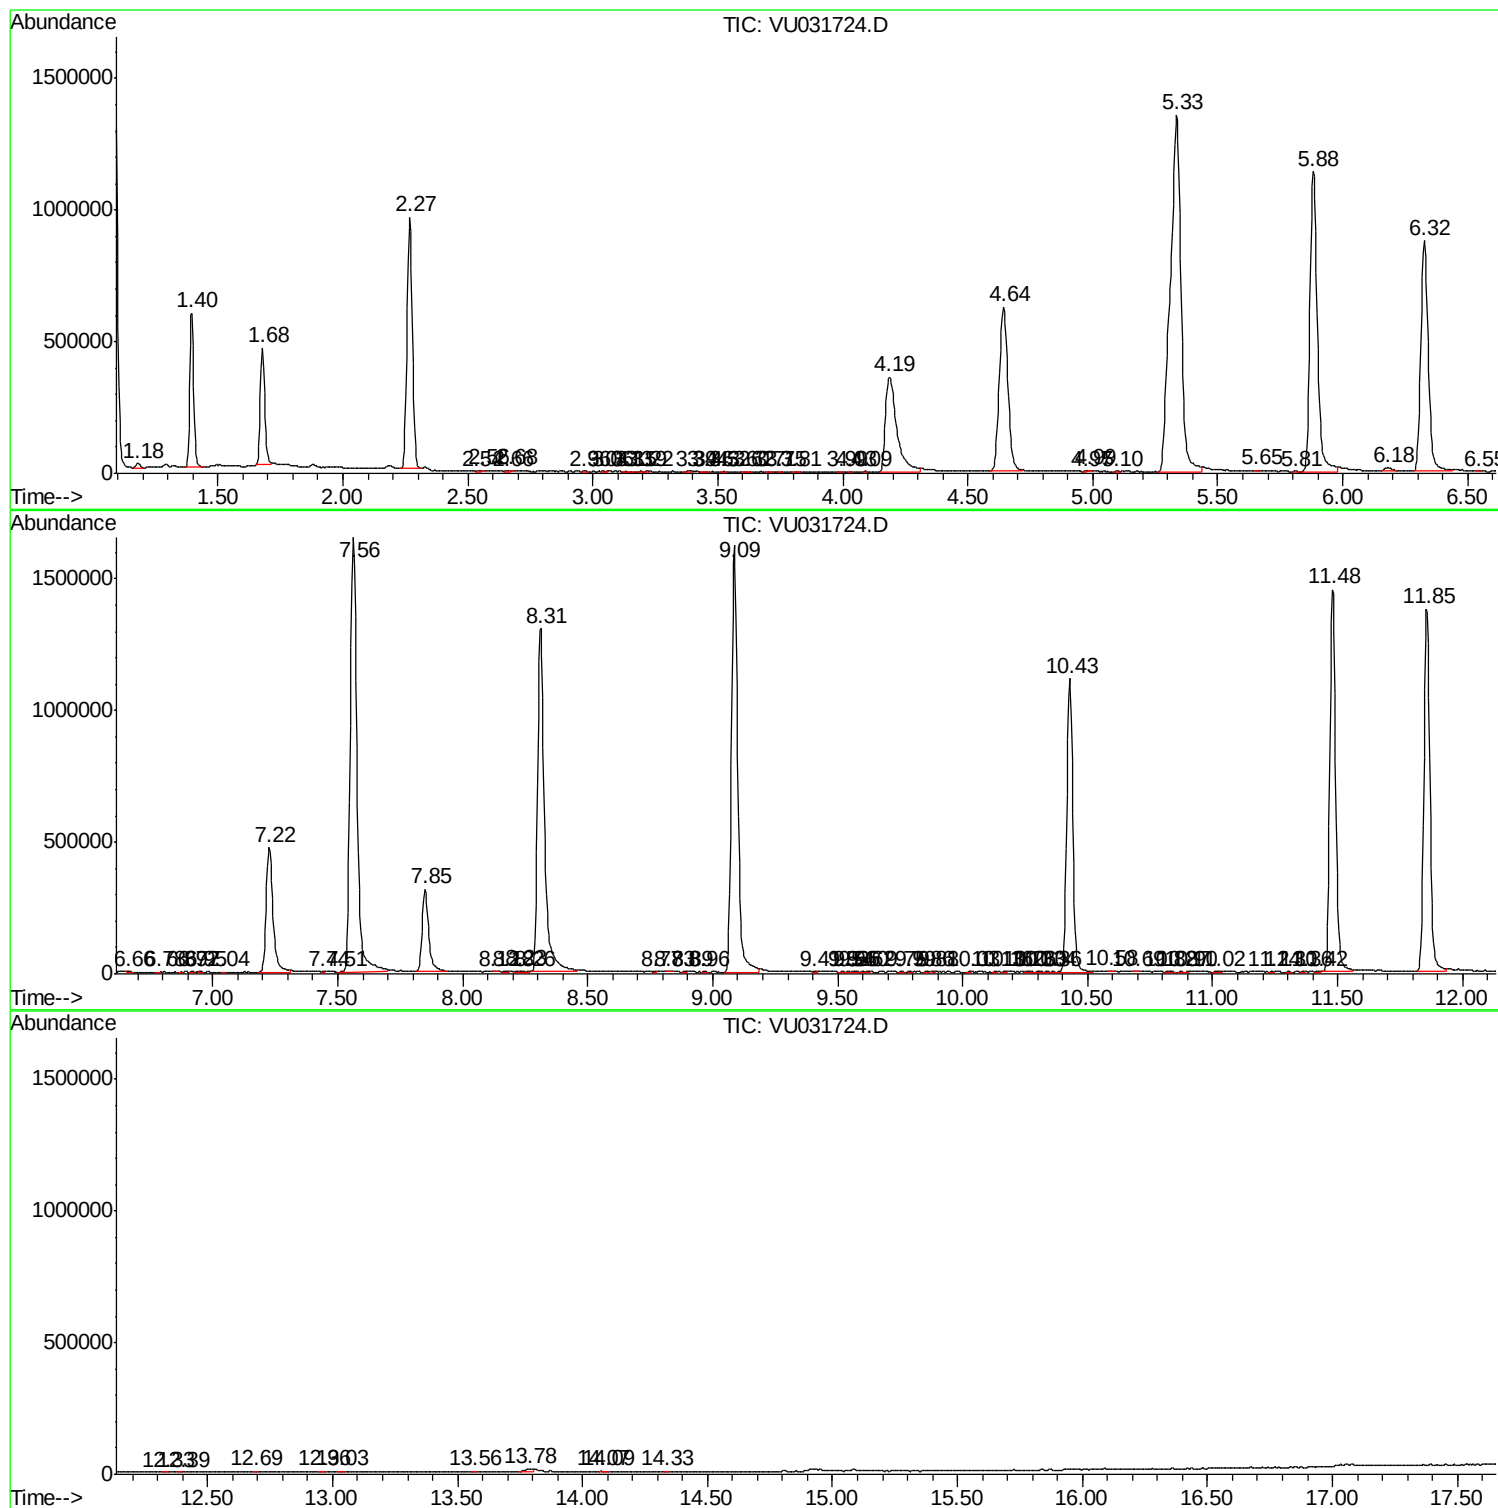

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031724.D
Acq On : 02 May 2019 19:59
Operator : JC/SP
Sample : K2661-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B32

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031724.D
Acq On : 02 May 2019 19:59
Operator : JC/SP
Sample : K2661-12 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B32

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc