

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031725.D
 Acq On : 02 May 2019 20:22
 Operator : JC/SP
 Sample : K2661-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	87	95	106	rVB	592526	643526	16.04%	2.127%
2	1.675	175	182	193	rBV	431598	539390	13.45%	1.783%
3	2.267	355	366	379	rBV	968989	1468762	36.62%	4.855%
4	2.431	415	417	421	rBV3	1149	940	0.02%	0.003%
5	2.527	445	447	452	rVB3	2186	1511	0.04%	0.005%
6	2.611	470	473	477	rVB3	2201	1434	0.04%	0.005%
7	2.634	477	480	483	rBV2	1987	1153	0.03%	0.004%
8	2.701	495	501	504	rBV7	3343	3481	0.09%	0.012%
9	2.865	549	552	556	rVB2	1916	1208	0.03%	0.004%
10	3.048	605	609	612	rBV3	1777	1254	0.03%	0.004%
11	3.087	617	621	624	rVV3	1411	1181	0.03%	0.004%
12	3.187	647	652	658	rBV5	1069	1211	0.03%	0.004%
13	3.225	659	664	668	rBV3	1073	951	0.02%	0.003%
14	3.248	668	671	676	rVB3	1231	1153	0.03%	0.004%
15	3.277	676	680	682	rBV2	1504	982	0.02%	0.003%
16	3.444	727	732	736	rBV2	1310	1265	0.03%	0.004%
17	3.563	765	769	774	rVB4	1681	1914	0.05%	0.006%
18	3.592	774	778	781	rBV2	1368	1251	0.03%	0.004%
19	3.682	803	806	810	rVB3	1257	869	0.02%	0.003%
20	3.733	819	822	825	rVB4	1134	842	0.02%	0.003%
21	3.820	846	849	853	rBV4	1111	924	0.02%	0.003%
22	4.016	902	910	912	rBV4	1754	1639	0.04%	0.005%
23	4.084	926	931	942	rVB4	2044	3465	0.09%	0.011%
24	4.125	942	944	948	rBV	1268	998	0.02%	0.003%
25	4.187	949	963	992	rBV	369107	1114740	27.79%	3.685%
26	4.643	1088	1105	1128	rVV	638040	1510894	37.67%	4.994%
27	4.984	1208	1211	1217	rVB6	2372	2764	0.07%	0.009%
28	5.093	1241	1245	1246	rBV	1134	893	0.02%	0.003%
29	5.334	1297	1320	1342	rBV2	1366118	4010781	100.00%	13.257%
30	5.598	1399	1402	1407	rVB6	1790	1246	0.03%	0.004%
31	5.785	1457	1460	1464	rBV3	1340	1085	0.03%	0.004%
32	5.881	1475	1490	1532	rBV	1165921	2426200	60.49%	8.019%
33	6.180	1577	1583	1585	rBV6	9760	11566	0.29%	0.038%
34	6.325	1614	1628	1656	rBV	877528	1835910	45.77%	6.068%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031725.D
 Acq On : 02 May 2019 20:22
 Operator : JC/SP
 Sample : K2661-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.569	1701	1704	1710	rVB6	1601	1417	0.04%	0.005%
36	6.711	1743	1748	1751	rBV3	2239	2199	0.05%	0.007%
37	6.784	1767	1771	1775	rBV5	1823	1413	0.04%	0.005%
38	6.855	1788	1793	1796	rBV4	1575	1543	0.04%	0.005%
39	6.897	1803	1806	1809	rBV4	1312	844	0.02%	0.003%
40	7.042	1849	1851	1856	rVB3	1953	1404	0.04%	0.005%
41	7.071	1856	1860	1866	rBV5	1892	2059	0.05%	0.007%
42	7.119	1872	1875	1880	rBV3	932	915	0.02%	0.003%
43	7.225	1896	1908	1930	rBV	480057	896656	22.36%	2.964%
44	7.501	1990	1994	1996	rBV3	1287	1085	0.03%	0.004%
45	7.563	1999	2013	2062	rBV	1677497	3133558	78.13%	10.357%
46	7.849	2091	2102	2127	rBV	317239	575786	14.36%	1.903%
47	8.051	2162	2165	2168	rBV5	1982	1476	0.04%	0.005%
48	8.225	2210	2219	2235	rBV5	27567	52732	1.31%	0.174%
49	8.312	2235	2246	2287	rBV	1304100	2503984	62.43%	8.276%
50	8.608	2336	2338	2344	rBV6	1467	1538	0.04%	0.005%
51	8.720	2370	2373	2377	rBV4	1472	1314	0.03%	0.004%
52	8.839	2408	2410	2414	rVV4	1648	1526	0.04%	0.005%
53	8.887	2418	2425	2429	rBV5	2582	3382	0.08%	0.011%
54	8.942	2439	2442	2444	rBV2	1571	1162	0.03%	0.004%
55	9.087	2474	2487	2534	rBV	1634914	2847528	71.00%	9.412%
56	9.370	2572	2575	2578	rBV3	2076	1424	0.04%	0.005%
57	9.395	2580	2583	2587	rVV3	1908	1706	0.04%	0.006%
58	9.460	2600	2603	2608	rBV3	1763	1755	0.04%	0.006%
59	9.694	2672	2676	2677	rBV	1508	918	0.02%	0.003%
60	9.730	2685	2687	2692	rBV3	1401	1038	0.03%	0.003%
61	9.781	2701	2703	2706	rVB2	1604	948	0.02%	0.003%
62	9.817	2711	2714	2717	rBV4	1512	1077	0.03%	0.004%
63	9.916	2742	2745	2748	rBV3	1779	1429	0.04%	0.005%
64	9.932	2748	2750	2757	rBV3	1107	992	0.02%	0.003%
65	10.074	2791	2794	2799	rVB2	1420	1180	0.03%	0.004%
66	10.109	2799	2805	2809	rBV5	1425	1714	0.04%	0.006%
67	10.280	2853	2858	2860	rVV3	1327	1084	0.03%	0.004%
68	10.353	2877	2881	2884	rBV2	1794	1425	0.04%	0.005%
69	10.427	2891	2904	2933	rBV	1136454	1831649	45.67%	6.054%
70	10.730	2995	2998	3000	rBV3	1503	864	0.02%	0.003%
71	10.781	3012	3014	3019	rVB4	1092	846	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050219\
 Data File : VU031725.D
 Acq On : 02 May 2019 20:22
 Operator : JC/SP
 Sample : K2661-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B33

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.813	3019	3024	3028	rBV3	2403	2317	0.06%	0.008%
73	10.868	3037	3041	3043	rBV4	1441	999	0.02%	0.003%
74	10.910	3051	3054	3057	rBV2	1676	1087	0.03%	0.004%
75	11.048	3095	3097	3103	rVB4	2205	1791	0.04%	0.006%
76	11.083	3103	3108	3112	rBV2	3181	2817	0.07%	0.009%
77	11.234	3151	3155	3160	rBV4	1541	1831	0.05%	0.006%
78	11.315	3175	3180	3183	rVB3	1426	1324	0.03%	0.004%
79	11.408	3205	3209	3212	rBV4	1583	1326	0.03%	0.004%
80	11.424	3212	3214	3219	rVB3	1804	1295	0.03%	0.004%
81	11.479	3219	3231	3254	rBV	1445432	2372439	59.15%	7.842%
82	11.855	3336	3348	3375	rBV	1404591	2339900	58.34%	7.734%
83	12.302	3484	3487	3490	rBV4	1408	1052	0.03%	0.003%
84	12.543	3560	3562	3565	rVB3	1898	966	0.02%	0.003%
85	12.569	3566	3570	3573	rBV5	1395	1274	0.03%	0.004%
86	12.611	3581	3583	3588	rVB2	2328	1825	0.05%	0.006%
87	12.636	3588	3591	3595	rBV3	1750	1487	0.04%	0.005%
88	12.678	3601	3604	3608	rBV5	1454	965	0.02%	0.003%
89	12.710	3612	3614	3617	rVB2	1977	1049	0.03%	0.003%
90	12.742	3620	3624	3628	rBV5	1845	1689	0.04%	0.006%
91	12.894	3668	3671	3675	rBV2	1633	1120	0.03%	0.004%
92	12.916	3675	3678	3681	rBV3	1407	1174	0.03%	0.004%
93	13.177	3754	3759	3763	rBV3	1771	1795	0.04%	0.006%
94	13.270	3786	3788	3793	rBV3	1289	958	0.02%	0.003%
95	13.350	3810	3813	3819	rBV3	1640	1492	0.04%	0.005%
96	13.405	3827	3830	3834	rBV3	1327	1009	0.03%	0.003%
97	13.595	3886	3889	3892	rBV3	1424	930	0.02%	0.003%
98	13.797	3940	3952	3959	rBV9	8646	21540	0.54%	0.071%
99	14.418	4142	4145	4149	rBV4	1999	1835	0.05%	0.006%
100	15.083	4347	4352	4353	rBV2	4681	4003	0.10%	0.013%


Sum of corrected areas: 30254242

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050219\
Data File : VU031725.D
Acq On : 02 May 2019 20:22
Operator : JC/SP
Sample : K2661-13 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B33

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

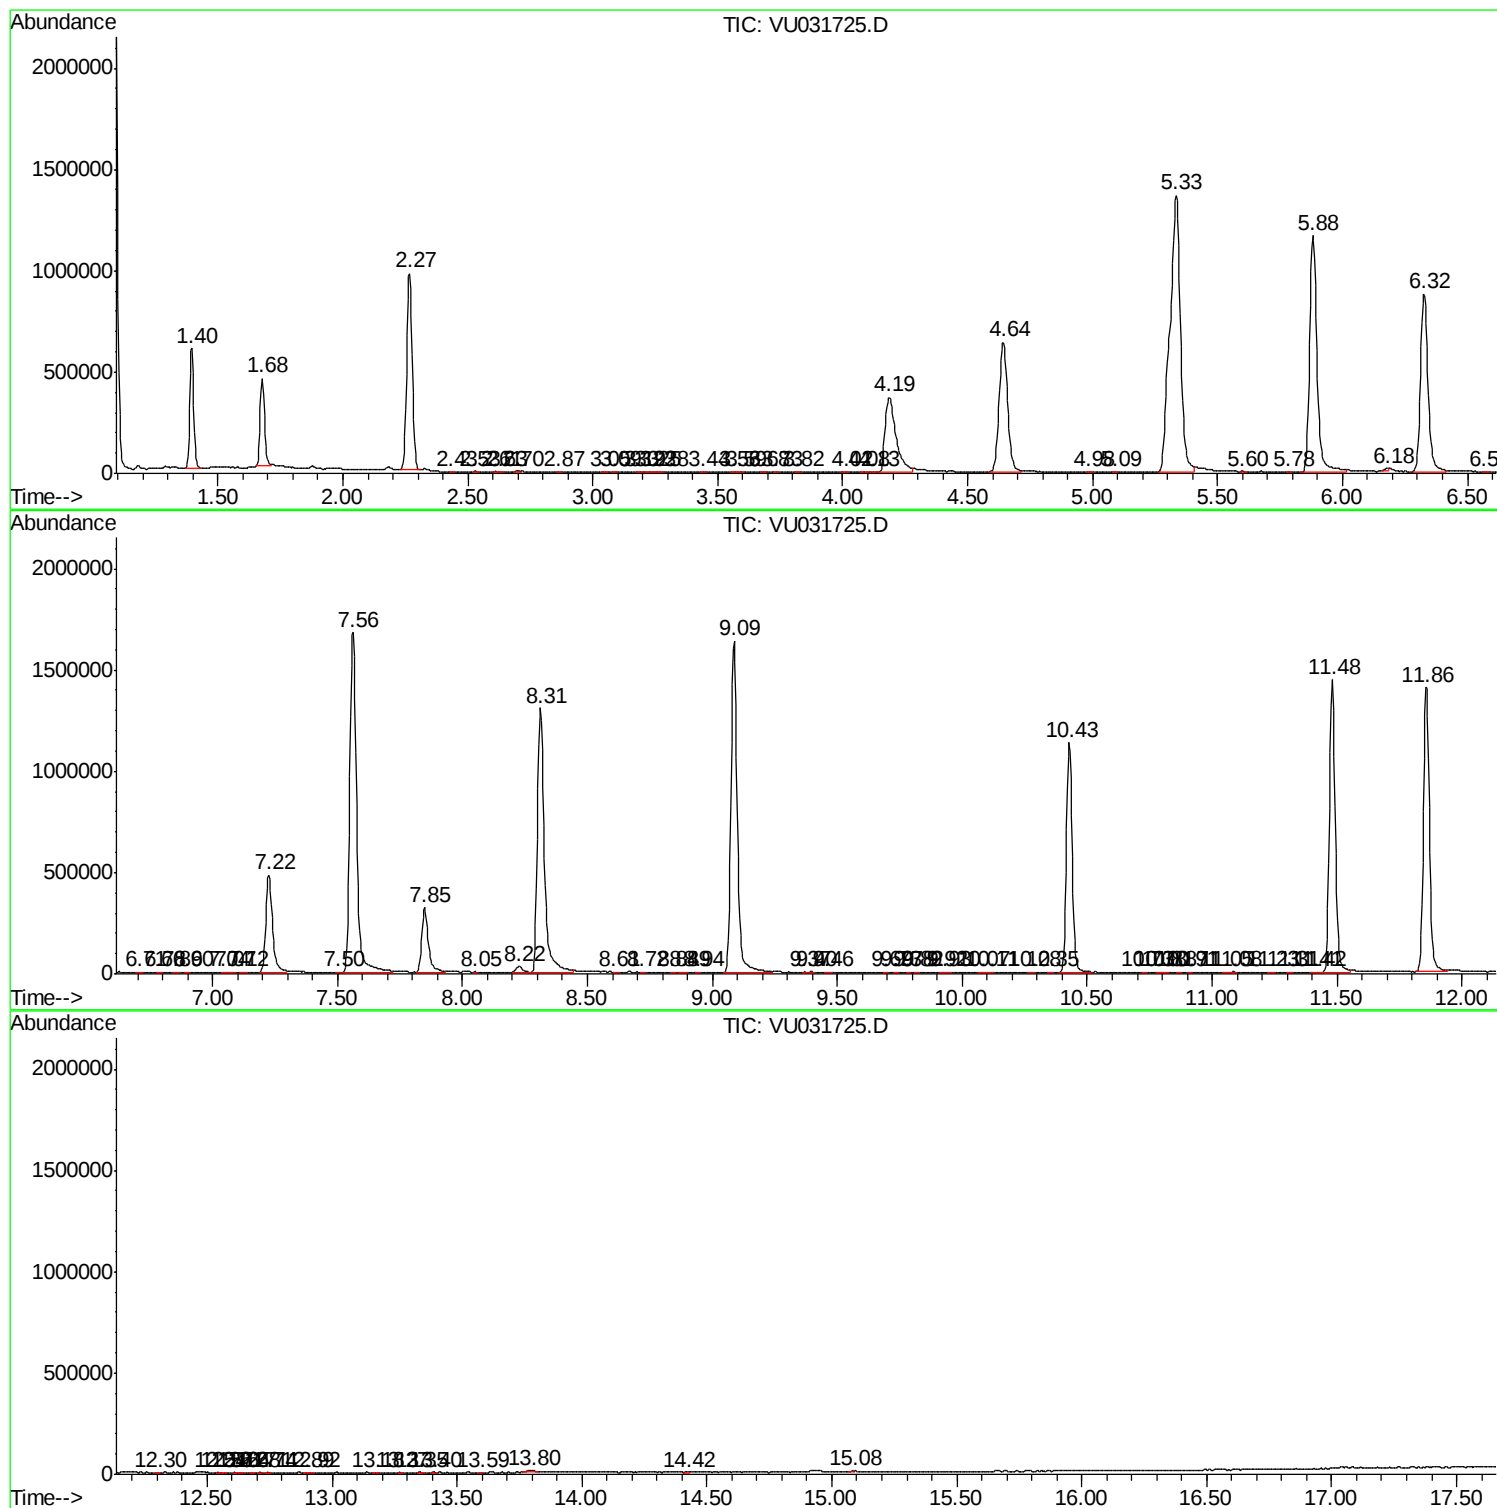

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031725.D
Acq On : 02 May 2019 20:22
Operator : JC/SP
Sample : K2661-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B33

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050219\
Data File : VU031725.D
Acq On : 02 May 2019 20:22
Operator : JC/SP
Sample : K2661-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B33

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc