


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050219\
 Data File : VU031698.D
 Acq On : 02 May 2019 09:31
 Operator : JC/SP
 Sample : BFB36
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB36

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Sat May 04 02:35:16 2019

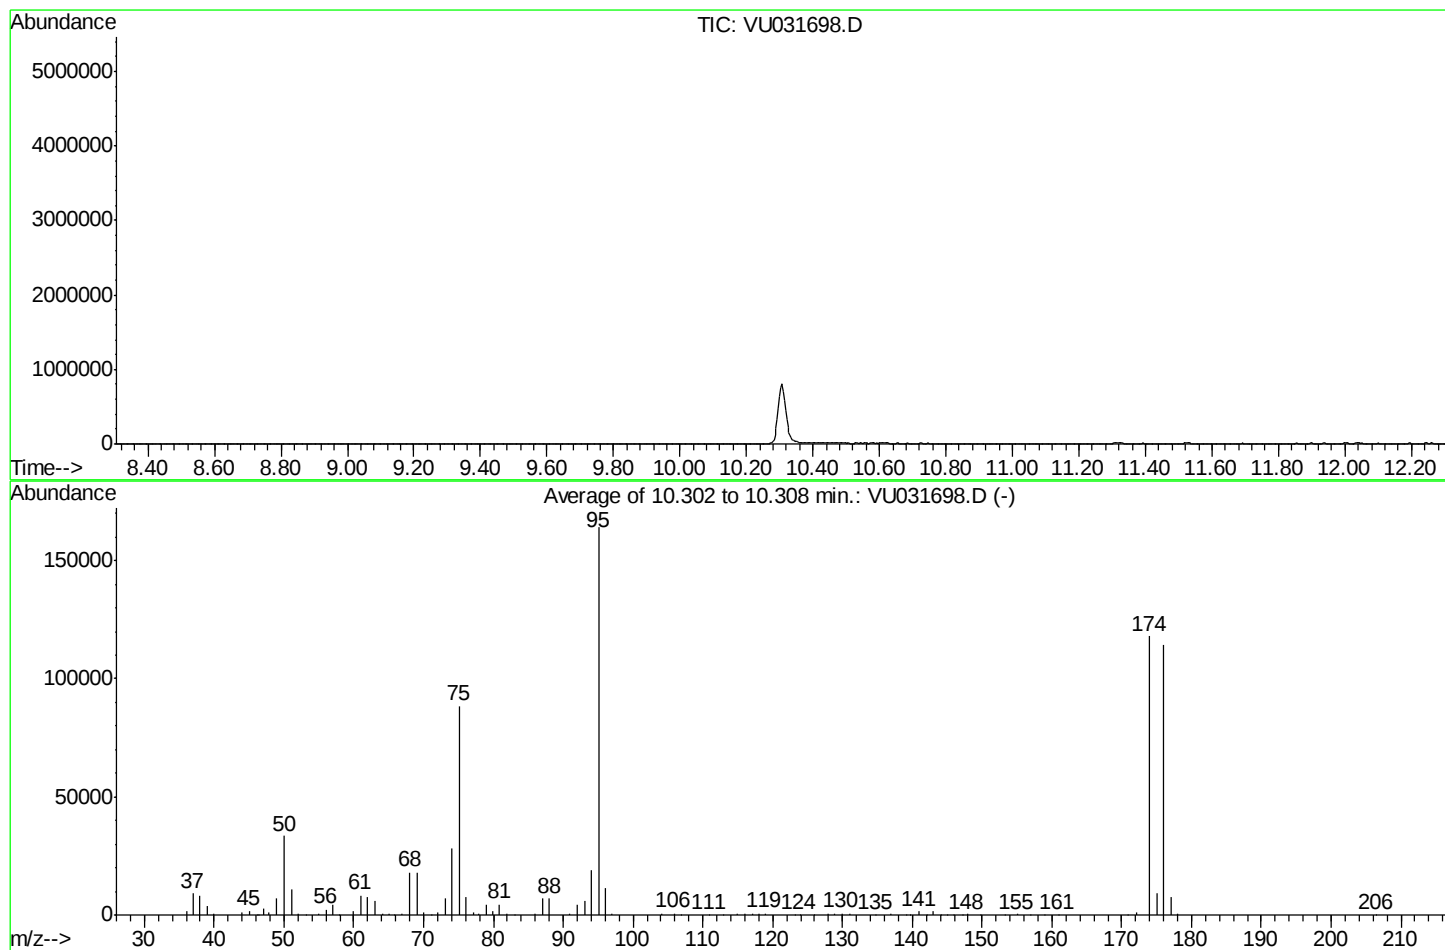

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	33442	PASS
75	95	30	80	54.0	88552	PASS
95	95	100	100	100.0	164117	PASS
96	95	5	9	6.8	11162	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.9	117946	PASS
175	174	5	9	8.0	9440	PASS
176	174	95	101	96.8	114224	PASS
177	176	5	9	6.6	7582	PASS

m/z	Abundance
36.00	124.0
40.00	5057.0
41.90	105.0
43.10	103.0
44.00	1396.0
207.20	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	1675.0
37.00	9081.0
38.00	8186.0
39.00	3561.0
40.00	5440.0
44.00	2715.0
45.00	1597.0
46.10	217.0
47.00	2250.0
47.90	928.0
49.00	7085.0
50.10	33328.0
51.10	10837.0
52.10	367.0
55.10	486.0
56.00	2343.0
57.10	4401.0
57.90	278.0
60.10	1258.0
61.00	7682.0
62.00	7662.0
63.00	6273.0
64.10	708.0
65.00	873.0
65.80	187.0
66.90	419.0
68.00	17480.0
69.00	17336.0
70.00	1270.0
71.10	148.0
71.90	973.0
73.10	6861.0
74.10	27384.0
75.10	86440.0
76.10	7184.0
77.10	1106.0
78.00	609.0
78.90	4131.0
79.90	1230.0
80.90	3979.0
81.80	872.0
83.00	213.0
86.00	422.0
87.00	6766.0
88.00	6843.0
90.90	579.0
92.00	4332.0
93.00	6252.0
94.10	18496.0
95.10	156608.0
96.10	11408.0
96.90	314.0
104.00	541.0
105.90	571.0
110.90	100.0
112.80	131.0
115.00	194.0
116.00	512.0
117.10	658.0
118.10	347.0
118.90	779.0
123.90	126.0
128.00	313.0
128.80	316.0
129.90	478.0
130.90	241.0
134.70	189.0
136.90	421.0
139.00	100.0
141.00	1426.0
143.00	1616.0
144.10	133.0
145.00	188.0
145.90	256.0
147.20	198.0
147.80	279.0
153.10	144.0
155.00	195.0
156.80	261.0
158.90	161.0
161.00	170.0
170.90	281.0
172.00	1106.0
174.00	112376.0
175.10	9264.0
176.00	108432.0
177.00	7376.0
177.90	404.0
207.10	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	1738.0
37.00	9467.0
38.00	8588.0
39.00	3767.0
40.00	5545.0
43.10	120.0
44.00	2720.0
45.00	1838.0
46.30	205.0
47.00	2540.0
47.90	882.0
49.00	7488.0
50.10	34288.0
51.00	11534.0
52.10	453.0
53.20	159.0
55.10	403.0
56.10	2233.0
57.00	4431.0
57.90	210.0
59.90	1449.0
61.00	8782.0
62.00	8007.0
63.00	6188.0
64.10	731.0
65.00	813.0
65.90	165.0
66.80	444.0
68.00	18568.0
69.00	18400.0
70.00	1422.0
71.10	189.0
72.00	1132.0
73.10	7372.0
74.10	29560.0
75.10	91712.0
76.10	7748.0
77.10	1094.0
77.90	708.0
78.90	4356.0
80.00	1525.0
80.90	4558.0
81.90	799.0
82.90	203.0
86.00	352.0
87.00	6992.0
88.00	7211.0
90.90	632.0
92.00	4608.0
93.10	6282.0
94.00	19336.0
95.10	168576.0
96.10	11477.0
96.90	389.0
104.10	564.0
105.90	654.0
106.80	140.0
110.90	153.0
112.90	123.0
115.00	333.0
116.00	488.0
117.10	818.0
118.10	437.0
118.90	852.0
123.10	139.0
123.80	116.0
125.90	113.0
127.90	369.0
128.80	433.0
129.90	682.0
131.00	318.0
134.80	165.0
136.90	366.0
141.00	1565.0
142.10	118.0
143.00	1379.0
144.10	121.0
145.10	265.0
146.00	271.0
147.10	252.0
147.90	287.0
149.80	124.0
153.10	198.0
155.00	425.0
156.90	221.0
158.90	125.0
160.90	205.0
170.90	214.0
172.00	1172.0
174.00	121872.0
175.10	9697.0
176.00	117704.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

177.00	7848.0
177.90	384.0
207.10	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

m/z	Abundance
36.00	1601.0
37.00	9025.0
38.00	8387.0
39.00	3484.0
40.00	5673.0
43.20	163.0
44.00	2607.0
45.00	1722.0
46.30	217.0
47.00	2628.0
47.80	1038.0
49.00	6960.0
50.10	32712.0
51.00	10829.0
52.10	422.0
53.20	189.0
55.00	359.0
56.10	2200.0
57.00	4307.0
57.90	142.0
59.90	1725.0
61.00	8608.0
62.00	7560.0
63.10	5851.0
64.20	697.0
65.10	788.0
66.80	395.0
68.00	18072.0
69.00	17528.0
70.00	1339.0
71.10	120.0
72.00	1111.0
73.10	7065.0
74.00	28464.0
75.10	87504.0
76.10	7592.0
77.10	917.0
77.80	708.0
78.90	4205.0
80.00	1609.0
80.90	4515.0
82.00	752.0
82.90	134.0
85.80	312.0
87.00	6804.0
88.00	6999.0
90.90	562.0
92.00	4439.0
93.10	6086.0
94.00	18624.0
95.10	167168.0
96.10	10602.0
96.90	393.0
104.10	565.0
105.90	678.0
106.90	179.0
110.90	227.0
113.00	143.0
115.00	364.0
115.90	428.0
117.10	923.0
118.10	518.0
118.90	838.0
123.10	130.0
123.80	116.0
125.80	157.0
127.90	354.0
128.90	458.0
129.90	784.0
131.10	358.0
134.80	149.0
136.80	344.0
139.10	115.0
139.60	111.0
141.00	1388.0
142.10	108.0
143.00	1203.0
145.10	283.0
146.00	316.0
147.10	302.0
147.90	304.0
149.80	217.0
153.20	217.0
155.00	591.0
157.00	221.0
158.90	115.0
160.80	163.0
172.10	1078.0
174.00	119592.0
175.00	9360.0
176.00	116536.0
177.10	7522.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36

177.90206.50

234.0100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB36