

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048362.D
 Acq On : 02 May 2022 12:00
 Operator : SY/MD
 Sample : N2638-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048362.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	51	rBV3	5523	7549	0.43%	0.056%
2	1.600	73	81	101	rBV	167596	217140	12.27%	1.611%
3	1.896	165	173	187	rBV	127853	189546	10.71%	1.407%
4	2.565	368	381	397	rBV	326320	538343	30.41%	3.995%
5	2.690	418	420	426	rVB2	305	216	0.01%	0.002%
6	2.774	434	446	469	rVB3	4855	13029	0.74%	0.097%
7	2.874	474	477	482	rBV2	412	293	0.02%	0.002%
8	2.906	482	487	488	rBV2	298	216	0.01%	0.002%
9	2.951	498	501	505	rBV2	285	220	0.01%	0.002%
10	3.047	522	531	541	rVV3	1188	2119	0.12%	0.016%
11	3.186	559	574	596	rVB	23383	57888	3.27%	0.430%
12	3.343	618	623	624	rBV	249	174	0.01%	0.001%
13	3.359	625	628	631	rVB3	524	334	0.02%	0.002%
14	3.729	739	743	746	rBV2	265	252	0.01%	0.002%
15	3.861	779	784	787	rBV3	231	198	0.01%	0.001%
16	3.906	795	798	804	rBV2	236	283	0.02%	0.002%
17	3.944	804	810	813	rVV2	212	278	0.02%	0.002%
18	3.960	813	815	819	rVV2	256	175	0.01%	0.001%
19	4.179	878	883	886	rBV2	159	179	0.01%	0.001%
20	4.298	916	920	927	rVB2	231	260	0.01%	0.002%
21	4.343	927	934	937	rBV2	276	284	0.02%	0.002%
22	4.366	937	941	946	rVB2	247	246	0.01%	0.002%
23	4.620	1007	1020	1049	rBV	192832	466956	26.38%	3.465%
24	4.845	1089	1090	1095	rVB3	333	185	0.01%	0.001%
25	5.063	1140	1158	1178	rBV	333723	740994	41.86%	5.499%
26	5.275	1220	1224	1225	rBV2	408	193	0.01%	0.001%
27	5.333	1235	1242	1251	rBV5	754	1330	0.08%	0.010%
28	5.388	1255	1259	1266	rVB2	550	446	0.03%	0.003%
29	5.726	1341	1364	1397	rBV2	659437	1770199	100.00%	13.137%
30	5.909	1419	1421	1426	rVB2	405	278	0.02%	0.002%
31	5.967	1435	1439	1449	rVB2	667	816	0.05%	0.006%
32	6.044	1457	1463	1469	rVB4	478	624	0.04%	0.005%
33	6.073	1469	1472	1476	rVB	262	162	0.01%	0.001%
34	6.111	1480	1484	1487	rBV2	502	407	0.02%	0.003%
35	6.128	1487	1489	1492	rVB2	440	286	0.02%	0.002%
36	6.150	1492	1496	1499	rVB2	307	234	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048362.D
 Acq On : 02 May 2022 12:00
 Operator : SY/MD
 Sample : N2638-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1557	rBV	452531	864590	48.84%	6.416%
38	6.539	1606	1617	1628	rVB7	2088	4079	0.23%	0.030%
39	6.587	1628	1632	1635	rBV3	378	300	0.02%	0.002%
40	6.619	1639	1642	1647	rBV2	266	185	0.01%	0.001%
41	6.690	1647	1664	1689	rBV	416437	808509	45.67%	6.000%
42	6.793	1693	1696	1697	rBV3	903	488	0.03%	0.004%
43	7.044	1770	1774	1779	rVV3	572	579	0.03%	0.004%
44	7.066	1779	1781	1786	rVV2	335	296	0.02%	0.002%
45	7.115	1790	1796	1803	rVB4	421	482	0.03%	0.004%
46	7.185	1806	1818	1829	rVV4	2935	6857	0.39%	0.051%
47	7.250	1836	1838	1841	rBV2	342	230	0.01%	0.002%
48	7.327	1858	1862	1865	rBB2	319	197	0.01%	0.001%
49	7.565	1921	1936	1955	rBV	227754	394827	22.30%	2.930%
50	7.684	1969	1973	1984	rVB3	1175	1816	0.10%	0.013%
51	7.742	1988	1991	2000	rVB3	285	321	0.02%	0.002%
52	7.793	2000	2007	2015	rBV6	1394	1938	0.11%	0.014%
53	7.899	2023	2040	2056	rBV	817497	1414861	79.93%	10.500%
54	8.179	2114	2127	2145	rBV	159061	266713	15.07%	1.979%
55	8.423	2201	2203	2207	rBV2	305	245	0.01%	0.002%
56	8.475	2207	2219	2229	rVB2	2763	5244	0.30%	0.039%
57	8.539	2236	2239	2241	rBV2	327	211	0.01%	0.002%
58	8.635	2256	2269	2302	rBV	580184	1048269	59.22%	7.779%
59	8.886	2341	2347	2350	rBV3	296	377	0.02%	0.003%
60	8.931	2354	2361	2365	rBV4	662	772	0.04%	0.006%
61	8.960	2366	2370	2372	rBV2	400	243	0.01%	0.002%
62	9.105	2410	2415	2424	rVB3	263	399	0.02%	0.003%
63	9.198	2440	2444	2447	rBV2	251	179	0.01%	0.001%
64	9.269	2462	2466	2468	rBV	340	207	0.01%	0.002%
65	9.417	2498	2512	2536	rBV	658320	1102057	62.26%	8.178%
66	9.571	2553	2560	2567	rBV	1017	1449	0.08%	0.011%
67	9.693	2591	2598	2605	rBV4	1478	2223	0.13%	0.016%
68	9.970	2680	2684	2689	rVB	328	290	0.02%	0.002%
69	10.028	2694	2702	2709	rBV2	266	357	0.02%	0.003%
70	10.108	2719	2727	2738	rVV6	1678	3185	0.18%	0.024%
71	10.172	2742	2747	2750	rBV	349	291	0.02%	0.002%
72	10.487	2838	2845	2849	rBV3	875	1032	0.06%	0.008%
73	10.603	2875	2881	2884	rBV2	245	303	0.02%	0.002%
74	10.642	2890	2893	2895	rBV2	259	164	0.01%	0.001%
75	10.671	2895	2902	2909	rVB5	1860	2536	0.14%	0.019%
76	10.758	2915	2929	2949	rBV	681749	1104684	62.40%	8.198%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048362.D
 Acq On : 02 May 2022 12:00
 Operator : SY/MD
 Sample : N2638-22
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL27

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.893	2961	2971	2981	rVB4	3461	6441	0.36%	0.048%
78	11.089	3026	3032	3036	rBV	467	613	0.03%	0.005%
79	11.153	3049	3052	3056	rBV2	288	204	0.01%	0.002%
80	11.201	3063	3067	3071	rVB2	388	271	0.02%	0.002%
81	11.246	3076	3081	3084	rVB2	314	250	0.01%	0.002%
82	11.340	3103	3110	3113	rBV2	314	321	0.02%	0.002%
83	11.414	3131	3133	3138	rVB2	551	330	0.02%	0.002%
84	11.455	3141	3146	3147	rBV	1624	1033	0.06%	0.008%
85	11.526	3162	3168	3173	rBV3	284	334	0.02%	0.002%
86	11.581	3181	3185	3187	rBV3	218	222	0.01%	0.002%
87	11.603	3190	3192	3195	rVB	282	160	0.01%	0.001%
88	11.668	3209	3212	3215	rVB2	397	284	0.02%	0.002%
89	11.696	3215	3221	3228	rBV4	958	1258	0.07%	0.009%
90	11.748	3233	3237	3245	rVB4	1353	1572	0.09%	0.012%
91	11.812	3245	3257	3280	rBV	663735	1050387	59.34%	7.795%
92	11.970	3304	3306	3313	rVB5	1639	1509	0.09%	0.011%
93	12.018	3317	3321	3325	rBV2	372	335	0.02%	0.002%
94	12.195	3360	3376	3397	rBV	811608	1337565	75.56%	9.926%
95	12.359	3425	3427	3431	rVB2	583	314	0.02%	0.002%
96	12.774	3548	3556	3564	rBV3	2689	3906	0.22%	0.029%
97	13.233	3690	3699	3706	rVB4	1437	2207	0.12%	0.016%
98	13.847	3885	3890	3899	rVB6	1782	2355	0.13%	0.017%
99	14.095	3959	3967	3976	rBV2	3377	5421	0.31%	0.040%
100	14.336	4037	4042	4051	rVB3	2378	3466	0.20%	0.026%




Sum of corrected areas: 13475075

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
Data File : VU048362.D
Acq On : 02 May 2022 12:00
Operator : SY/MD
Sample : N2638-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

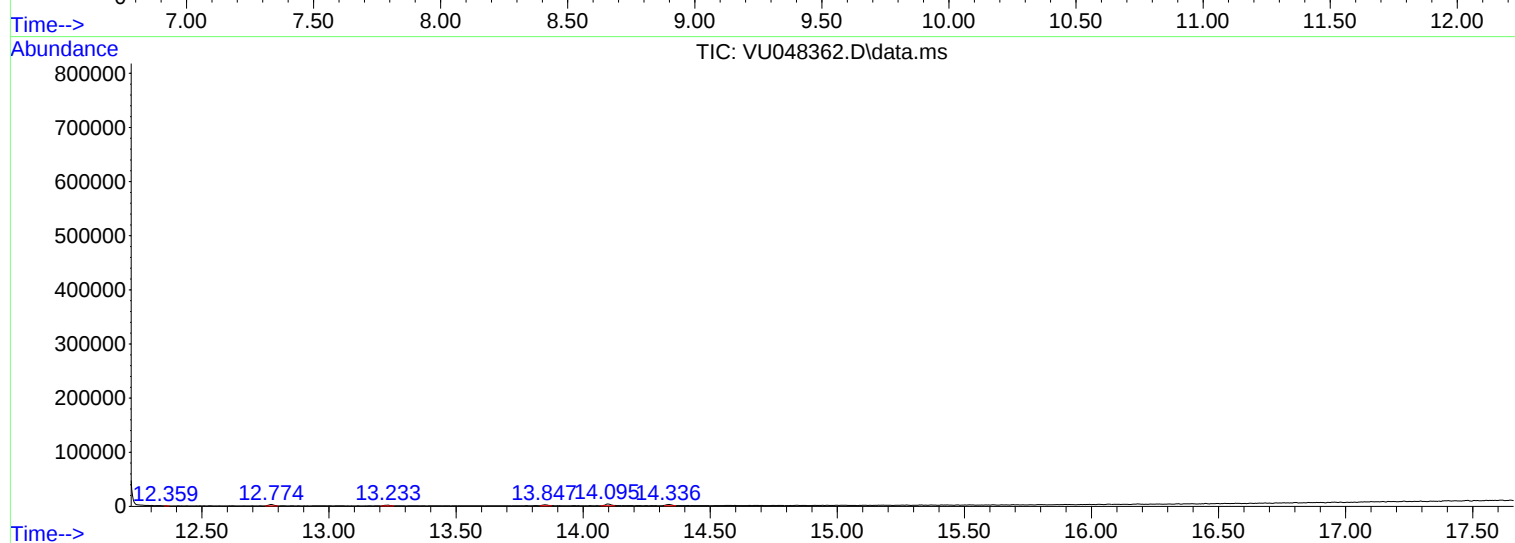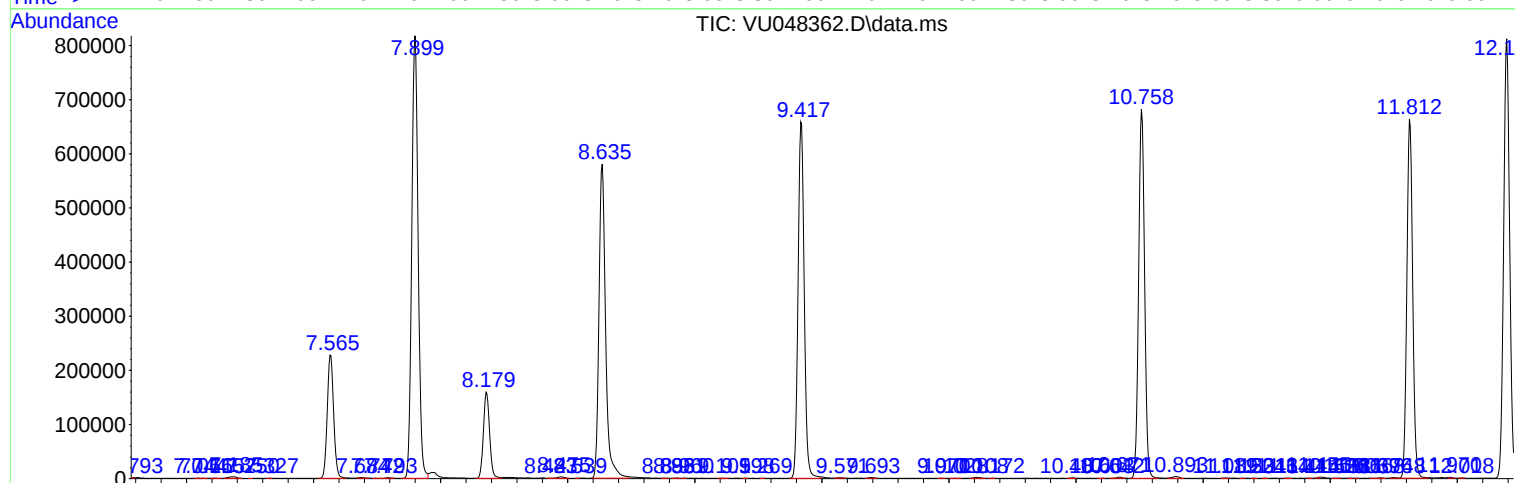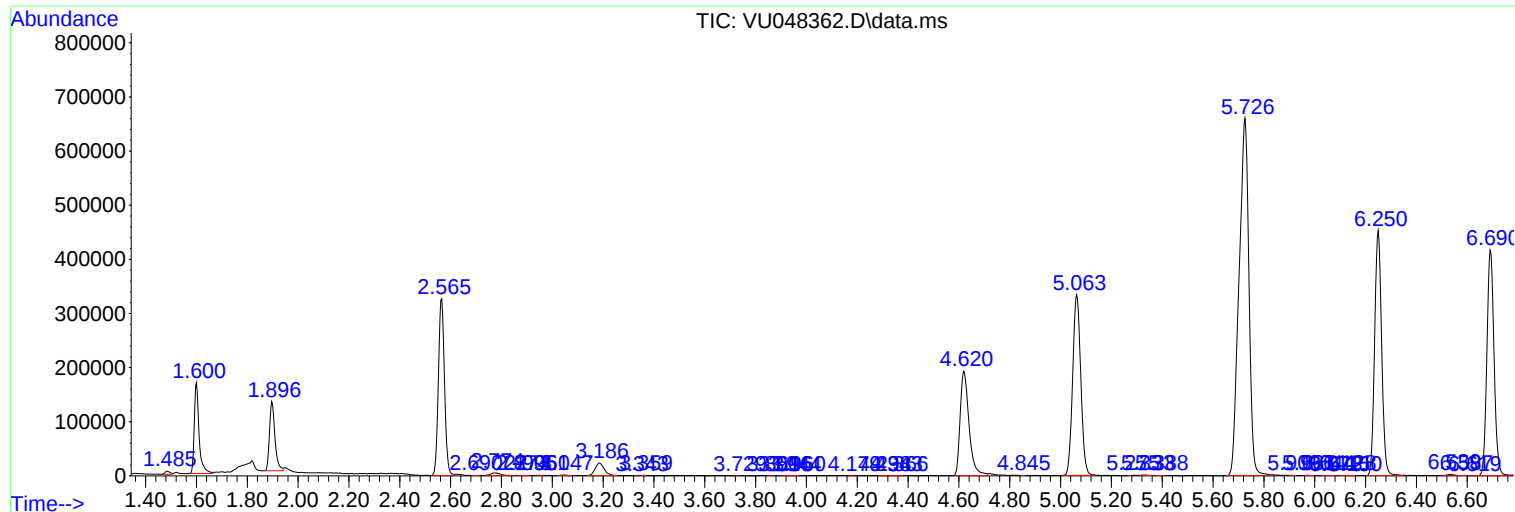

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
Data File : VU048362.D
Acq On : 02 May 2022 12:00
Operator : SY/MD
Sample : N2638-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
Data File : VU048362.D
Acq On : 02 May 2022 12:00
Operator : SY/MD
Sample : N2638-22
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL27

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc