

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048363.D
 Acq On : 02 May 2022 12:24
 Operator : SY/MD
 Sample : N2639-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	99	rBV	160372	200487	11.85%	1.565%
2	1.896	165	173	187	rBV	122354	178527	10.55%	1.393%
3	2.565	368	381	395	rBV	310547	504482	29.82%	3.938%
4	2.697	419	422	425	rVB2	395	282	0.02%	0.002%
5	2.774	432	446	464	rBV2	7840	19925	1.18%	0.156%
6	2.851	468	470	474	rVB2	202	122	0.01%	0.001%
7	3.034	524	527	528	rBV	483	293	0.02%	0.002%
8	3.128	553	556	558	rBV2	166	150	0.01%	0.001%
9	3.186	559	574	595	rVV	29928	74177	4.38%	0.579%
10	3.350	622	625	627	rVV	235	158	0.01%	0.001%
11	3.366	627	630	635	rVB2	253	224	0.01%	0.002%
12	3.433	648	651	654	rVB	256	146	0.01%	0.001%
13	3.526	677	680	685	rVB3	442	379	0.02%	0.003%
14	3.552	685	688	692	rBV	249	301	0.02%	0.002%
15	3.681	724	728	730	rBV2	148	120	0.01%	0.001%
16	3.797	762	764	769	rBV	118	120	0.01%	0.001%
17	3.896	791	795	798	rBV2	419	392	0.02%	0.003%
18	4.025	832	835	837	rVV	247	171	0.01%	0.001%
19	4.134	867	869	877	rBV2	244	360	0.02%	0.003%
20	4.202	887	890	894	rVV2	204	136	0.01%	0.001%
21	4.382	944	946	949	rVB	256	154	0.01%	0.001%
22	4.414	949	956	958	rBV	293	323	0.02%	0.003%
23	4.430	958	961	966	rBV2	129	143	0.01%	0.001%
24	4.565	999	1003	1005	rBV	192	155	0.01%	0.001%
25	4.620	1005	1020	1063	rVV	195191	477937	28.25%	3.730%
26	5.063	1141	1158	1181	rBV	325190	718217	42.46%	5.606%
27	5.221	1203	1207	1210	rBV2	378	359	0.02%	0.003%
28	5.292	1226	1229	1233	rBV2	239	196	0.01%	0.002%
29	5.468	1279	1284	1287	rBV2	156	169	0.01%	0.001%
30	5.485	1287	1289	1294	rVB2	143	137	0.01%	0.001%
31	5.726	1341	1364	1389	rBV2	625771	1691649	100.00%	13.204%
32	5.896	1415	1417	1421	rVB2	266	188	0.01%	0.001%
33	5.925	1424	1426	1429	rBV2	248	127	0.01%	0.001%
34	5.967	1437	1439	1442	rBV4	300	182	0.01%	0.001%
35	6.034	1458	1460	1461	rBV2	370	176	0.01%	0.001%
36	6.092	1474	1478	1480	rBV	188	140	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048363.D
 Acq On : 02 May 2022 12:24
 Operator : SY/MD
 Sample : N2639-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.112	1481	1484	1487	rBV3	259	214	0.01%	0.002%
38	6.250	1512	1527	1553	rBV	425413	808286	47.78%	6.309%
39	6.526	1605	1613	1628	rBV7	1619	3375	0.20%	0.026%
40	6.591	1628	1633	1636	rBV3	566	515	0.03%	0.004%
41	6.690	1649	1664	1686	rBV	395730	773293	45.71%	6.036%
42	6.774	1688	1690	1693	rVB2	512	207	0.01%	0.002%
43	6.806	1695	1700	1701	rBV	948	743	0.04%	0.006%
44	6.954	1743	1746	1747	rBV	245	123	0.01%	0.001%
45	6.989	1753	1757	1762	rVV3	275	304	0.02%	0.002%
46	7.185	1804	1818	1830	rBV6	3041	6927	0.41%	0.054%
47	7.288	1848	1850	1854	rBV	200	116	0.01%	0.001%
48	7.452	1896	1901	1906	rBV2	174	266	0.02%	0.002%
49	7.565	1922	1936	1959	rBV	215272	372609	22.03%	2.908%
50	7.687	1967	1974	1980	rBV5	1551	1900	0.11%	0.015%
51	7.783	2002	2004	2005	rBV	325	159	0.01%	0.001%
52	7.899	2026	2040	2056	rBV	769365	1334123	78.87%	10.413%
53	8.128	2108	2111	2114	rBV	319	216	0.01%	0.002%
54	8.179	2115	2127	2149	rBV2	150898	253853	15.01%	1.981%
55	8.472	2213	2218	2227	rVB5	1764	2844	0.17%	0.022%
56	8.507	2227	2229	2232	rBV2	244	186	0.01%	0.001%
57	8.552	2241	2243	2246	rBV2	296	162	0.01%	0.001%
58	8.571	2246	2249	2255	rBV4	262	224	0.01%	0.002%
59	8.636	2255	2269	2305	rBV	581541	1068228	63.15%	8.338%
60	8.835	2328	2331	2336	rBV3	480	379	0.02%	0.003%
61	8.906	2349	2353	2357	rBV2	589	432	0.03%	0.003%
62	8.957	2367	2369	2371	rBV	385	187	0.01%	0.001%
63	9.021	2387	2389	2394	rVB2	255	229	0.01%	0.002%
64	9.047	2394	2397	2399	rBV	269	154	0.01%	0.001%
65	9.066	2399	2403	2404	rBV2	229	150	0.01%	0.001%
66	9.121	2417	2420	2421	rBV2	324	165	0.01%	0.001%
67	9.131	2421	2423	2426	rVB	357	169	0.01%	0.001%
68	9.153	2426	2430	2432	rBV2	723	556	0.03%	0.004%
69	9.417	2499	2512	2542	rBV	611074	1023886	60.53%	7.992%
70	9.558	2555	2556	2560	rBV2	281	206	0.01%	0.002%
71	9.636	2577	2580	2585	rBV2	281	316	0.02%	0.002%
72	9.684	2591	2595	2597	rBV2	671	621	0.04%	0.005%
73	9.938	2672	2674	2679	rBV3	180	168	0.01%	0.001%
74	10.005	2690	2695	2699	rBV2	311	348	0.02%	0.003%
75	10.057	2707	2711	2713	rBV	247	212	0.01%	0.002%
76	10.099	2720	2724	2726	rBV2	421	291	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048363.D
 Acq On : 02 May 2022 12:24
 Operator : SY/MD
 Sample : N2639-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.144	2734	2738	2742	rBV2	244	272	0.02%	0.002%
78	10.279	2778	2780	2784	rBV2	193	126	0.01%	0.001%
79	10.455	2832	2835	2840	rBV2	228	208	0.01%	0.002%
80	10.671	2895	2902	2911	rVV4	1668	2349	0.14%	0.018%
81	10.758	2915	2929	2948	rBV	677720	1077380	63.69%	8.409%
82	10.867	2957	2963	2964	rBV2	668	579	0.03%	0.005%
83	10.893	2964	2971	2980	rVB4	2952	4336	0.26%	0.034%
84	11.086	3029	3031	3037	rBV3	276	249	0.01%	0.002%
85	11.259	3080	3085	3088	rBV	269	365	0.02%	0.003%
86	11.410	3129	3132	3135	rVB3	497	346	0.02%	0.003%
87	11.462	3139	3148	3158	rVB5	1429	2582	0.15%	0.020%
88	11.742	3232	3235	3236	rBV	377	192	0.01%	0.001%
89	11.812	3244	3257	3276	rBV	593434	942774	55.73%	7.359%
90	12.021	3320	3322	3323	rBV	316	144	0.01%	0.001%
91	12.195	3357	3376	3396	rBV	761888	1242439	73.45%	9.697%
92	12.401	3435	3440	3441	rBV	383	290	0.02%	0.002%
93	12.504	3467	3472	3474	rBV2	288	303	0.02%	0.002%
94	12.632	3508	3512	3514	rBV	470	355	0.02%	0.003%
95	12.774	3546	3556	3565	rBV4	2194	3802	0.22%	0.030%
96	13.118	3659	3663	3670	rBV2	459	590	0.03%	0.005%
97	13.230	3694	3698	3700	rBV2	541	443	0.03%	0.003%
98	13.854	3884	3892	3898	rBV4	820	1458	0.09%	0.011%
99	14.102	3963	3969	3974	rVB3	1067	1303	0.08%	0.010%
100	14.323	4035	4038	4040	rBV	800	593	0.04%	0.005%




Sum of corrected areas: 12812024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
Data File : VU048363.D
Acq On : 02 May 2022 12:24
Operator : SY/MD
Sample : N2639-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

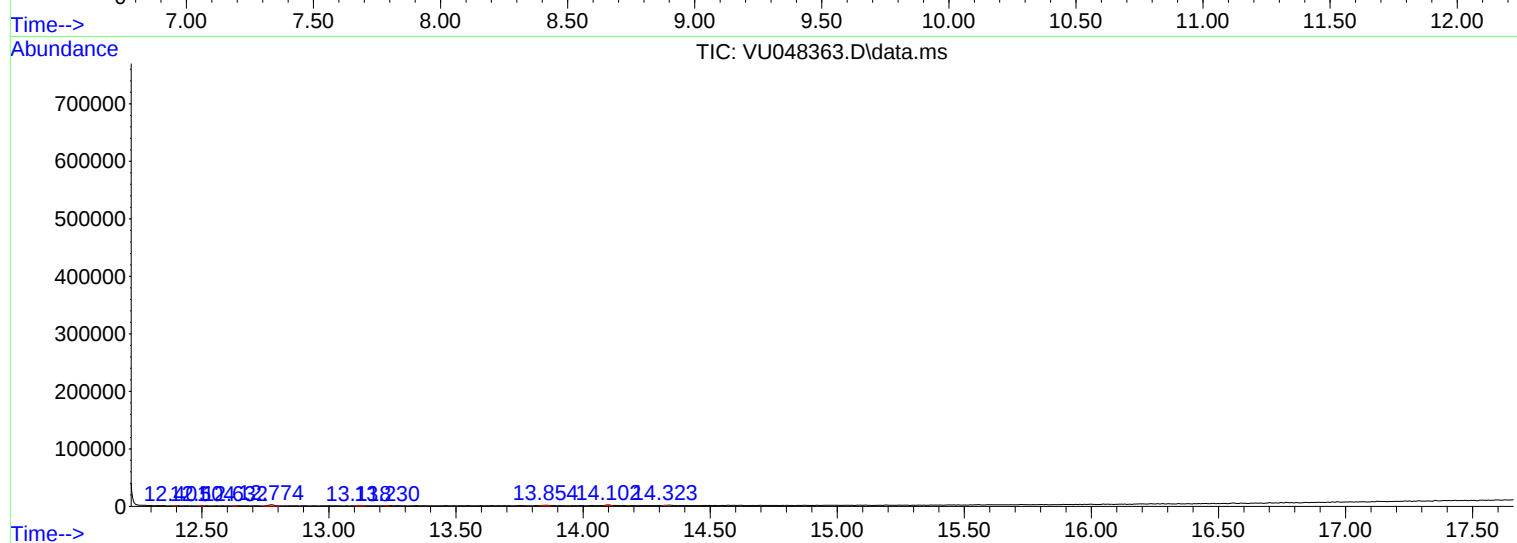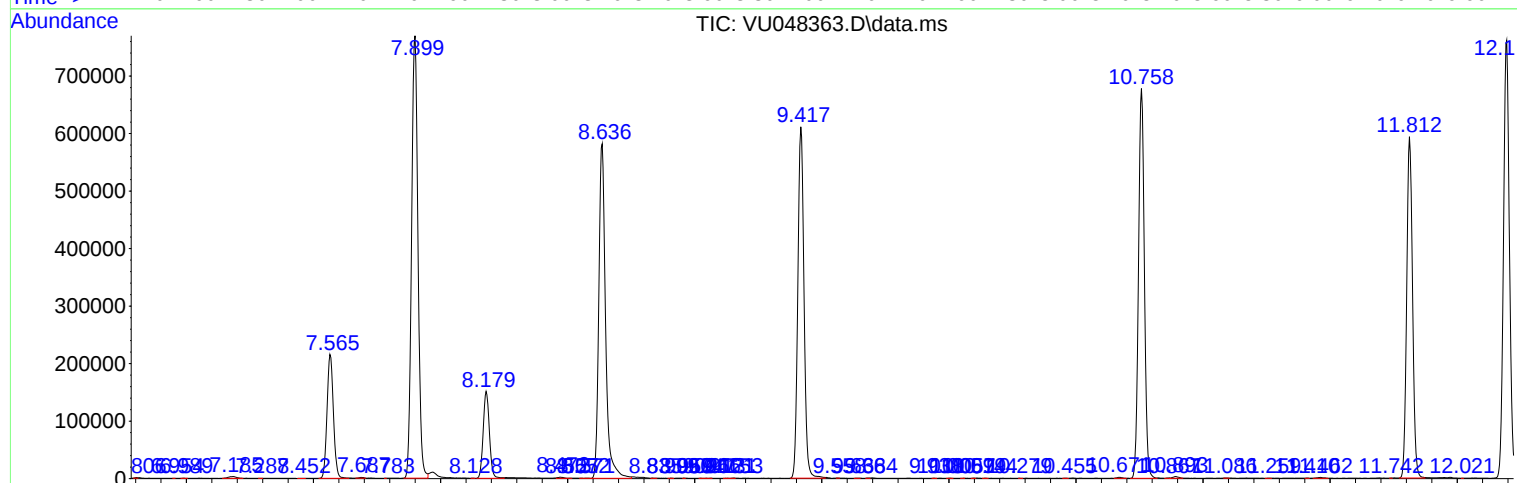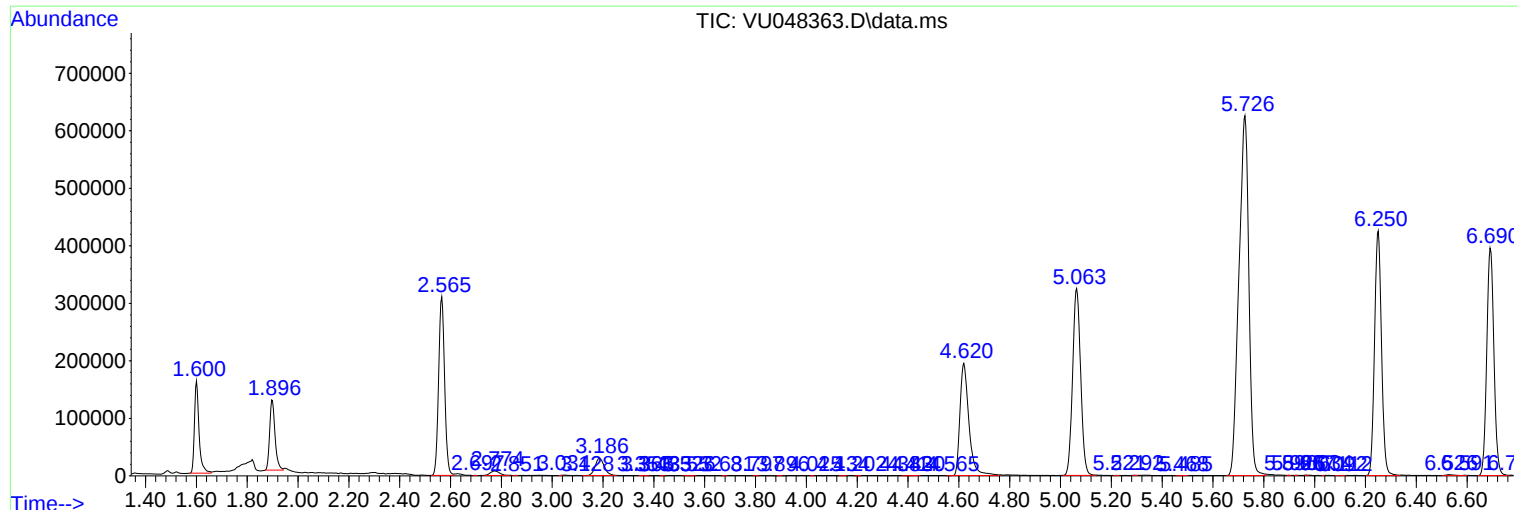

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
Data File : VU048363.D
Acq On : 02 May 2022 12:24
Operator : SY/MD
Sample : N2639-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
Data File : VU048363.D
Acq On : 02 May 2022 12:24
Operator : SY/MD
Sample : N2639-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------