


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050222\
 Data File : VU048358.D
 Acq On : 02 May 2022 09:14
 Operator : SY/MD
 Sample : BFB077
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB077

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Wed May 04 01:37:47 2022

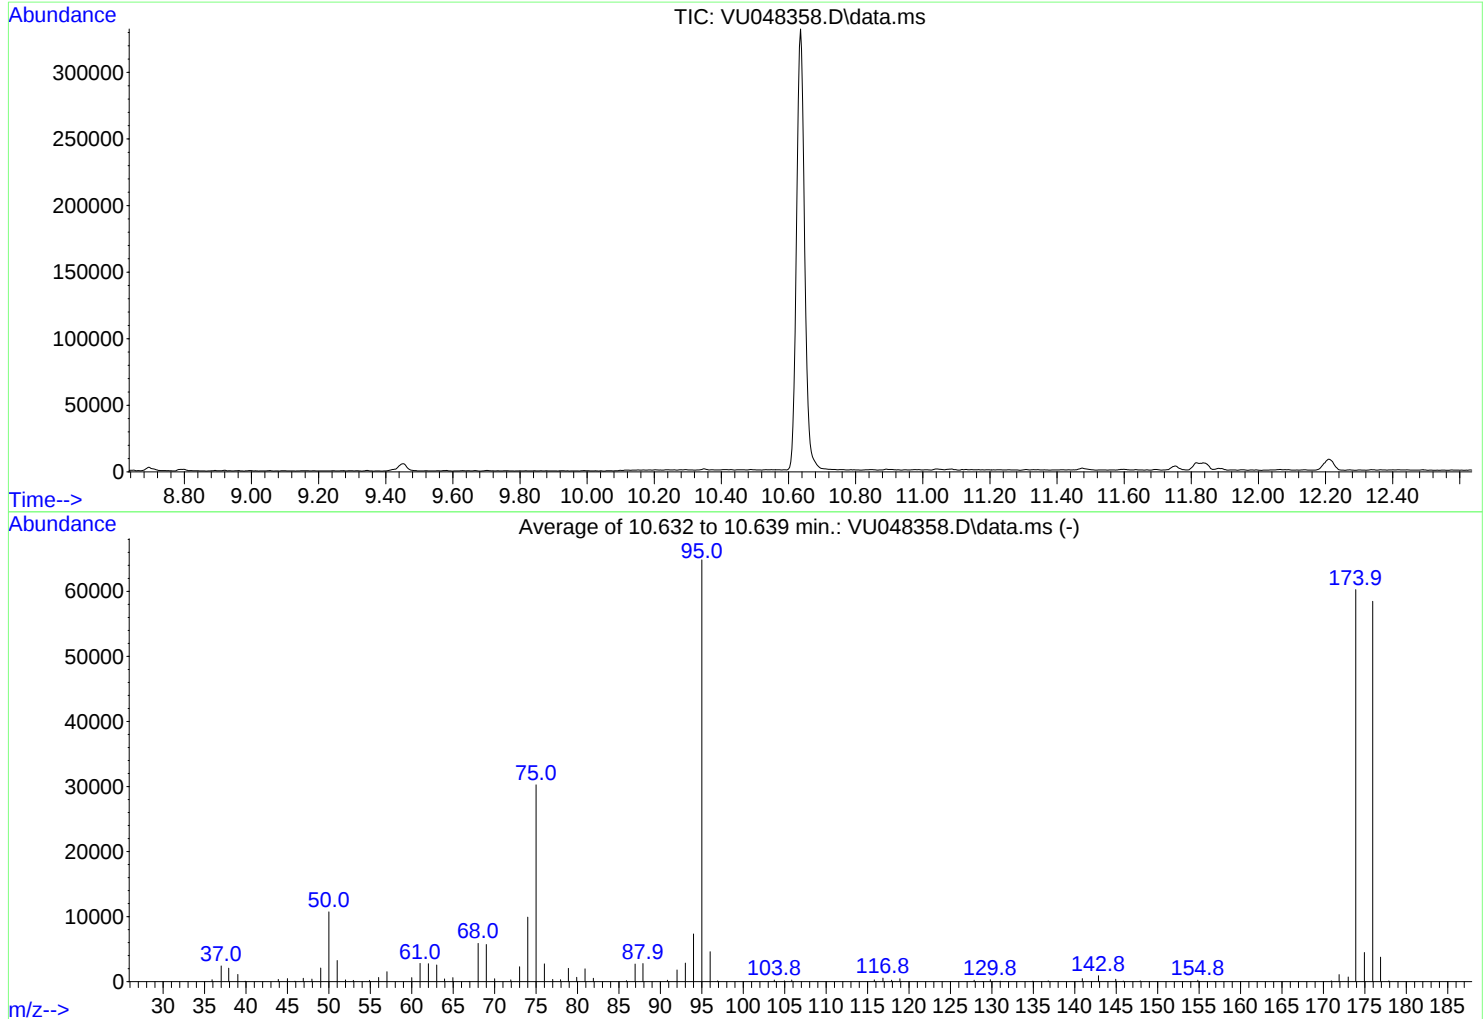

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	10717	PASS
75	95	30	80	46.6	30251	PASS
95	95	100	100	100.0	64851	PASS
96	95	5	9	7.1	4599	PASS
173	174	0.00	2	1.2	715	PASS
174	95	50	120	92.9	60264	PASS
175	174	5	9	7.4	4476	PASS
176	174	95	101	97.0	58480	PASS
177	176	5	9	6.4	3771	PASS

m/z	Abundance
35.90	571.0
37.90	215.0
39.90	365.0
43.90	302.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077

m/z	Abundance
35.90	852.0
37.00	2343.0
38.00	2308.0
39.00	1099.0
39.90	444.0
43.90	674.0
45.00	440.0
45.90	104.0
46.90	479.0
48.00	363.0
49.00	2157.0
50.00	10924.0
51.00	3223.0
52.00	285.0
52.90	171.0
54.90	189.0
56.00	636.0
57.00	1448.0
60.00	651.0
61.00	2926.0
62.00	2756.0
63.00	2492.0
63.90	336.0
65.00	622.0
66.90	137.0
68.00	5840.0
69.00	5688.0
70.00	447.0
72.00	276.0
73.00	2412.0
74.00	9736.0
75.00	30328.0
76.00	2682.0
77.00	373.0
78.00	282.0
78.90	2047.0
79.90	719.0
80.90	1997.0
81.90	550.0
85.90	141.0
86.90	2669.0
87.90	2635.0
90.80	216.0
92.00	1764.0
93.00	2852.0
94.00	7241.0
95.00	64192.0
96.00	4743.0
96.90	135.0
103.70	240.0
104.90	108.0
105.90	246.0
115.80	246.0
116.80	509.0
117.90	227.0
118.90	509.0
127.90	218.0
129.80	308.0
131.00	104.0
136.80	122.0
140.90	398.0
142.90	823.0
145.00	395.0
145.90	110.0
147.90	103.0
154.90	216.0
171.00	135.0
171.90	1120.0
173.00	771.0
173.90	59528.0
174.90	4562.0
176.00	56176.0
176.90	3796.0
177.90	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077

m/z	Abundance
35.90	843.0
37.00	2473.0
37.90	2332.0
39.00	1147.0
39.90	428.0
43.90	668.0
45.00	488.0
45.90	114.0
46.90	528.0
48.00	404.0
49.00	2140.0
50.00	11050.0
51.00	3357.0
52.00	285.0
52.90	198.0
54.90	198.0
56.00	648.0
57.00	1588.0
60.00	653.0
61.00	2892.0
62.00	2834.0
63.00	2634.0
64.00	406.0
64.90	635.0
68.00	6059.0
69.00	5854.0
70.00	441.0
71.90	278.0
73.00	2332.0
74.00	10224.0
75.00	31288.0
76.00	2824.0
77.00	340.0
77.90	311.0
78.90	2109.0
79.90	684.0
80.90	2017.0
81.90	529.0
85.90	141.0
86.90	2755.0
87.90	2870.0
90.90	239.0
92.00	1879.0
93.00	2944.0
94.00	7548.0
95.00	66960.0
96.00	4715.0
96.90	131.0
103.80	270.0
105.00	127.0
105.80	262.0
115.80	276.0
116.80	570.0
117.90	241.0
118.90	459.0
127.90	230.0
129.80	290.0
131.00	112.0
134.90	112.0
136.80	125.0
140.90	469.0
142.00	100.0
142.90	934.0
145.00	391.0
145.80	112.0
147.90	125.0
154.90	229.0
171.00	132.0
171.90	1128.0
173.00	723.0
173.90	61944.0
174.90	4610.0
175.90	60200.0
176.90	3847.0
177.90	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077

m/z	Abundance
36.00	876.0
37.00	2391.0
38.00	2214.0
39.00	1089.0
39.90	418.0
43.90	627.0
45.00	495.0
46.90	569.0
47.90	401.0
49.00	2017.0
50.00	10176.0
51.00	3158.0
52.00	228.0
53.00	195.0
54.90	197.0
56.00	629.0
57.00	1564.0
60.00	561.0
61.00	2584.0
62.00	2691.0
63.00	2579.0
64.00	481.0
64.90	584.0
68.00	5772.0
69.00	5590.0
70.00	418.0
71.90	283.0
73.00	2141.0
74.00	9801.0
75.00	29136.0
76.00	2715.0
77.00	324.0
78.00	305.0
78.90	1971.0
79.90	624.0
80.90	1876.0
81.90	514.0
85.90	144.0
87.00	2706.0
87.90	2839.0
90.90	247.0
92.00	1786.0
93.00	2793.0
94.00	7178.0
95.00	63400.0
96.00	4339.0
96.90	102.0
103.80	261.0
104.90	128.0
105.80	221.0
115.80	268.0
116.90	552.0
117.90	222.0
118.90	369.0
127.80	204.0
128.90	112.0
129.80	265.0
135.00	140.0
136.80	118.0
140.90	564.0
142.80	972.0
144.90	361.0
145.80	103.0
147.90	128.0
154.80	191.0
156.90	109.0
170.90	138.0
171.90	1023.0
173.00	650.0
173.90	59320.0
175.00	4256.0
175.90	59064.0
176.90	3671.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB077