

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
 Data File : VU054044.D
 Acq On : 02 May 2023 10:53
 Operator : JC/MD
 Sample : VU0502WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK086

Quant Time: May 03 05:20:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 03 05:19:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.243	114	258873	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.410	117	246595	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	119586	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	81434	41.593	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.180%		
7) Chloroethane-d5	1.909	69	56190	43.721	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.440%		
11) 1,1-Dichloroethene-d2	2.562	63	113062	32.558	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.120%		
21) 2-Butanone-d5	4.620	46	108296	96.983	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	96.980%		
24) Chloroform-d	5.057	84	157499	43.800	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.600%		
26) 1,2-Dichloroethane-d4	5.694	65	105374	45.640	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.280%		
32) Benzene-d6	5.719	84	312093	42.997	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.000%		
36) 1,2-Dichloropropane-d6	6.684	67	100848	44.011	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.020%		
41) Toluene-d8	7.893	98	276471	42.189	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.380%		
43) trans-1,3-Dichloroprop...	8.173	79	48366	42.651	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.300%		
47) 2-Hexanone-d5	8.629	63	70214	85.550	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	85.550%		
56) 1,1,2,2-Tetrachloroeth...	10.751	84	136380	45.184	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.360%		
66) 1,2-Dichlorobenzene-d4	12.188	152	112161	48.011	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.020%		
Target Compounds					Qvalue	
12) 1,1-Dichloroethene	2.562	96	893	0.595	ug/L #	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
Data File : VU054044.D
Acq On : 02 May 2023 10:53
Operator : JC/MD
Sample : VU0502WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK086

Quant Time: May 03 05:20:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 03 05:19:13 2023
Response via : Initial Calibration

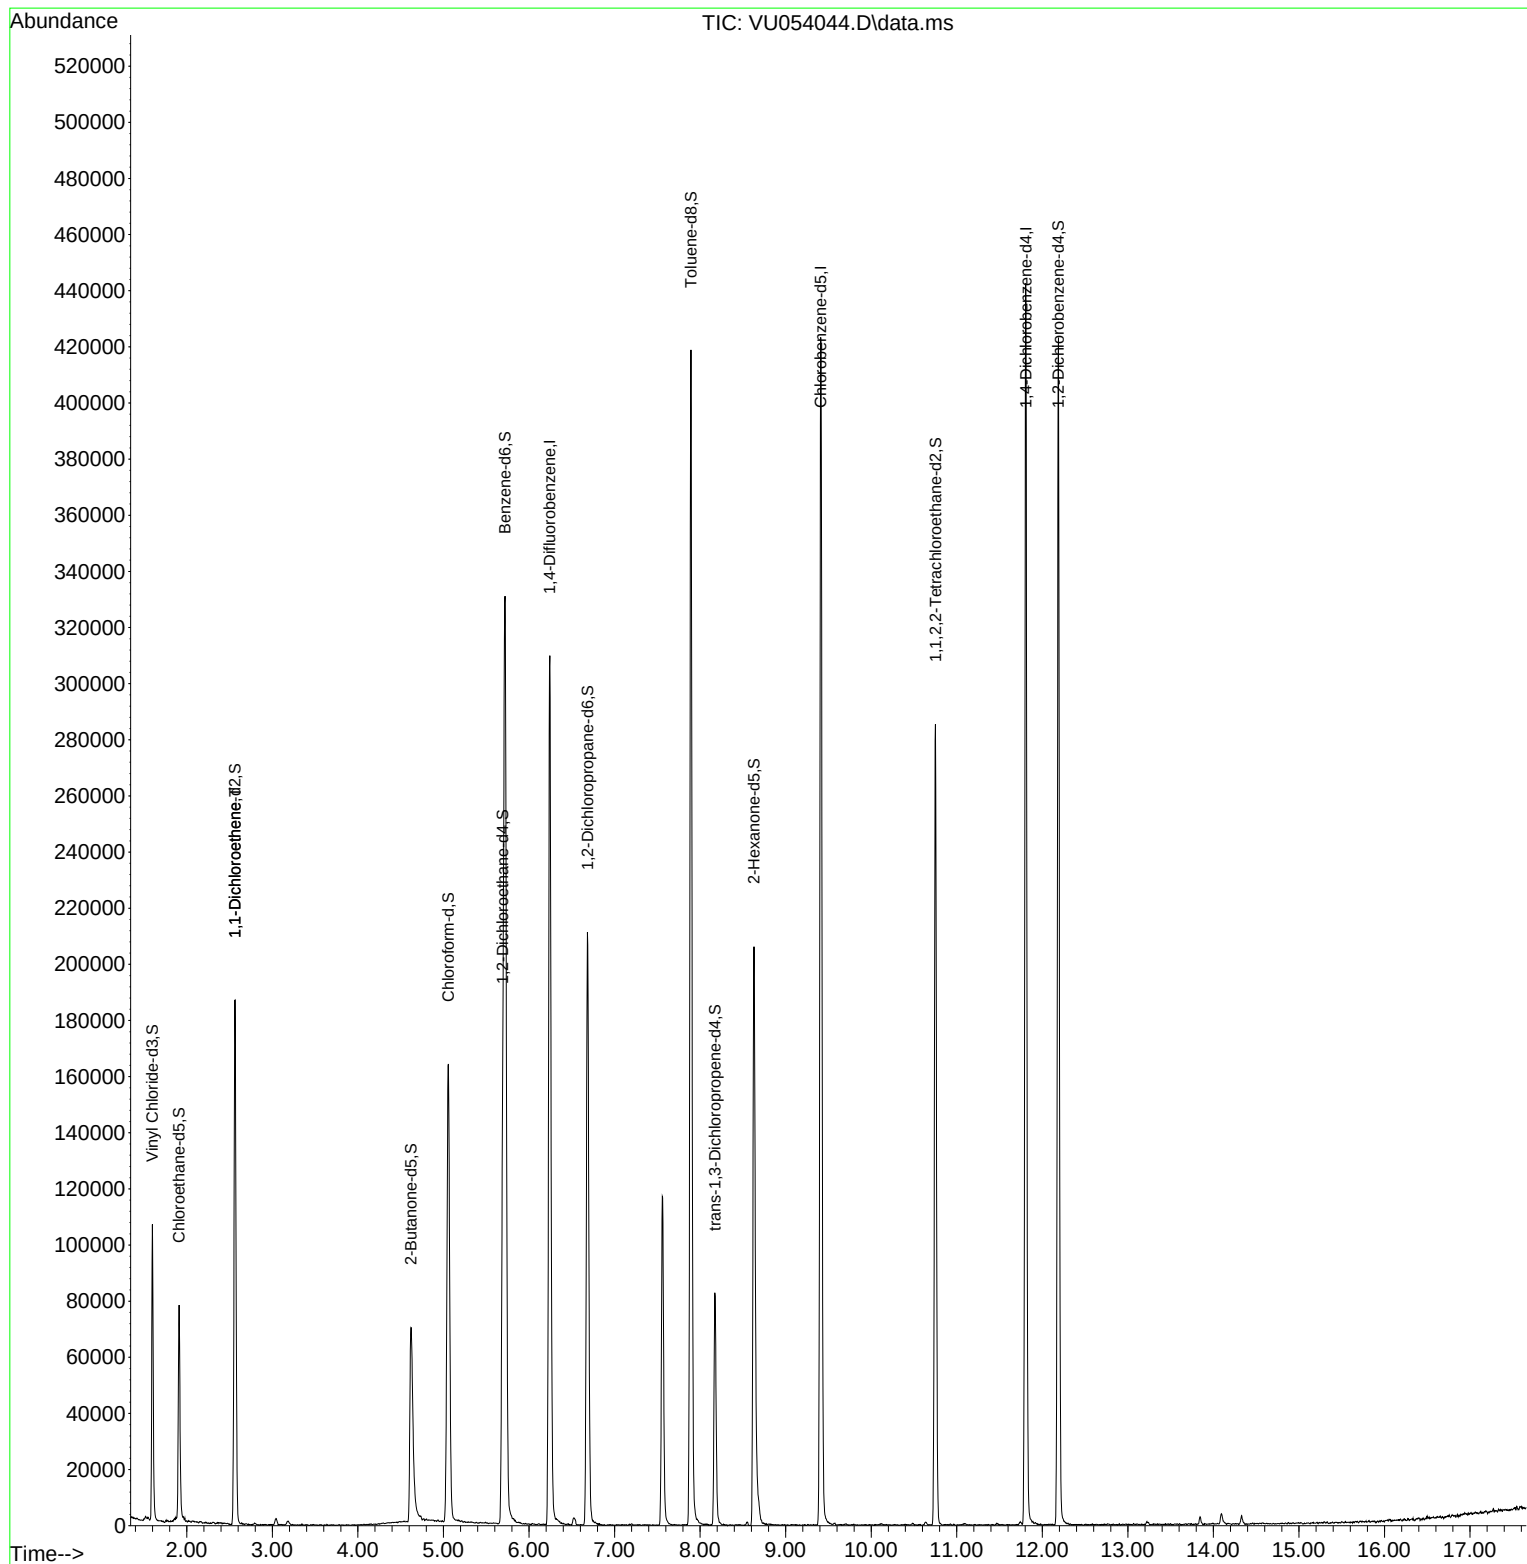

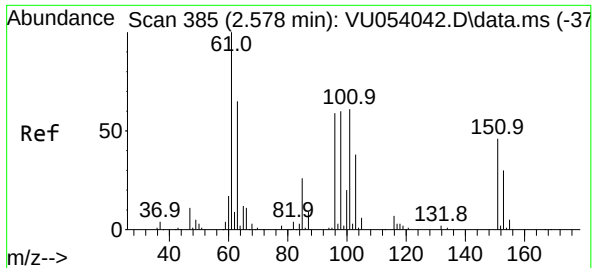

#12
 1,1-Dichloroethene
 Concen: 0.595 ug/L
 RT: 2.562 min Scan# 380
 Delta R.T. -0.016 min
 Lab File: VU054044.D
 Acq: 02 May 2023 10:53

Instrument : MSVOA_U
 ClientSampleId : VBLK086

Tgt Ion: 96 Resp: 893

Ion	Ratio	Lower	Upper
96	100		
61	1542.8	118.3	219.7#
63	13277.8	92.3	171.5#

