

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
 Data File : VU054045.D
 Acq On : 02 May 2023 12:35
 Operator : JC/MD
 Sample : 02565-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

Signal : TIC: VU054045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rVB	106888	124303	12.33%	1.491%
2	1.912	170	178	194	rVB	87826	117545	11.66%	1.410%
3	2.565	369	381	397	rBV	196285	320526	31.78%	3.844%
4	2.932	493	495	497	rBV2	189	131	0.01%	0.002%
5	3.031	522	526	527	rBV	754	444	0.04%	0.005%
6	3.176	566	571	585	rVB3	725	1482	0.15%	0.018%
7	3.305	608	611	612	rBV3	219	105	0.01%	0.001%
8	3.391	634	638	640	rBV	200	169	0.02%	0.002%
9	3.587	696	699	703	rVB2	212	168	0.02%	0.002%
10	3.623	708	710	712	rBV	282	84	0.01%	0.001%
11	3.678	725	727	728	rBV	126	52	0.01%	0.001%
12	3.719	736	740	742	rBV2	172	141	0.01%	0.002%
13	3.793	760	763	766	rBV	354	253	0.03%	0.003%
14	3.825	769	773	776	rVB2	316	238	0.02%	0.003%
15	3.848	777	780	783	rBV2	345	309	0.03%	0.004%
16	3.932	803	806	810	rBV	190	183	0.02%	0.002%
17	4.086	853	854	855	rBV	113	29	0.00%	0.000%
18	4.169	877	880	883	rBV	212	147	0.01%	0.002%
19	4.279	911	914	917	rBV	110	107	0.01%	0.001%
20	4.330	929	930	933	rBV	212	114	0.01%	0.001%
21	4.388	946	948	950	rVB	181	73	0.01%	0.001%
22	4.407	950	954	959	rBV2	255	205	0.02%	0.002%
23	4.446	963	966	968	rBV	166	112	0.01%	0.001%
24	4.526	989	991	993	rBV	113	77	0.01%	0.001%
25	4.565	1000	1003	1006	rBV2	167	150	0.01%	0.002%
26	4.623	1009	1021	1057	rBV	70736	197148	19.55%	2.364%
27	5.057	1141	1156	1182	rBV2	177118	394803	39.15%	4.734%
28	5.311	1224	1235	1250	rVB4	7171	16139	1.60%	0.194%
29	5.369	1251	1253	1256	rBV2	225	116	0.01%	0.001%
30	5.433	1270	1273	1280	rBV2	378	504	0.05%	0.006%
31	5.468	1281	1284	1285	rBV	181	94	0.01%	0.001%
32	5.510	1295	1297	1299	rVB	134	68	0.01%	0.001%
33	5.523	1299	1301	1303	rBV	119	63	0.01%	0.001%
34	5.587	1317	1321	1327	rBV2	228	316	0.03%	0.004%
35	5.623	1327	1332	1337	rVB2	200	163	0.02%	0.002%
36	5.719	1341	1362	1383	rBV2	357966	972923	96.48%	11.667%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
 Data File : VU054045.D
 Acq On : 02 May 2023 12:35
 Operator : JC/MD
 Sample : 02565-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

37	6.025	1454	1457	1459	rBV2	489	403	0.04%	0.005%
38	6.102	1475	1481	1483	rBV2	195	212	0.02%	0.003%
39	6.131	1488	1490	1494	rBV2	245	172	0.02%	0.002%
40	6.243	1512	1525	1555	rBV	299812	577350	57.25%	6.923%
41	6.430	1577	1583	1595	rVB2	518	984	0.10%	0.012%
42	6.481	1595	1599	1602	rBV3	405	377	0.04%	0.005%
43	6.539	1602	1617	1637	rBV	523911	1008424	100.00%	12.093%
44	6.687	1650	1663	1685	rVB	222860	434379	43.08%	5.209%
45	6.832	1706	1708	1711	rVB2	346	212	0.02%	0.003%
46	6.848	1711	1713	1717	rVB	203	143	0.01%	0.002%
47	6.870	1717	1720	1721	rBV	290	123	0.01%	0.001%
48	6.880	1721	1723	1724	rBV	139	41	0.00%	0.000%
49	6.999	1757	1760	1764	rVB2	198	151	0.01%	0.002%
50	7.028	1765	1769	1771	rBV2	246	197	0.02%	0.002%
51	7.124	1796	1799	1801	rBV2	233	161	0.02%	0.002%
52	7.195	1814	1821	1823	rBV2	531	498	0.05%	0.006%
53	7.308	1854	1856	1858	rBV	209	145	0.01%	0.002%
54	7.382	1877	1879	1882	rVB	193	97	0.01%	0.001%
55	7.401	1883	1885	1887	rBV2	154	90	0.01%	0.001%
56	7.423	1890	1892	1895	rBV	218	144	0.01%	0.002%
57	7.504	1914	1917	1918	rBV	168	92	0.01%	0.001%
58	7.562	1923	1935	1961	rVV	128549	226888	22.50%	2.721%
59	7.751	1991	1994	1997	rBV	199	185	0.02%	0.002%
60	7.835	2018	2020	2024	rVB2	230	148	0.01%	0.002%
61	7.896	2024	2039	2076	rBV	445541	787905	78.13%	9.448%
62	8.115	2105	2107	2109	rBV	337	188	0.02%	0.002%
63	8.176	2113	2126	2150	rBV	90262	154580	15.33%	1.854%
64	8.410	2197	2199	2205	rBV2	266	227	0.02%	0.003%
65	8.629	2256	2267	2297	rBV2	203293	397939	39.46%	4.772%
66	8.935	2360	2362	2366	rBV2	252	167	0.02%	0.002%
67	8.992	2377	2380	2382	rBV	185	125	0.01%	0.001%
68	9.121	2417	2420	2424	rBV	214	200	0.02%	0.002%
69	9.189	2439	2441	2444	rBV	299	197	0.02%	0.002%
70	9.237	2453	2456	2457	rBV	181	84	0.01%	0.001%
71	9.291	2470	2473	2476	rBV	186	148	0.01%	0.002%
72	9.353	2489	2492	2494	rBV2	271	167	0.02%	0.002%
73	9.414	2498	2511	2538	rBV	410745	694624	68.88%	8.330%
74	9.844	2642	2645	2650	rBV2	287	209	0.02%	0.003%
75	10.102	2720	2725	2729	rBV2	460	385	0.04%	0.005%
76	10.156	2739	2742	2744	rBV2	251	159	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
 Data File : VU054045.D
 Acq On : 02 May 2023 12:35
 Operator : JC/MD
 Sample : 02565-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
 Title : VOC Analysis

77	10.195	2751	2754	2757	rBV	288	249	0.02%	0.003%
78	10.471	2838	2840	2841	rBV	242	64	0.01%	0.001%
79	10.613	2881	2884	2886	rBV	225	163	0.02%	0.002%
80	10.652	2892	2896	2902	rBV2	305	349	0.03%	0.004%
81	10.751	2915	2927	2950	rBV	294637	472575	46.86%	5.667%
82	10.883	2966	2968	2969	rBV2	634	288	0.03%	0.003%
83	11.002	3002	3005	3009	rBV2	247	216	0.02%	0.003%
84	11.809	3243	3256	3274	rBV	432002	689239	68.35%	8.265%
85	12.188	3360	3374	3406	rBV	452874	736226	73.01%	8.829%
86	13.127	3663	3666	3671	rVB	511	381	0.04%	0.005%
87	13.227	3694	3697	3701	rBV	568	433	0.04%	0.005%
88	15.327	4347	4350	4352	rBV3	692	413	0.04%	0.005%




Sum of corrected areas: 8339000

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
Data File : VU054045.D
Acq On : 02 May 2023 12:35
Operator : JC/MD
Sample : 02565-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

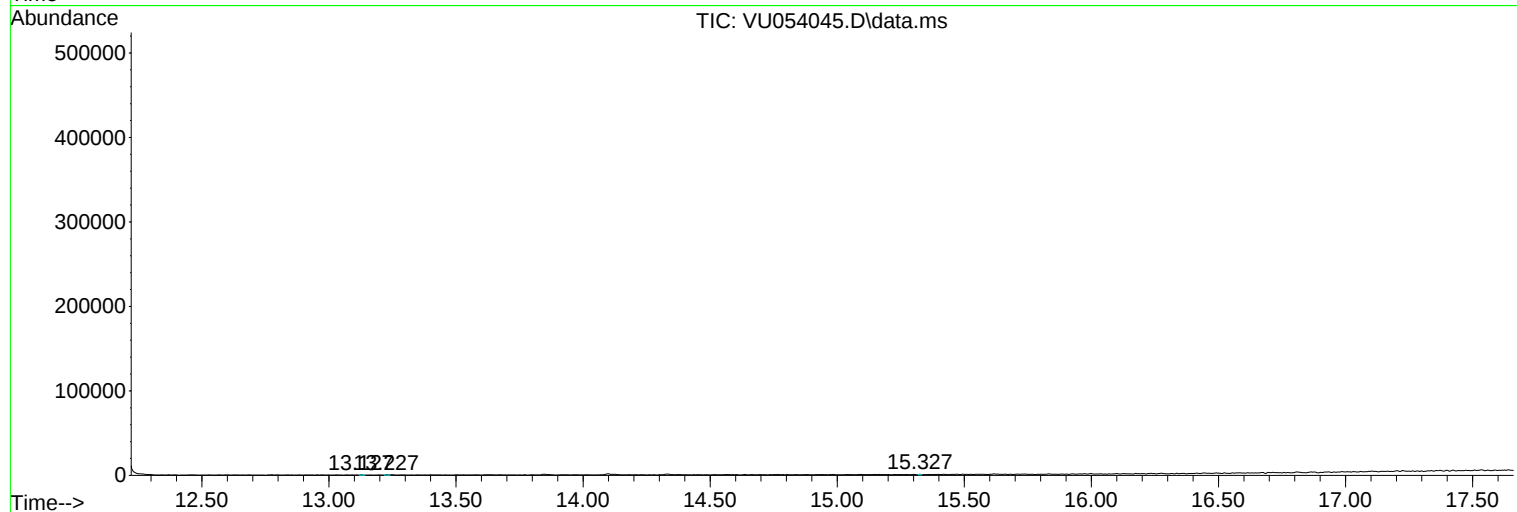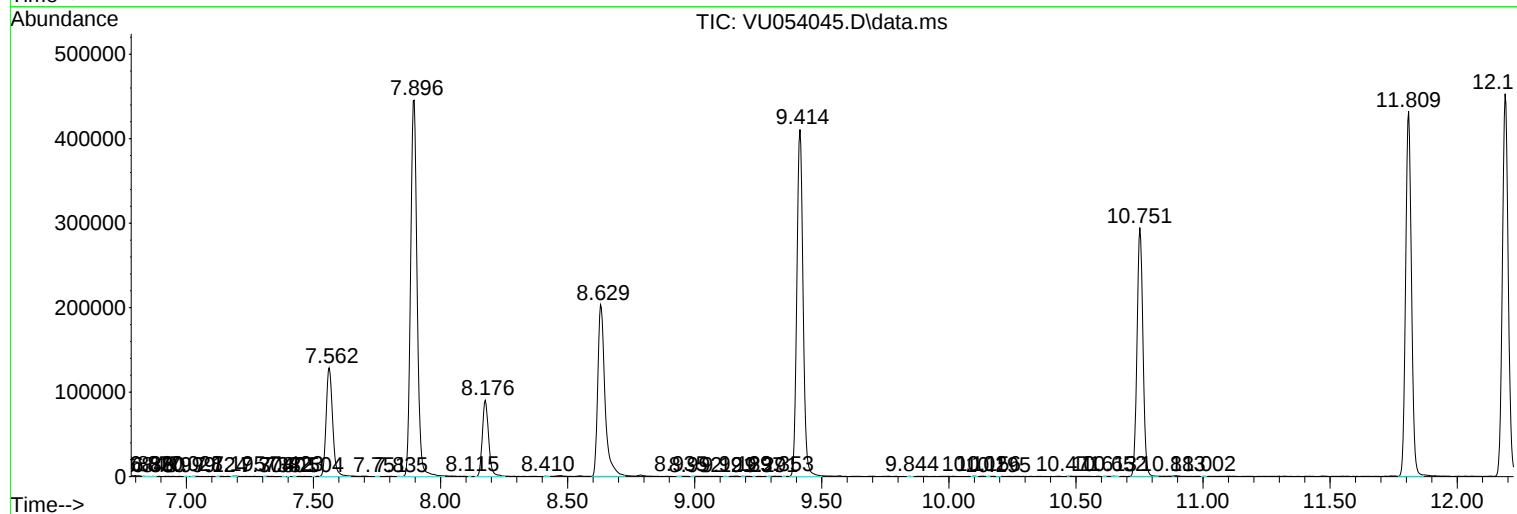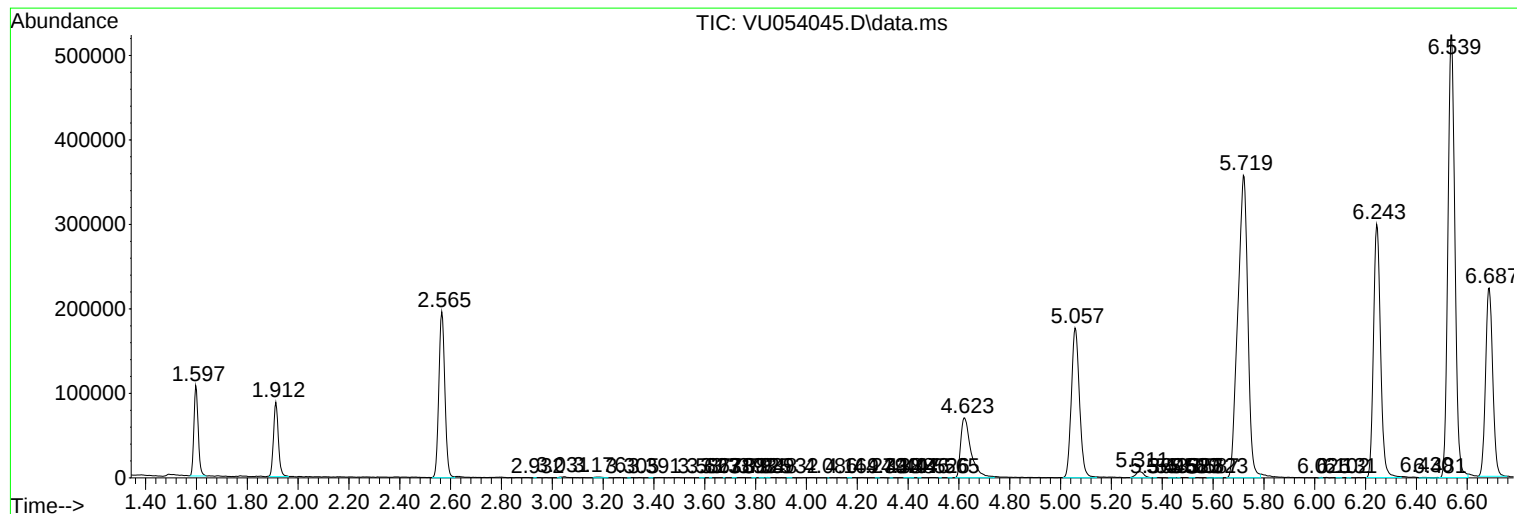

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
Data File : VU054045.D
Acq On : 02 May 2023 12:35
Operator : JC/MD
Sample : 02565-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
Data File : VU054045.D
Acq On : 02 May 2023 12:35
Operator : JC/MD
Sample : 02565-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AX4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------