
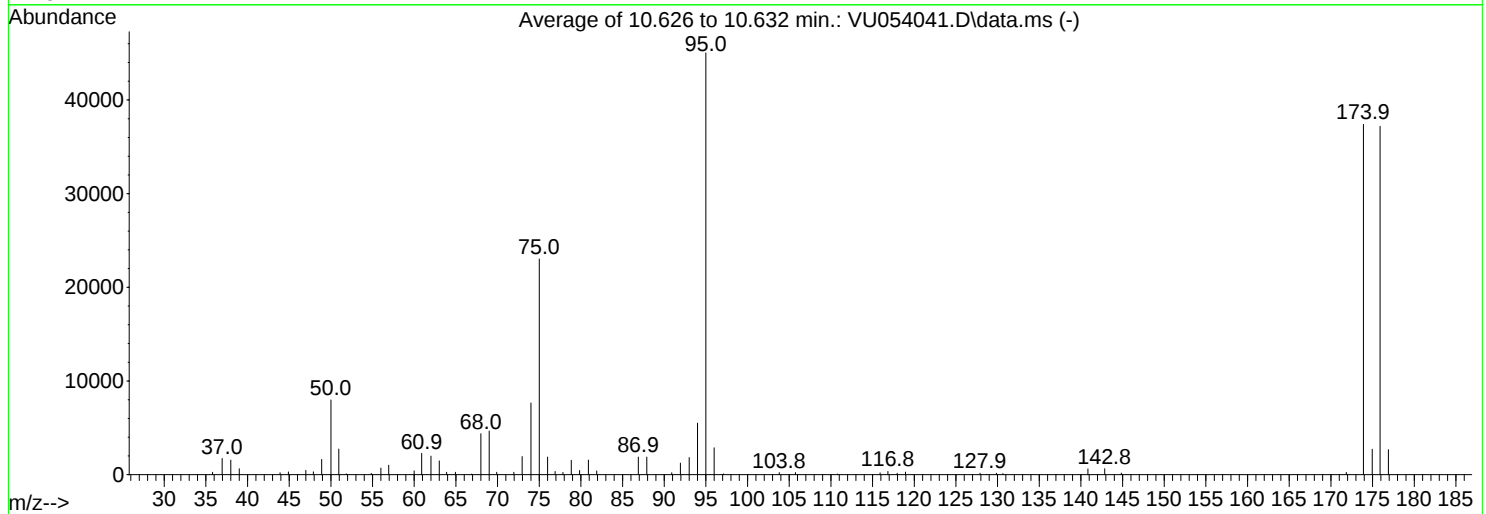


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050223\
Data File : VU054041.D
Acq On : 02 May 2023 09:08
Operator : JC/MD
Sample : BFB184
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB184

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042923WMA.M
Title : VOC Analysis
Last Update : Wed May 03 05:19:13 2023

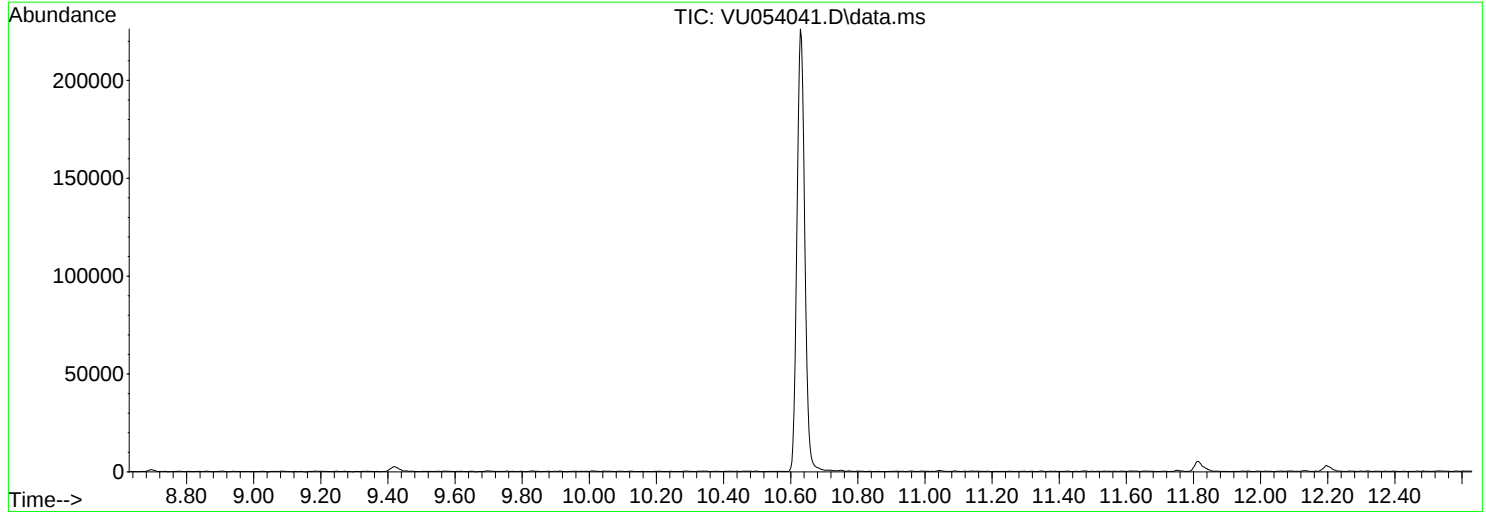

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	7971	PASS
75	95	30	80	51.1	23029	PASS
95	95	100	100	100.0	45032	PASS
96	95	5	9	6.4	2863	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.1	37400	PASS
175	174	5	9	7.3	2723	PASS
176	174	95	101	99.4	37192	PASS
177	176	5	9	7.2	2666	PASS

m/z	Abundance
39.70	112.0
43.90	171.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
35.80	250.0
36.90	1742.0
38.00	1555.0
39.00	614.0
44.00	343.0
44.90	287.0
47.00	513.0
47.90	267.0
48.90	1603.0
50.00	7693.0
51.00	2644.0
51.80	125.0
54.80	118.0
56.00	644.0
57.00	1061.0
60.00	393.0
60.90	2310.0
62.00	1933.0
63.00	1419.0
63.90	259.0
64.90	278.0
66.90	127.0
68.00	4365.0
69.00	4421.0
69.90	244.0
72.00	239.0
73.00	1975.0
74.00	7647.0
75.00	22360.0
76.00	1900.0
76.90	422.0
77.90	268.0
78.80	1521.0
79.80	435.0
80.90	1489.0
81.90	345.0
86.90	1882.0
87.90	1754.0
90.90	153.0
91.90	1133.0
93.00	1906.0
94.00	5453.0
95.00	43544.0
96.00	2806.0
97.10	126.0
103.80	193.0
105.80	234.0
110.80	103.0
115.90	185.0
116.90	387.0
117.90	148.0
119.00	255.0
127.90	133.0
129.80	127.0
130.60	115.0
140.90	601.0
142.80	607.0
144.90	181.0
171.90	208.0
173.90	34728.0
175.00	2604.0
175.90	34792.0
176.90	2577.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
35.80	278.0
37.00	1743.0
38.00	1612.0
39.00	665.0
43.90	400.0
44.90	299.0
47.00	460.0
47.90	294.0
48.90	1649.0
50.00	8250.0
51.00	2867.0
51.90	113.0
54.90	133.0
56.00	727.0
57.00	1011.0
60.00	423.0
60.90	2321.0
62.00	1997.0
63.00	1498.0
63.90	269.0
64.90	266.0
66.90	104.0
68.00	4542.0
69.00	4815.0
69.90	246.0
72.00	248.0
72.90	1958.0
74.00	7921.0
75.00	23808.0
76.00	1924.0
76.90	370.0
77.90	265.0
78.80	1554.0
79.90	444.0
80.90	1619.0
81.90	404.0
86.90	1940.0
87.90	2004.0
90.90	216.0
92.00	1235.0
93.00	1865.0
94.00	5708.0
95.00	46496.0
96.00	2978.0
97.10	119.0
103.80	235.0
105.70	230.0
110.80	107.0
115.90	199.0
116.80	355.0
117.90	164.0
119.00	280.0
127.90	175.0
129.80	159.0
130.70	123.0
140.90	665.0
142.80	648.0
144.80	180.0
171.80	245.0
173.90	38520.0
175.00	2703.0
175.90	38424.0
176.90	2755.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
35.80	267.0
37.00	1678.0
38.00	1509.0
39.00	632.0
43.90	395.0
44.90	294.0
47.00	389.0
47.90	352.0
48.90	1604.0
50.00	7969.0
50.90	2682.0
54.90	169.0
56.00	747.0
56.90	969.0
60.00	405.0
60.90	2182.0
62.00	2004.0
63.00	1515.0
63.90	244.0
65.00	206.0
68.00	4233.0
69.00	4763.0
69.90	272.0
71.90	272.0
72.90	1871.0
74.00	7381.0
75.00	22920.0
76.00	1798.0
76.90	262.0
77.80	186.0
78.90	1546.0
79.90	451.0
80.90	1553.0
81.90	415.0
86.90	1822.0
87.90	1873.0
90.90	272.0
92.00	1346.0
93.00	1739.0
94.00	5351.0
95.00	45056.0
96.00	2806.0
103.80	245.0
105.80	192.0
115.90	187.0
116.80	291.0
118.00	171.0
118.90	292.0
127.90	182.0
128.70	111.0
129.90	172.0
130.70	119.0
137.00	102.0
140.80	598.0
142.90	659.0
144.80	141.0
171.80	256.0
173.90	38952.0
174.90	2863.0
175.90	38360.0
176.90	2666.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184