

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050318\
 Data File : VU023600.D
 Acq On : 03 May 2018 14:21
 Operator : MD/SY
 Sample : J2627-18
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 04 03:02:39 2018
 Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri May 04 02:54:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.89	114	252307	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	244270	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.49	152	114305	50.00	ug/L	0.00

System Monitoring Compounds


4) Vinyl Chloride-d3	1.40	65	115040	64.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	128.66%
7) Chloroethane-d5	1.68	69	87865	64.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	128.92%
11) 1,1-Dichloroethene-d2	2.27	63	165044	47.34	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.68%
21) 2-Butanone-d5	4.18	46	196664	159.18	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	159.18%#
24) Chloroform-d	4.65	84	203191	68.71	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	137.42%#
26) 1,2-Dichloroethane-d4	5.31	65	135532	65.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	131.80%#
32) Benzene-d6	5.35	84	417706	63.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	127.48%#
36) 1,2-Dichloropropane-d6	6.34	67	142728	65.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	130.04%#
41) Toluene-d8	7.57	98	378247	62.60	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	125.20%#
43) trans-1,3-Dichloropropene-	7.85	79	60000	63.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	126.98%#
47) 2-Hexanone-d5	8.31	63	136846	164.16	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	164.16%#
57) 1,1,2,2-Tetrachloroethane-	10.44	84	188990	66.56	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	133.12%#
64) 1,2-Dichlorobenzene-d4	11.87	152	150066	67.30	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	134.60%#


Target Compounds					Ovalue
13) Acetone	2.32	43	10055	5.48 ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050318\
Data File : VU023600.D
Acq On : 03 May 2018 14:21
Operator : MD/SY
Sample : J2627-18
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 7 Sample Multiplier: 1

Quant Time: May 04 03:02:39 2018
Quant Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Quant Title : VOC Analysis
QLast Update : Fri May 04 02:54:31 2018
Response via : Initial Calibration

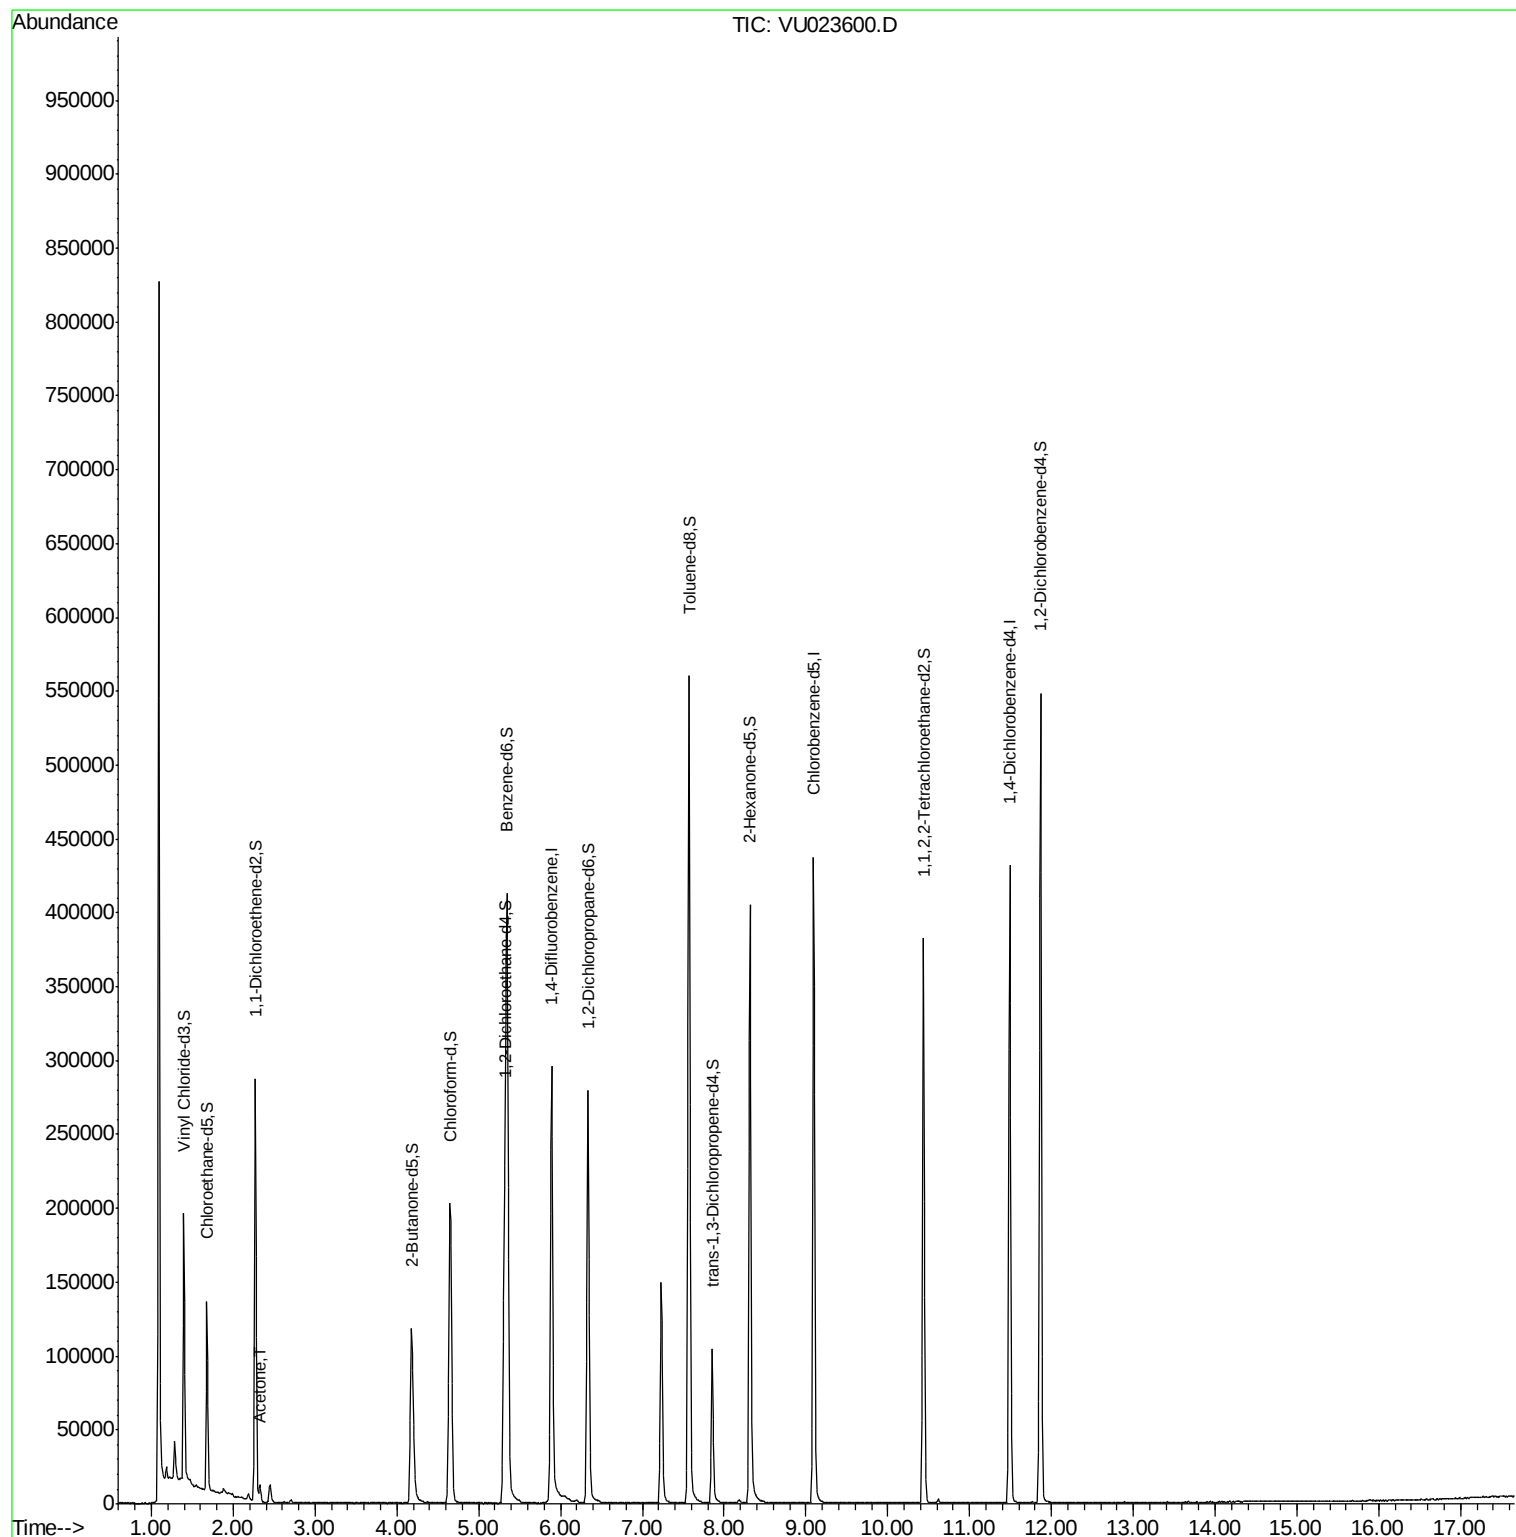

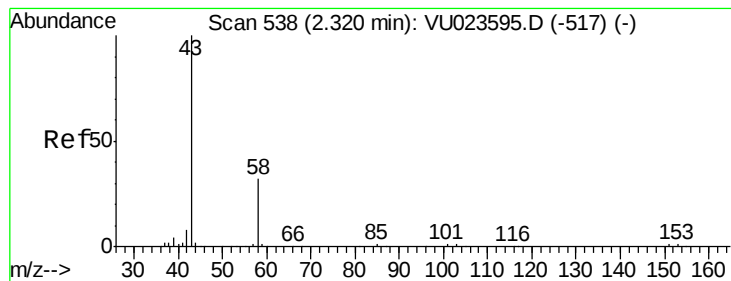

#13
 Acetone
 Concen: 5.48 ug/L
 RT: 2.32 min Scan# 539
 Delta R.T. 0.00 min
 Lab File: VU023600.D
 Acq: 03 May 2018 14:21

Tot Ion	Ratio	Lower	Upper
43	100		
58	32.4	0.0	64.8

