


Data Path : W:\HPCHEM1\MSVOA U\DATA\VU050318\
Data File : VU023594.D
Acq On : 03 May 2018 09:37
Operator : MD/SY
Sample : BFB47
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : W:\HPCHEM1\MSVOA_U\METHOD\SOMULM050118WMA.M
Title : VOC Analysis
Last Update : Mon May 07 00:51:10 2018

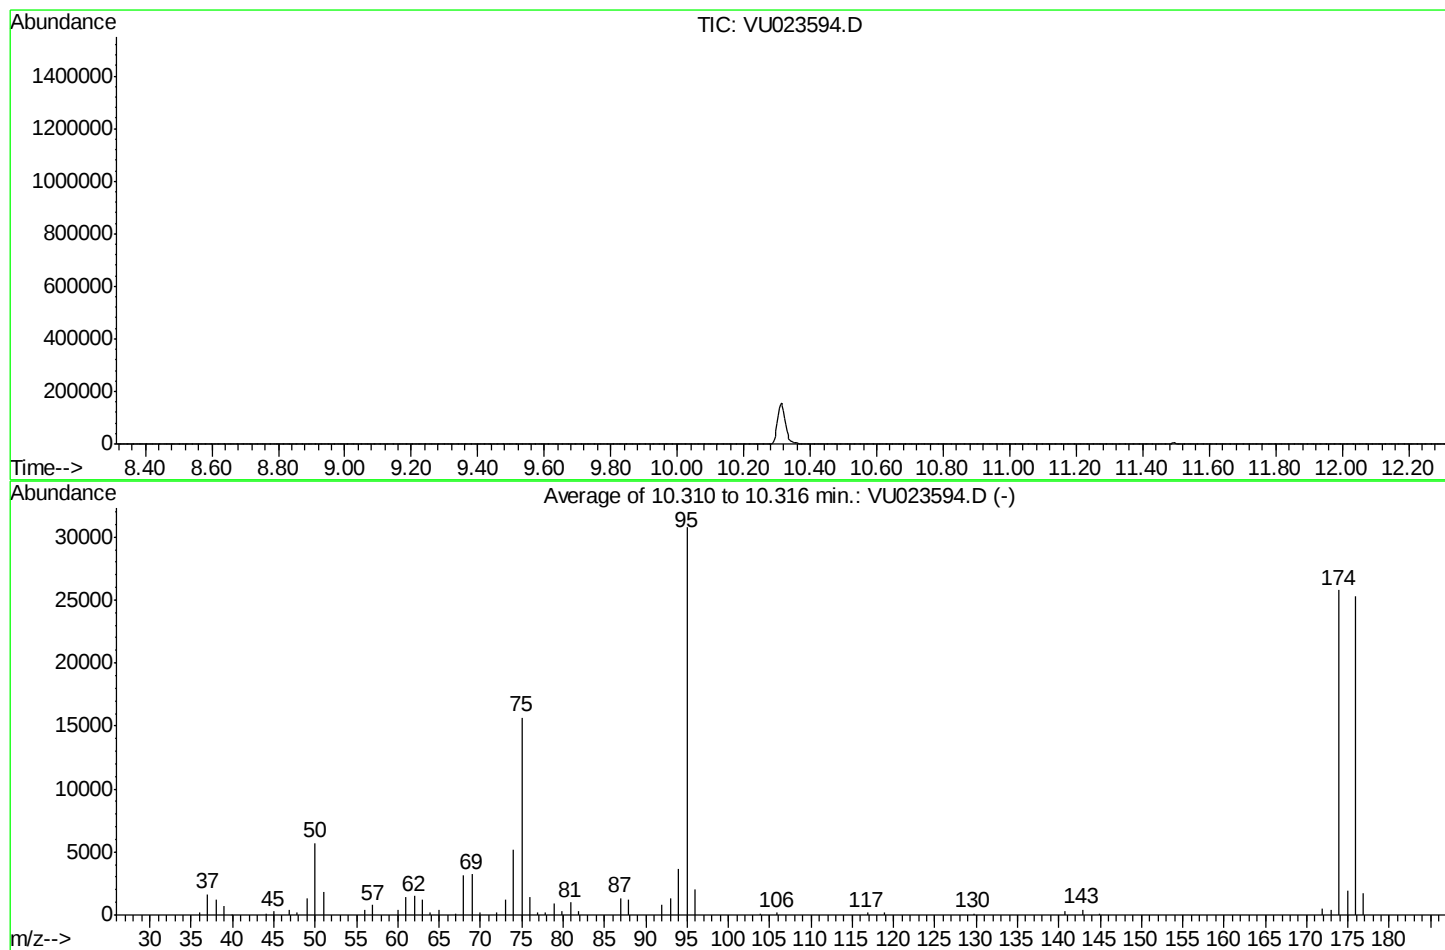

AutoFind: Scans 3023, 3024, 3025; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5689	PASS
75	95	30	80	51.0	15680	PASS
95	95	100	100	100.0	30765	PASS
96	95	5	9	6.5	2009	PASS
173	174	0.00	2	1.6	408	PASS
174	95	50	120	83.9	25800	PASS
175	174	5	9	7.4	1915	PASS
176	174	95	101	98.2	25346	PASS
177	176	5	9	6.9	1750	PASS

Scan 3011 (10.271 min): VU023594.D
BFB47

m/z	Abundance
40.00	201.0
44.00	490.0

m/z	Abundance
36.00	220.0
37.00	1693.0
38.00	1253.0
39.00	673.0
40.00	271.0
44.00	651.0
45.00	259.0
46.90	411.0
47.90	221.0
49.00	1309.0
50.00	5801.0
51.00	1833.0
56.00	357.0
57.00	843.0
60.00	356.0
61.00	1493.0
62.00	1450.0
63.00	1350.0
63.90	280.0
65.00	330.0
68.00	3216.0
69.00	3274.0
70.00	248.0
71.90	222.0
73.00	1340.0
74.00	5107.0
75.00	16009.0
76.00	1379.0
76.90	187.0
77.80	241.0
78.90	931.0
79.90	269.0
80.90	1006.0
81.80	332.0
86.90	1370.0
87.90	1296.0
91.90	823.0
93.00	1379.0
94.00	3722.0
95.00	30728.0
96.00	2099.0
103.80	102.0
105.90	169.0
116.90	168.0
118.90	187.0
129.70	100.0
140.80	239.0
142.90	392.0
144.90	149.0
171.90	443.0
173.00	397.0
173.90	25640.0
175.00	1886.0
175.90	24912.0
176.90	1776.0

Scan 3024 (10.313 min): VU023594.D
BFB47

m/z	Abundance
36.00	210.0
37.00	1698.0
38.00	1229.0
39.00	701.0
39.90	250.0
44.00	608.0
45.00	260.0
46.90	426.0
47.90	219.0
49.00	1359.0
50.00	5867.0
51.00	1892.0
55.90	393.0
57.00	826.0
60.00	393.0
61.00	1496.0
62.00	1590.0
62.90	1310.0
63.90	268.0
65.00	357.0
67.00	118.0
68.00	3329.0
69.00	3268.0
70.00	210.0
71.90	185.0
73.00	1268.0
74.00	5271.0
75.00	16180.0
76.00	1440.0
76.90	219.0
77.80	194.0
78.90	934.0
79.90	302.0
80.90	1009.0
81.80	297.0
86.90	1413.0
87.90	1308.0
92.00	855.0
93.00	1404.0
94.00	3764.0
95.00	31744.0
96.00	2062.0
103.80	118.0
105.90	163.0
116.80	180.0
118.90	184.0
129.70	102.0
140.80	290.0
142.90	450.0
144.90	155.0
171.90	548.0
173.00	430.0
173.90	26552.0
175.00	1977.0
175.90	26176.0
176.90	1806.0

Scan 3025 (10.316 min): VU023594.D
BFB47

m/z	Abundance
35.90	206.0
37.00	1503.0
38.00	1136.0
39.00	657.0
39.90	232.0
44.00	541.0
45.00	255.0
46.90	403.0
47.80	178.0
49.00	1328.0
50.00	5400.0
51.00	1751.0
55.90	368.0
57.00	763.0
60.00	348.0
61.00	1340.0
62.00	1531.0
62.90	1150.0
64.00	223.0
65.00	390.0
67.00	140.0
68.00	3052.0
69.00	3079.0
69.90	183.0
72.00	157.0
73.00	1191.0
74.00	5028.0
75.00	14851.0
76.00	1355.0
76.90	199.0
77.80	149.0
78.90	875.0
79.80	295.0
80.90	935.0
81.90	252.0
87.00	1335.0
88.00	1192.0
92.00	852.0
93.00	1245.0
94.00	3421.0
95.00	29824.0
96.00	1867.0
103.80	135.0
105.90	138.0
116.80	189.0
118.90	162.0
129.70	104.0
140.80	301.0
142.90	418.0
144.80	129.0
171.90	559.0
173.00	398.0
173.90	25208.0
175.00	1883.0
176.00	24952.0
176.90	1670.0