

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031753.D
 Acq On : 03 May 2019 16:27
 Operator : JC/SP
 Sample : K2694-02
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFHH2

Manual Integrations
 APPROVED

MMDadoda
 5/6/2019 11:43:28 AM

Quant Time: May 04 06:47:49 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 04 02:35:16 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	773757	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	748416	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	294564	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	307068	47.42	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	94.84%
7) Chloroethane-d5	1.68	69	249592	49.88	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	99.76%
11) 1,1-Dichloroethene-d2	2.27	63	450234	34.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.82%
21) 2-Butanone-d5	4.19	46	635853	108.37	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.37%
24) Chloroform-d	4.64	84	526209	44.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.74%
26) 1,2-Dichloroethane-d4	5.31	65	361833	46.70	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.40%
32) Benzene-d6	5.34	84	1077058	46.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.74%
36) 1,2-Dichloropropane-d6	6.33	67	381290	47.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.32%
41) Toluene-d8	7.56	98	881404	44.03	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.06%
43) trans-1,3-Dichloropropene-	7.85	79	152406	43.91	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.82%
47) 2-Hexanone-d5	8.31	63	383831	109.68	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.68%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	505042	46.54	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.08%
64) 1,2-Dichlorobenzene-d4	11.86	152	289179	46.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.36%

Target Compounds				Ovalue
13) Acetone	2.35	43	12576m	1.903 ug/L
34) Trichloroethene	6.19	95	4408	0.661 ug/L # 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031753.D
Acq On : 03 May 2019 16:27
Operator : JC/SP
Sample : K2694-02
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
BFHH2

Manual Integrations
APPROVED

MMDadoda
5/6/2019 11:43:28 AM

Quant Time: May 04 06:47:49 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 04 02:35:16 2019
Response via : Initial Calibration

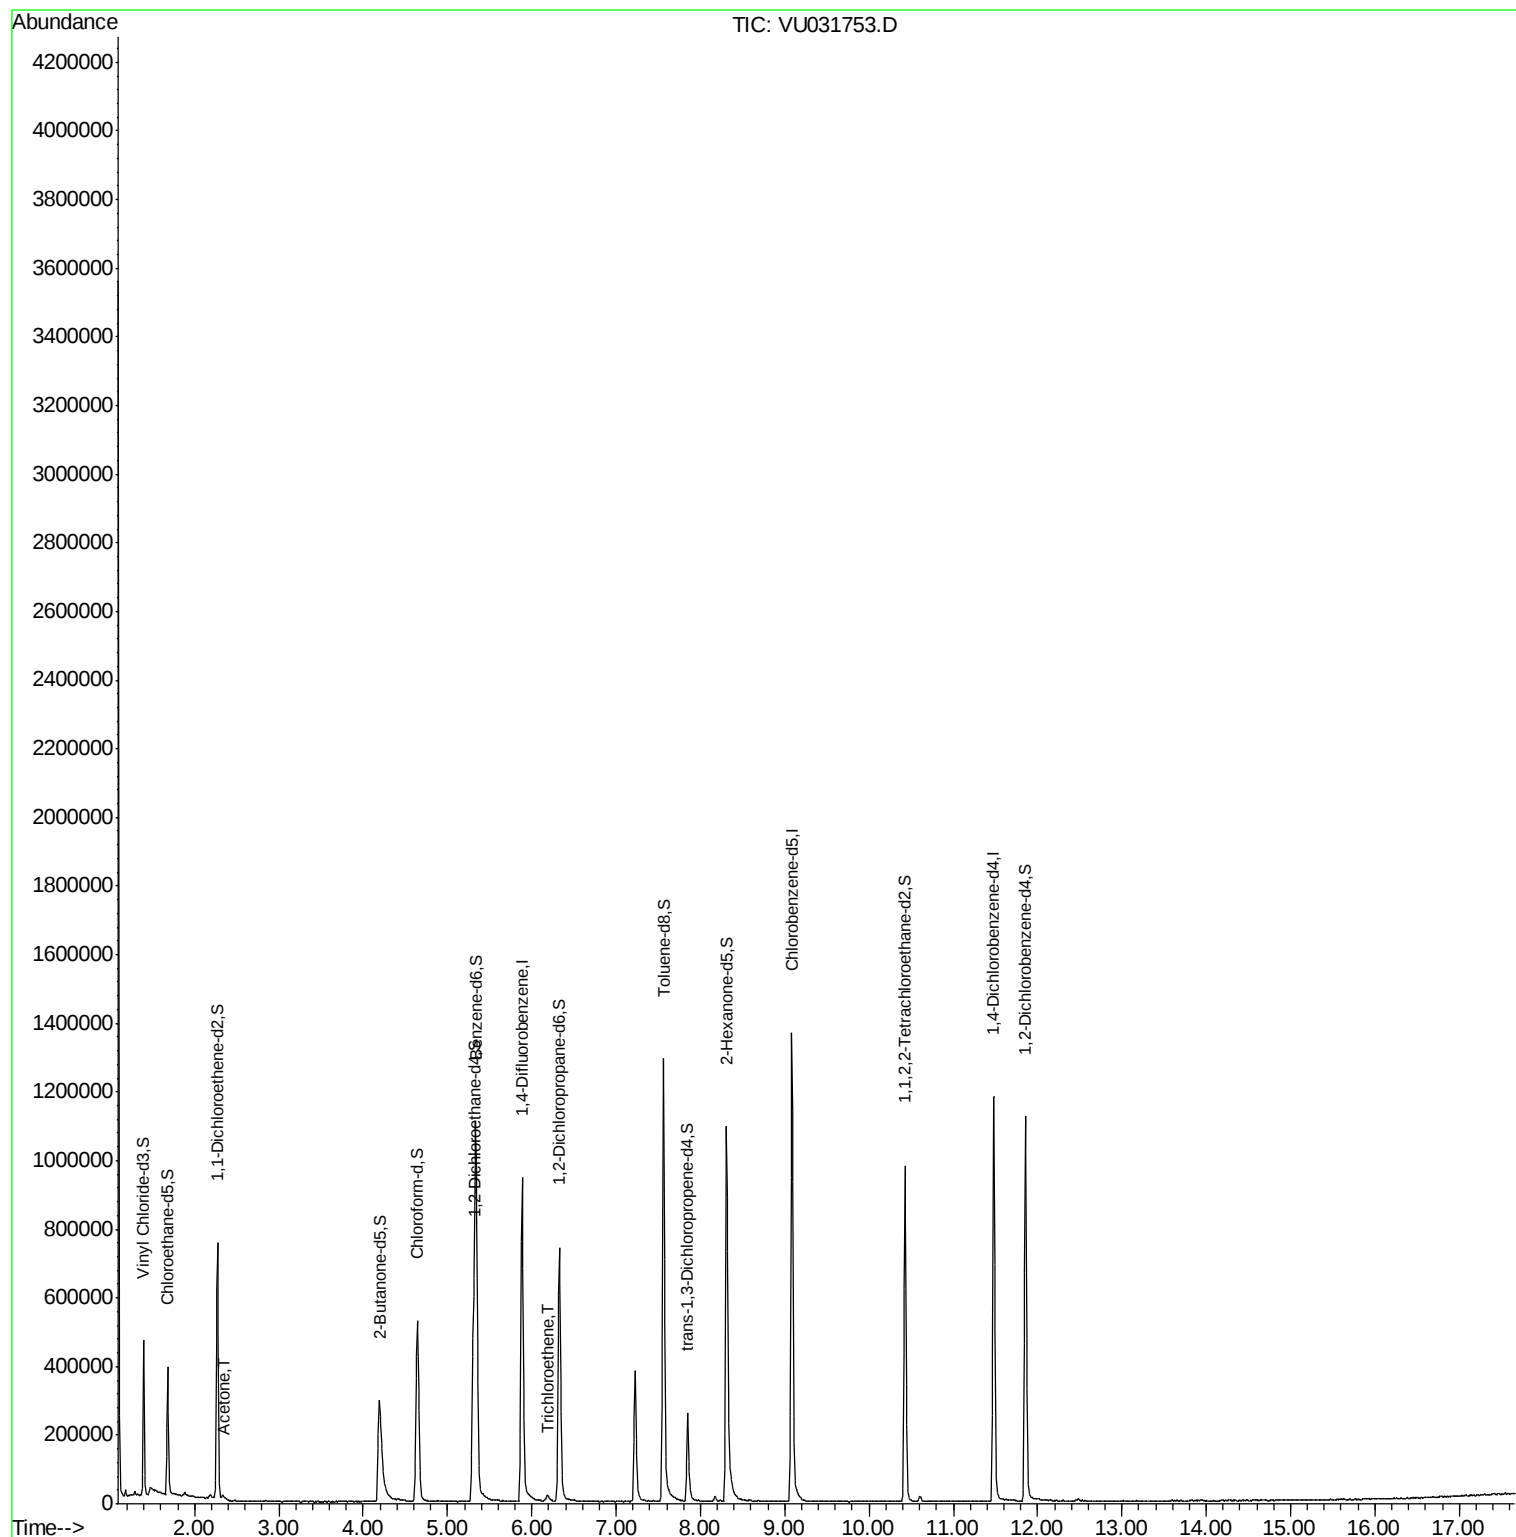

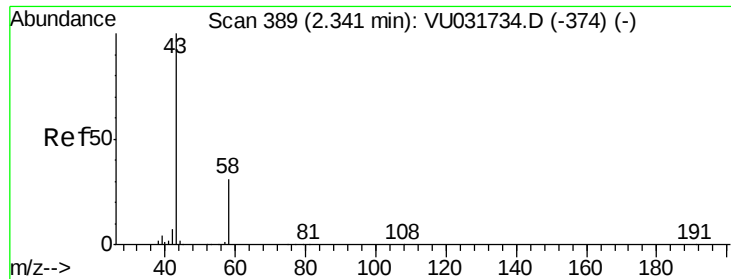





#13
Acetone
Concen: 1.903 ug/L m
RT: 2.35 min Scan# 393
Delta R.T. 0.01 min
Lab File: VU031753.D
Acq: 03 May 2019 16:27

Instrument :
MSVOA_U
ClientSampleId :
BFHH2

Tot Ion: 43 Resp: 12576
Ion Ratio Lower Upper
43 100
58 24.5 0.0 64.4

Manual Integrations
APPROVED

MMDadoda
5/6/2019 11:43:28 AM

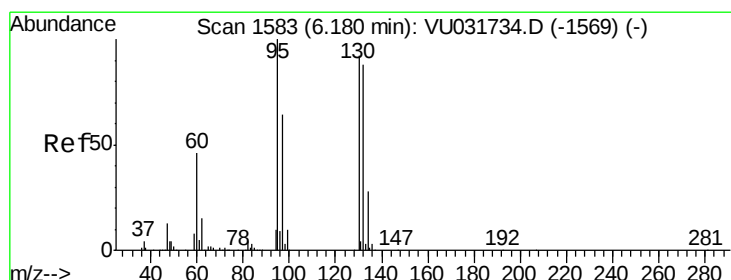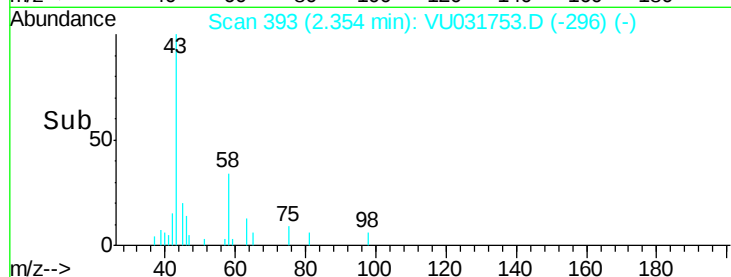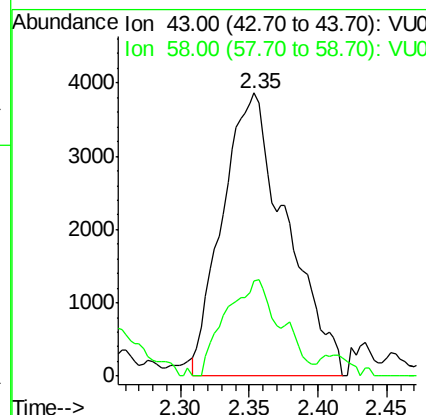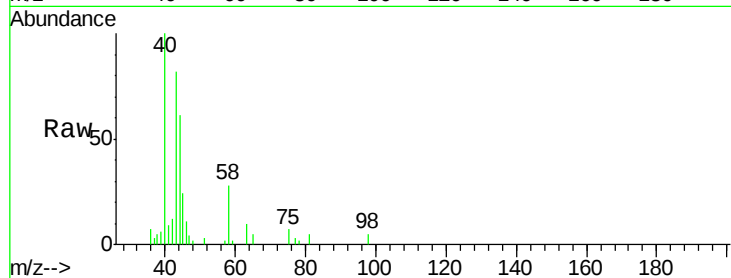

#34
Trichloroethene
Concen: 0.661 ug/L
RT: 6.19 min Scan# 1587
Delta R.T. 0.01 min
Lab File: VU031753.D
Acq: 03 May 2019 16:27

Tgt Ion: 95 Resp: 4408
Ion Ratio Lower Upper
95 100
97 83.3 44.8 83.2#
132 109.2 63.1 117.1
130 107.2 66.5 123.5

