

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031744.D
 Acq On : 03 May 2019 12:58
 Operator : JC/SP
 Sample : K2661-09DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.283	55	60	68	rVB2	41126	42031	1.13%	0.141%
2	1.396	88	95	108	rBV	552550	587353	15.79%	1.971%
3	1.679	176	183	198	rVB	401546	523070	14.06%	1.755%
4	2.270	356	367	380	rBV	862060	1320358	35.49%	4.431%
5	2.460	424	426	428	rBV2	1551	725	0.02%	0.002%
6	2.479	428	432	437	rVB5	1970	1961	0.05%	0.007%
7	2.781	523	526	532	rBV5	1761	1785	0.05%	0.006%
8	2.945	574	577	579	rBV	1306	969	0.03%	0.003%
9	2.974	583	586	588	rBV3	2540	1921	0.05%	0.006%
10	3.071	614	616	619	rVB4	1139	622	0.02%	0.002%
11	3.090	619	622	626	rBV3	1364	943	0.03%	0.003%
12	3.145	636	639	643	rBV3	854	709	0.02%	0.002%
13	3.193	651	654	656	rBV2	1245	719	0.02%	0.002%
14	3.238	664	668	670	rBV3	818	622	0.02%	0.002%
15	3.296	680	686	688	rBV3	1262	1101	0.03%	0.004%
16	3.370	703	709	711	rBV5	1077	1230	0.03%	0.004%
17	3.396	712	717	720	rVB4	1560	1438	0.04%	0.005%
18	3.489	742	746	749	rBV2	1420	1204	0.03%	0.004%
19	3.588	770	777	780	rBV4	1342	1375	0.04%	0.005%
20	3.675	802	804	808	rVB2	1258	765	0.02%	0.003%
21	3.756	826	829	831	rBV3	1466	928	0.02%	0.003%
22	3.801	841	843	851	rVB6	965	934	0.03%	0.003%
23	3.836	851	854	857	rBV4	1208	1040	0.03%	0.003%
24	3.910	873	877	880	rVB3	1949	1290	0.03%	0.004%
25	3.933	880	884	894	rBV3	1402	1805	0.05%	0.006%
26	4.042	915	918	919	rBV	953	630	0.02%	0.002%
27	4.116	936	941	944	rVB	977	706	0.02%	0.002%
28	4.190	951	964	1015	rBV	317370	1154474	31.03%	3.874%
29	4.643	1088	1105	1131	rBV	585771	1401192	37.66%	4.702%
30	4.865	1170	1174	1175	rBV	1973	1325	0.04%	0.004%
31	4.904	1184	1186	1191	rVB2	2071	1275	0.03%	0.004%
32	5.055	1229	1233	1237	rBV5	863	967	0.03%	0.003%
33	5.193	1272	1276	1280	rBV4	1390	1303	0.04%	0.004%
34	5.334	1297	1320	1356	rBV2	1225953	3720305	100.00%	12.485%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031744.D
 Acq On : 03 May 2019 12:58
 Operator : JC/SP
 Sample : K2661-09DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.752	1447	1450	1452	rBV3	1877	1010	0.03%	0.003%
36	5.765	1452	1454	1457	rVB3	1386	650	0.02%	0.002%
37	5.785	1457	1460	1464	rBV6	1728	1162	0.03%	0.004%
38	5.881	1476	1490	1521	rBV	1018447	2116662	56.89%	7.103%
39	6.186	1570	1585	1602	rBV4	85066	187780	5.05%	0.630%
40	6.328	1615	1629	1658	rBV	801044	1669157	44.87%	5.602%
41	6.640	1723	1726	1731	rBV3	2221	1515	0.04%	0.005%
42	6.685	1738	1740	1744	rVB5	1186	636	0.02%	0.002%
43	6.768	1762	1766	1770	rVB4	1382	1290	0.03%	0.004%
44	6.791	1770	1773	1776	rBV2	1162	994	0.03%	0.003%
45	6.881	1796	1801	1803	rBV2	1211	1135	0.03%	0.004%
46	6.903	1805	1808	1811	rBV2	1311	803	0.02%	0.003%
47	6.948	1819	1822	1824	rBV2	1575	1239	0.03%	0.004%
48	6.965	1824	1827	1830	rVV3	1405	1216	0.03%	0.004%
49	7.000	1834	1838	1839	rBV	1226	777	0.02%	0.003%
50	7.151	1882	1885	1888	rBV2	1066	630	0.02%	0.002%
51	7.225	1895	1908	1926	rBV	423748	788094	21.18%	2.645%
52	7.373	1951	1954	1956	rBV3	1177	616	0.02%	0.002%
53	7.460	1978	1981	1989	rVB7	2302	2315	0.06%	0.008%
54	7.511	1993	1997	1998	rBV4	1235	923	0.02%	0.003%
55	7.563	2000	2013	2059	rBV	1508064	2801109	75.29%	9.400%
56	7.849	2091	2102	2125	rBV	279088	522827	14.05%	1.755%
57	7.990	2143	2146	2149	rBV4	1268	715	0.02%	0.002%
58	8.077	2168	2173	2177	rBV4	1130	1258	0.03%	0.004%
59	8.122	2183	2187	2192	rBV3	1016	1161	0.03%	0.004%
60	8.173	2197	2203	2205	rBV4	4303	4603	0.12%	0.015%
61	8.222	2206	2218	2236	rVV	1222128	2138225	57.47%	7.176%
62	8.312	2236	2246	2282	rVB	1126345	2251902	60.53%	7.557%
63	8.665	2353	2356	2361	rVB5	2223	1441	0.04%	0.005%
64	8.907	2427	2431	2435	rVB5	1964	1745	0.05%	0.006%
65	8.997	2457	2459	2461	rBV2	1285	675	0.02%	0.002%
66	9.087	2474	2487	2532	rBV	1483861	2601462	69.93%	8.730%
67	9.325	2558	2561	2564	rBV4	1761	1335	0.04%	0.004%
68	9.514	2617	2620	2623	rBV4	1148	896	0.02%	0.003%
69	9.550	2627	2631	2634	rBV2	1558	1298	0.03%	0.004%
70	9.601	2645	2647	2650	rBV2	986	741	0.02%	0.002%
71	9.820	2712	2715	2718	rVB2	1189	808	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031744.D
 Acq On : 03 May 2019 12:58
 Operator : JC/SP
 Sample : K2661-09DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.849	2721	2724	2726	rBV2	1318	806	0.02%	0.003%
73	9.890	2733	2737	2739	rBV2	1628	1383	0.04%	0.005%
74	9.987	2764	2767	2774	rBV3	1789	1581	0.04%	0.005%
75	10.087	2794	2798	2802	rBV4	1391	1251	0.03%	0.004%
76	10.135	2808	2813	2816	rBV4	672	634	0.02%	0.002%
77	10.247	2845	2848	2851	rVB2	1348	935	0.03%	0.003%
78	10.270	2851	2855	2857	rBV2	990	622	0.02%	0.002%
79	10.283	2857	2859	2862	rVB	1321	708	0.02%	0.002%
80	10.305	2862	2866	2868	rBV2	1790	1431	0.04%	0.005%
81	10.344	2876	2878	2881	rVB2	1258	798	0.02%	0.003%
82	10.363	2881	2884	2888	rBV2	1311	1256	0.03%	0.004%
83	10.427	2892	2904	2931	rVV	1026617	1683805	45.26%	5.651%
84	10.736	2996	3000	3004	rBV4	1261	1351	0.04%	0.005%
85	10.813	3019	3024	3030	rBV6	1153	1369	0.04%	0.005%
86	10.884	3043	3046	3048	rBV2	1436	925	0.02%	0.003%
87	10.977	3072	3075	3079	rBV3	1209	1184	0.03%	0.004%
88	11.051	3092	3098	3102	rBV9	2537	3680	0.10%	0.012%
89	11.154	3127	3130	3132	rBV4	1425	974	0.03%	0.003%
90	11.247	3155	3159	3164	rBV	1762	1739	0.05%	0.006%
91	11.402	3204	3207	3208	rBV2	2091	1176	0.03%	0.004%
92	11.479	3217	3231	3256	rBV	1266356	2076623	55.82%	6.969%
93	11.855	3336	3348	3374	rBV	1276906	2113065	56.80%	7.091%
94	12.771	3630	3633	3636	rBV3	2045	1342	0.04%	0.005%
95	12.948	3685	3688	3693	rBV4	1320	1404	0.04%	0.005%
96	13.138	3745	3747	3752	rVB2	1772	1204	0.03%	0.004%
97	13.305	3796	3799	3805	rBV4	1725	1464	0.04%	0.005%
98	13.450	3839	3844	3846	rBV3	1594	1265	0.03%	0.004%
99	13.543	3870	3873	3875	rBV2	1631	1138	0.03%	0.004%
100	13.736	3928	3933	3937	rBV3	2400	2467	0.07%	0.008%


Sum of corrected areas: 29797460

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031744.D
Acq On : 03 May 2019 12:58
Operator : JC/SP
Sample : K2661-09DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

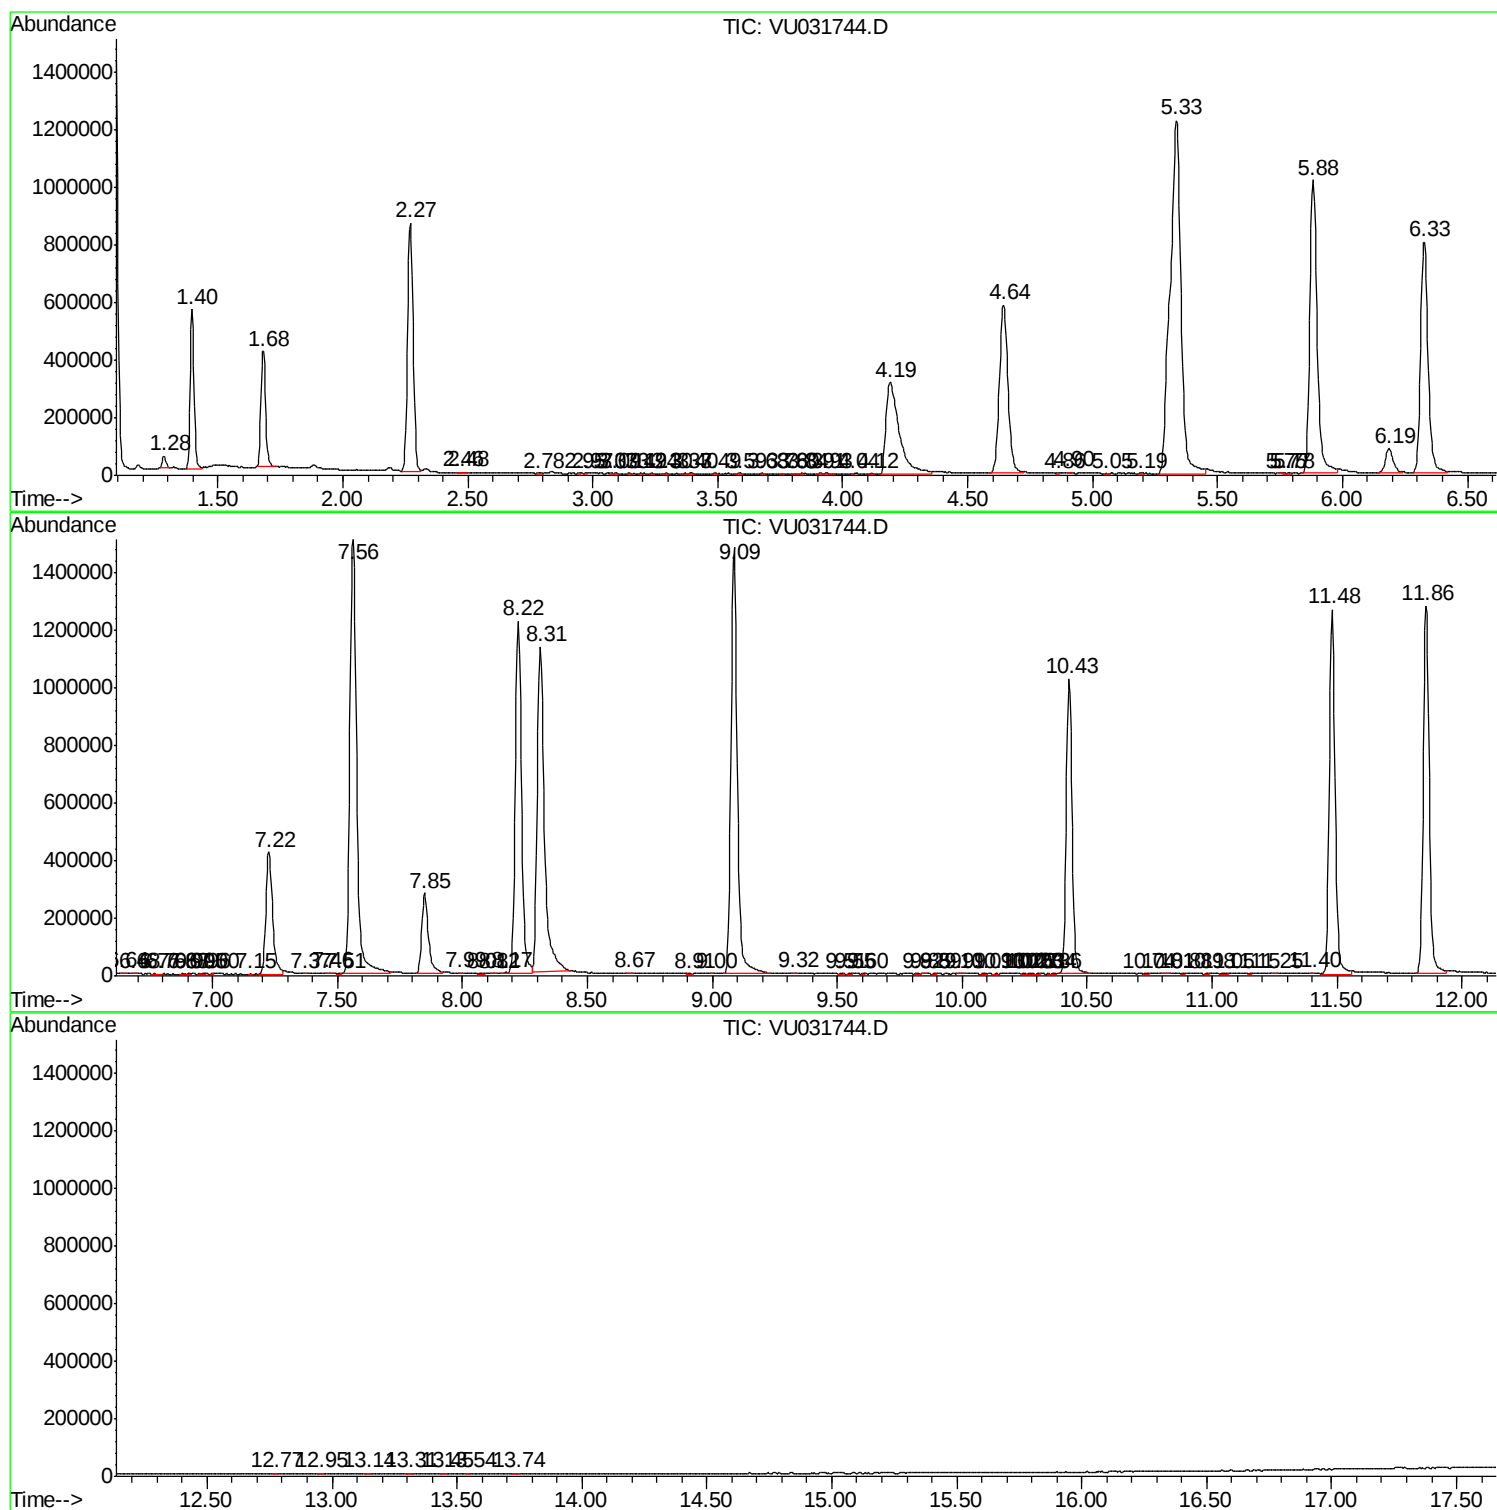

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031744.D
Acq On : 03 May 2019 12:58
Operator : JC/SP
Sample : K2661-09DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031744.D
Acq On : 03 May 2019 12:58
Operator : JC/SP
Sample : K2661-09DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
