

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031746.D
 Acq On : 03 May 2019 13:44
 Operator : JC/SP
 Sample : K2661-05 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.283	55	60	70	rBV2	66445	68030	1.83%	0.205%
2	1.396	88	95	107	rBV	535472	576536	15.47%	1.734%
3	1.679	176	183	201	rVB	415431	529645	14.21%	1.593%
4	2.270	356	367	380	rBV	858114	1312360	35.22%	3.946%
5	2.560	453	457	459	rBV3	1416	1026	0.03%	0.003%
6	2.611	470	473	476	rBV4	1766	1321	0.04%	0.004%
7	2.769	519	522	526	rVB4	1552	1159	0.03%	0.003%
8	2.978	579	587	598	rBV4	10918	21166	0.57%	0.064%
9	3.119	623	631	634	rBV3	1901	2568	0.07%	0.008%
10	3.174	646	648	652	rVB2	1116	753	0.02%	0.002%
11	3.235	659	667	670	rBV5	1760	2429	0.07%	0.007%
12	3.312	688	691	693	rBV2	1319	769	0.02%	0.002%
13	3.370	704	709	713	rBV3	1770	1755	0.05%	0.005%
14	3.441	726	731	735	rBV4	2506	3129	0.08%	0.009%
15	3.492	742	747	748	rBV2	1554	1189	0.03%	0.004%
16	3.550	761	765	769	rVV3	2059	1667	0.04%	0.005%
17	3.621	785	787	790	rVV2	1234	768	0.02%	0.002%
18	3.640	790	793	799	rVB4	1193	1048	0.03%	0.003%
19	3.672	799	803	807	rVB4	959	753	0.02%	0.002%
20	3.717	814	817	820	rBV2	1030	765	0.02%	0.002%
21	3.817	844	848	851	rBV2	1367	921	0.02%	0.003%
22	3.878	864	867	871	rBV3	958	751	0.02%	0.002%
23	4.006	903	907	909	rBV3	1563	936	0.03%	0.003%
24	4.212	949	971	1004	rBV2	419011	1741379	46.74%	5.236%
25	4.643	1089	1105	1130	rBV	582191	1378999	37.01%	4.147%
26	4.846	1165	1168	1170	rBV2	1584	788	0.02%	0.002%
27	4.974	1199	1208	1212	rBV8	2843	4045	0.11%	0.012%
28	5.042	1227	1229	1233	rVB3	1015	735	0.02%	0.002%
29	5.125	1250	1255	1260	rBV6	1826	1502	0.04%	0.005%
30	5.167	1265	1268	1274	rBV5	1384	1599	0.04%	0.005%
31	5.199	1274	1278	1283	rBV4	944	777	0.02%	0.002%
32	5.334	1294	1320	1351	rBV3	1231476	3726038	100.00%	11.204%
33	5.881	1473	1490	1535	rBV	1039146	2200256	59.05%	6.616%
34	6.183	1569	1584	1614	rBV	1217223	2469704	66.28%	7.426%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031746.D
 Acq On : 03 May 2019 13:44
 Operator : JC/SP
 Sample : K2661-05 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.325	1616	1628	1653	rVB	815886	1664431	44.67%	5.005%
36	6.556	1697	1700	1702	rBV2	1523	885	0.02%	0.003%
37	6.688	1738	1741	1747	rVB3	1918	1521	0.04%	0.005%
38	6.733	1750	1755	1759	rBV5	1009	1120	0.03%	0.003%
39	6.768	1762	1766	1769	rBV3	1543	1303	0.03%	0.004%
40	6.849	1785	1791	1794	rBV4	1817	1919	0.05%	0.006%
41	6.903	1803	1808	1809	rBV3	1712	1370	0.04%	0.004%
42	6.971	1826	1829	1830	rBV	1613	878	0.02%	0.003%
43	6.993	1834	1836	1840	rVB4	1480	1019	0.03%	0.003%
44	7.029	1844	1847	1851	rVB2	1323	1028	0.03%	0.003%
45	7.061	1854	1857	1860	rBV4	958	746	0.02%	0.002%
46	7.132	1876	1879	1884	rVB3	1086	763	0.02%	0.002%
47	7.225	1895	1908	1926	rBV	431303	802898	21.55%	2.414%
48	7.447	1974	1977	1979	rBV	1698	1223	0.03%	0.004%
49	7.563	1998	2013	2037	rBV	1505970	2746800	73.72%	8.260%
50	7.849	2089	2102	2135	rBV	282594	539413	14.48%	1.622%
51	8.112	2181	2184	2190	rBV4	910	764	0.02%	0.002%
52	8.177	2194	2204	2206	rBV4	6154	7913	0.21%	0.024%
53	8.222	2206	2218	2235	rVV	1391198	2423863	65.05%	7.288%
54	8.312	2236	2246	2281	rVB	1168525	2321806	62.31%	6.982%
55	8.579	2326	2329	2332	rBV4	1172	932	0.03%	0.003%
56	8.678	2357	2360	2364	rVB3	1954	1110	0.03%	0.003%
57	8.720	2364	2373	2378	rBV8	1726	2889	0.08%	0.009%
58	8.788	2391	2394	2398	rVB4	1856	1410	0.04%	0.004%
59	8.810	2398	2401	2404	rBV3	1316	1071	0.03%	0.003%
60	8.884	2419	2424	2427	rBV7	1199	1297	0.03%	0.004%
61	8.926	2435	2437	2439	rBV2	1449	831	0.02%	0.002%
62	9.016	2462	2465	2470	rVB4	2122	1585	0.04%	0.005%
63	9.087	2470	2487	2535	rBV	1494187	2652228	71.18%	7.975%
64	9.386	2577	2580	2583	rVB5	2064	1150	0.03%	0.003%
65	9.421	2588	2591	2595	rBV3	1373	1155	0.03%	0.003%
66	9.514	2613	2620	2622	rBV4	1304	1229	0.03%	0.004%
67	9.540	2626	2628	2631	rVB2	1560	795	0.02%	0.002%
68	9.608	2645	2649	2652	rVB3	1025	823	0.02%	0.002%
69	9.633	2652	2657	2658	rBV3	1755	1224	0.03%	0.004%
70	9.759	2692	2696	2701	rBV6	1418	1642	0.04%	0.005%
71	9.833	2716	2719	2728	rBV6	1722	1672	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031746.D
 Acq On : 03 May 2019 13:44
 Operator : JC/SP
 Sample : K2661-05 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B25

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.900	2736	2740	2742	rBV2	1545	1190	0.03%	0.004%
73	10.006	2770	2773	2776	rBV3	1259	832	0.02%	0.003%
74	10.109	2803	2805	2810	rVB3	1958	1667	0.04%	0.005%
75	10.141	2810	2815	2818	rBV3	1726	1773	0.05%	0.005%
76	10.328	2869	2873	2878	rBV4	1366	1451	0.04%	0.004%
77	10.376	2884	2888	2892	rBV2	3565	3643	0.10%	0.011%
78	10.427	2892	2904	2929	rVV	1038660	1699159	45.60%	5.109%
79	10.566	2943	2947	2949	rBV4	1629	1388	0.04%	0.004%
80	10.604	2955	2959	2962	rBV6	2262	1901	0.05%	0.006%
81	10.903	3049	3052	3056	rBV	2406	2150	0.06%	0.006%
82	10.993	3077	3080	3084	rVB2	1573	1176	0.03%	0.004%
83	11.077	3100	3106	3109	rBV5	2594	3174	0.09%	0.010%
84	11.189	3136	3141	3144	rBV3	1823	1872	0.05%	0.006%
85	11.302	3171	3176	3180	rBV4	1366	1564	0.04%	0.005%
86	11.341	3186	3188	3191	rVB	1519	857	0.02%	0.003%
87	11.373	3195	3198	3200	rBV2	1812	1134	0.03%	0.003%
88	11.421	3209	3213	3217	rBV4	1700	1871	0.05%	0.006%
89	11.479	3217	3231	3257	rBV	1306272	2135529	57.31%	6.421%
90	11.855	3336	3348	3377	rBV	1280394	2129469	57.15%	6.403%
91	12.813	3644	3646	3651	rVB3	1222	820	0.02%	0.002%
92	12.942	3684	3686	3689	rBV	1350	890	0.02%	0.003%
93	13.148	3748	3750	3756	rBV3	1921	2077	0.06%	0.006%
94	13.247	3778	3781	3785	rBV3	1127	883	0.02%	0.003%
95	13.418	3831	3834	3839	rVB3	2380	1986	0.05%	0.006%
96	13.527	3866	3868	3869	rBV	1578	730	0.02%	0.002%
97	13.559	3876	3878	3880	rBV2	1456	887	0.02%	0.003%
98	14.215	4079	4082	4084	rBV2	1478	1008	0.03%	0.003%
99	14.411	4141	4143	4145	rBV2	1275	783	0.02%	0.002%
100	14.791	4258	4261	4267	rVB4	2084	2397	0.06%	0.007%


Sum of corrected areas: 33256233

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031746.D
Acq On : 03 May 2019 13:44
Operator : JC/SP
Sample : K2661-05 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

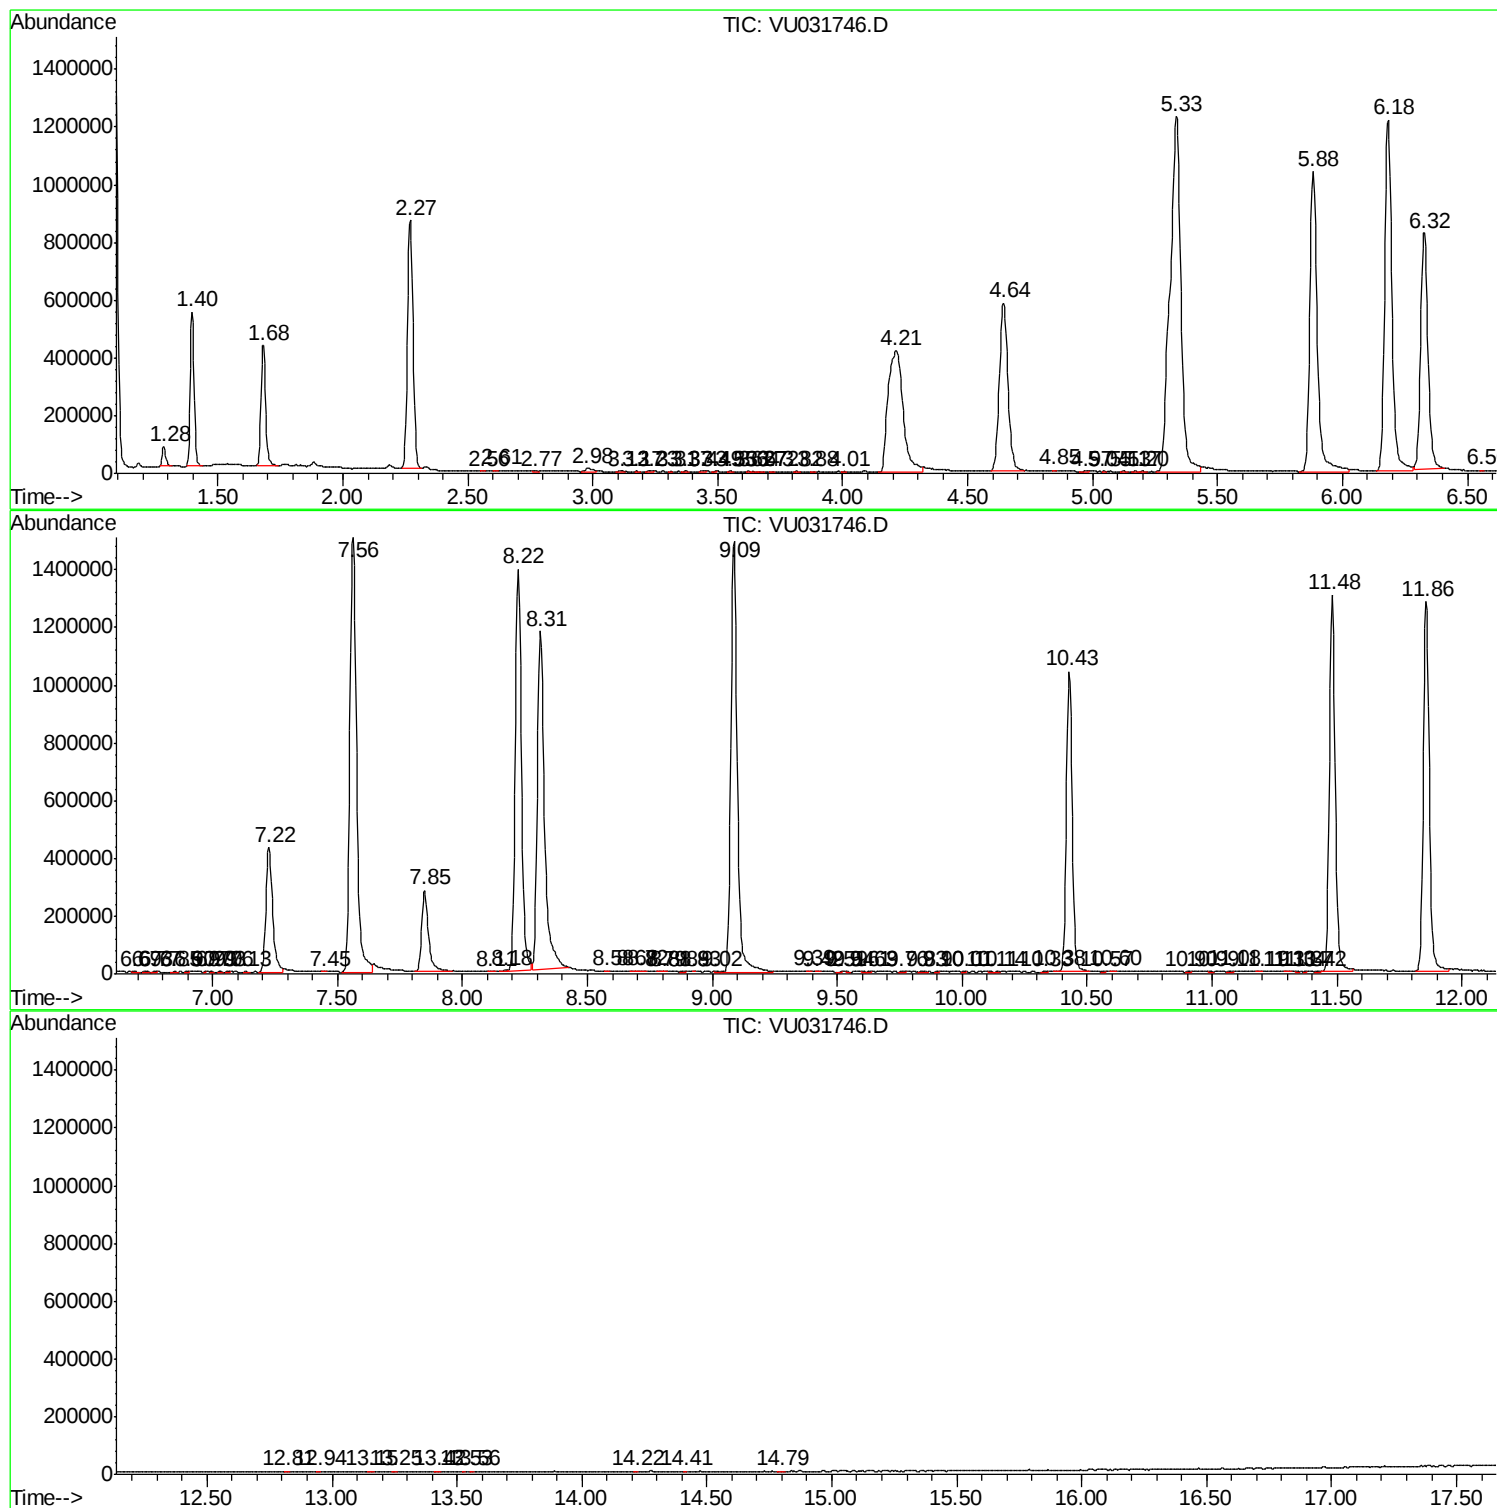

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031746.D
Acq On : 03 May 2019 13:44
Operator : JC/SP
Sample : K2661-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031746.D
Acq On : 03 May 2019 13:44
Operator : JC/SP
Sample : K2661-05 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B25

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc