

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031748.D
 Acq On : 03 May 2019 14:31
 Operator : JC/SP
 Sample : K2661-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	35	rVB3	14696	12994	0.07%	0.028%
2	1.395	88	95	108	rBV	537148	575961	3.17%	1.224%
3	1.682	176	184	196	rBV	402487	508410	2.80%	1.081%
4	2.270	357	367	381	rVV	855239	1303100	7.18%	2.769%
5	2.334	381	387	404	rVB6	16855	35932	0.20%	0.076%
6	2.788	524	528	531	rBV3	2255	2191	0.01%	0.005%
7	2.987	580	590	598	rBV3	5057	9238	0.05%	0.020%
8	3.103	622	626	629	rBV3	1321	1187	0.01%	0.003%
9	3.331	694	697	701	rVB2	1200	972	0.01%	0.002%
10	3.553	761	766	771	rVV	2414	2629	0.01%	0.006%
11	3.601	775	781	789	rBV3	1804	2580	0.01%	0.005%
12	3.707	811	814	819	rVB3	1283	889	0.00%	0.002%
13	3.778	830	836	839	rBV4	797	895	0.00%	0.002%
14	3.913	874	878	882	rVB2	1584	1460	0.01%	0.003%
15	3.939	882	886	889	rBV3	1029	825	0.00%	0.002%
16	3.958	889	892	900	rVB5	1100	1095	0.01%	0.002%
17	4.006	900	907	909	rBV3	1667	1832	0.01%	0.004%
18	4.022	909	912	916	rVB4	1542	1044	0.01%	0.002%
19	4.064	920	925	932	rVB6	873	1166	0.01%	0.002%
20	4.189	950	964	1002	rBV2	350862	1244193	6.86%	2.644%
21	4.643	1089	1105	1130	rBV	579197	1381116	7.61%	2.935%
22	4.887	1176	1181	1184	rBV6	2925	2220	0.01%	0.005%
23	4.907	1184	1187	1190	rVV4	1614	987	0.01%	0.002%
24	4.952	1197	1201	1203	rBV2	1473	1020	0.01%	0.002%
25	4.984	1205	1211	1218	rVV5	2072	2848	0.02%	0.006%
26	5.231	1285	1288	1292	rBV4	1060	1028	0.01%	0.002%
27	5.337	1297	1321	1363	rBV2	1228014	3712302	20.46%	7.890%
28	5.656	1417	1420	1422	rBV3	1331	828	0.00%	0.002%
29	5.681	1425	1428	1432	rVB6	2103	1543	0.01%	0.003%
30	5.723	1437	1441	1445	rBV6	2192	1920	0.01%	0.004%
31	5.884	1476	1491	1525	rBV	1007299	2105846	11.60%	4.475%
32	6.183	1570	1584	1611	rBV2	529431	1086644	5.99%	2.309%
33	6.328	1615	1629	1660	rVB	811748	1665556	9.18%	3.540%
34	6.559	1698	1701	1709	rVB6	1931	2083	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031748.D
 Acq On : 03 May 2019 14:31
 Operator : JC/SP
 Sample : K2661-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.601	1709	1714	1720	rBV6	1864	2774	0.02%	0.006%
36	6.784	1768	1771	1773	rBV5	1360	840	0.00%	0.002%
37	6.797	1773	1775	1780	rVB2	1528	1315	0.01%	0.003%
38	6.832	1780	1786	1790	rBV5	2075	2313	0.01%	0.005%
39	6.871	1793	1798	1801	rBV3	1945	1623	0.01%	0.003%
40	6.894	1801	1805	1807	rBV3	1323	968	0.01%	0.002%
41	6.948	1818	1822	1828	rBV7	1508	1575	0.01%	0.003%
42	7.225	1896	1908	1932	rBV	413859	799926	4.41%	1.700%
43	7.562	1999	2013	2029	rBV	1485830	2678356	14.76%	5.692%
44	7.849	2091	2102	2132	rBV	283698	530574	2.92%	1.128%
45	8.000	2146	2149	2151	rBV3	2259	1510	0.01%	0.003%
46	8.038	2159	2161	2166	rVB3	1393	1037	0.01%	0.002%
47	8.064	2166	2169	2177	rVB7	1847	2502	0.01%	0.005%
48	8.099	2177	2180	2184	rBV4	1718	1453	0.01%	0.003%
49	8.138	2189	2192	2194	rBV4	1697	1042	0.01%	0.002%
50	8.225	2196	2219	2237	rBV	10498629	18148232	100.00%	38.570%
51	8.308	2238	2245	2291	rVB	1261312	2607089	14.37%	5.541%
52	8.604	2335	2337	2341	rBV4	1347	1203	0.01%	0.003%
53	8.794	2389	2396	2400	rBV6	1518	2126	0.01%	0.005%
54	8.919	2433	2435	2440	rVB4	1969	1490	0.01%	0.003%
55	8.948	2440	2444	2448	rVB6	1399	1053	0.01%	0.002%
56	9.019	2463	2466	2470	rVB4	1712	1196	0.01%	0.003%
57	9.086	2470	2487	2527	rBV	1466846	2605406	14.36%	5.537%
58	9.266	2540	2543	2548	rVB7	1355	1358	0.01%	0.003%
59	9.398	2582	2584	2589	rVB3	1510	1224	0.01%	0.003%
60	9.447	2596	2599	2604	rVB5	1357	1084	0.01%	0.002%
61	9.469	2604	2606	2608	rBV2	1423	931	0.01%	0.002%
62	9.549	2626	2631	2632	rBV2	1145	875	0.00%	0.002%
63	9.562	2632	2635	2637	rVB2	1688	947	0.01%	0.002%
64	9.681	2668	2672	2678	rBV4	768	979	0.01%	0.002%
65	9.713	2680	2682	2688	rVB4	1874	1433	0.01%	0.003%
66	9.791	2701	2706	2710	rBV4	2231	1691	0.01%	0.004%
67	9.848	2720	2724	2728	rBV4	1178	1147	0.01%	0.002%
68	9.910	2740	2743	2746	rVB3	1885	1256	0.01%	0.003%
69	10.276	2854	2857	2859	rBV	1564	1065	0.01%	0.002%
70	10.308	2864	2867	2872	rVB3	1307	908	0.01%	0.002%
71	10.427	2889	2904	2922	rBV	1028945	1676148	9.24%	3.562%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031748.D
 Acq On : 03 May 2019 14:31
 Operator : JC/SP
 Sample : K2661-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B26

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.553	2940	2943	2949	rVB5	1988	1738	0.01%	0.004%
73	10.578	2949	2951	2952	rBV2	1919	953	0.01%	0.002%
74	10.604	2952	2959	2970	rVB4	10435	16636	0.09%	0.035%
75	10.723	2993	2996	3000	rVB3	1909	1629	0.01%	0.003%
76	10.797	3017	3019	3024	rVB4	1507	1142	0.01%	0.002%
77	10.819	3024	3026	3032	rBV3	1224	1139	0.01%	0.002%
78	10.852	3033	3036	3041	rVB4	1845	1221	0.01%	0.003%
79	11.035	3086	3093	3095	rBV4	1625	1668	0.01%	0.004%
80	11.051	3096	3098	3102	rVB3	1756	1051	0.01%	0.002%
81	11.080	3102	3107	3115	rBV8	1916	2550	0.01%	0.005%
82	11.122	3116	3120	3123	rBV2	1381	1217	0.01%	0.003%
83	11.176	3133	3137	3141	rBV4	1840	1658	0.01%	0.004%
84	11.479	3219	3231	3256	rBV	1280930	2103558	11.59%	4.471%
85	11.774	3321	3323	3325	rBV2	1864	1014	0.01%	0.002%
86	11.855	3335	3348	3366	rBV	1282639	2129887	11.74%	4.527%
87	12.157	3436	3442	3446	rVB6	3026	3810	0.02%	0.008%
88	12.183	3446	3450	3453	rBV4	1156	1283	0.01%	0.003%
89	12.237	3464	3467	3469	rBV3	1558	1047	0.01%	0.002%
90	12.279	3477	3480	3486	rVB6	1750	1487	0.01%	0.003%
91	12.443	3528	3531	3534	rBV5	1432	1006	0.01%	0.002%
92	12.655	3592	3597	3599	rBV5	1630	1647	0.01%	0.004%
93	12.781	3632	3636	3642	rVB4	2483	2832	0.02%	0.006%
94	12.810	3642	3645	3648	rBV2	1376	994	0.01%	0.002%
95	13.106	3728	3737	3743	rBV5	2651	3650	0.02%	0.008%
96	13.179	3758	3760	3764	rBV3	1795	1488	0.01%	0.003%
97	13.212	3768	3770	3773	rBV2	1714	1134	0.01%	0.002%
98	13.639	3901	3903	3909	rVB4	1374	1275	0.01%	0.003%
99	14.247	4089	4092	4093	rBV3	1861	1040	0.01%	0.002%
100	14.919	4299	4301	4309	rBV8	2318	2084	0.01%	0.004%


Sum of corrected areas: 47053021

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031748.D
Acq On : 03 May 2019 14:31
Operator : JC/SP
Sample : K2661-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

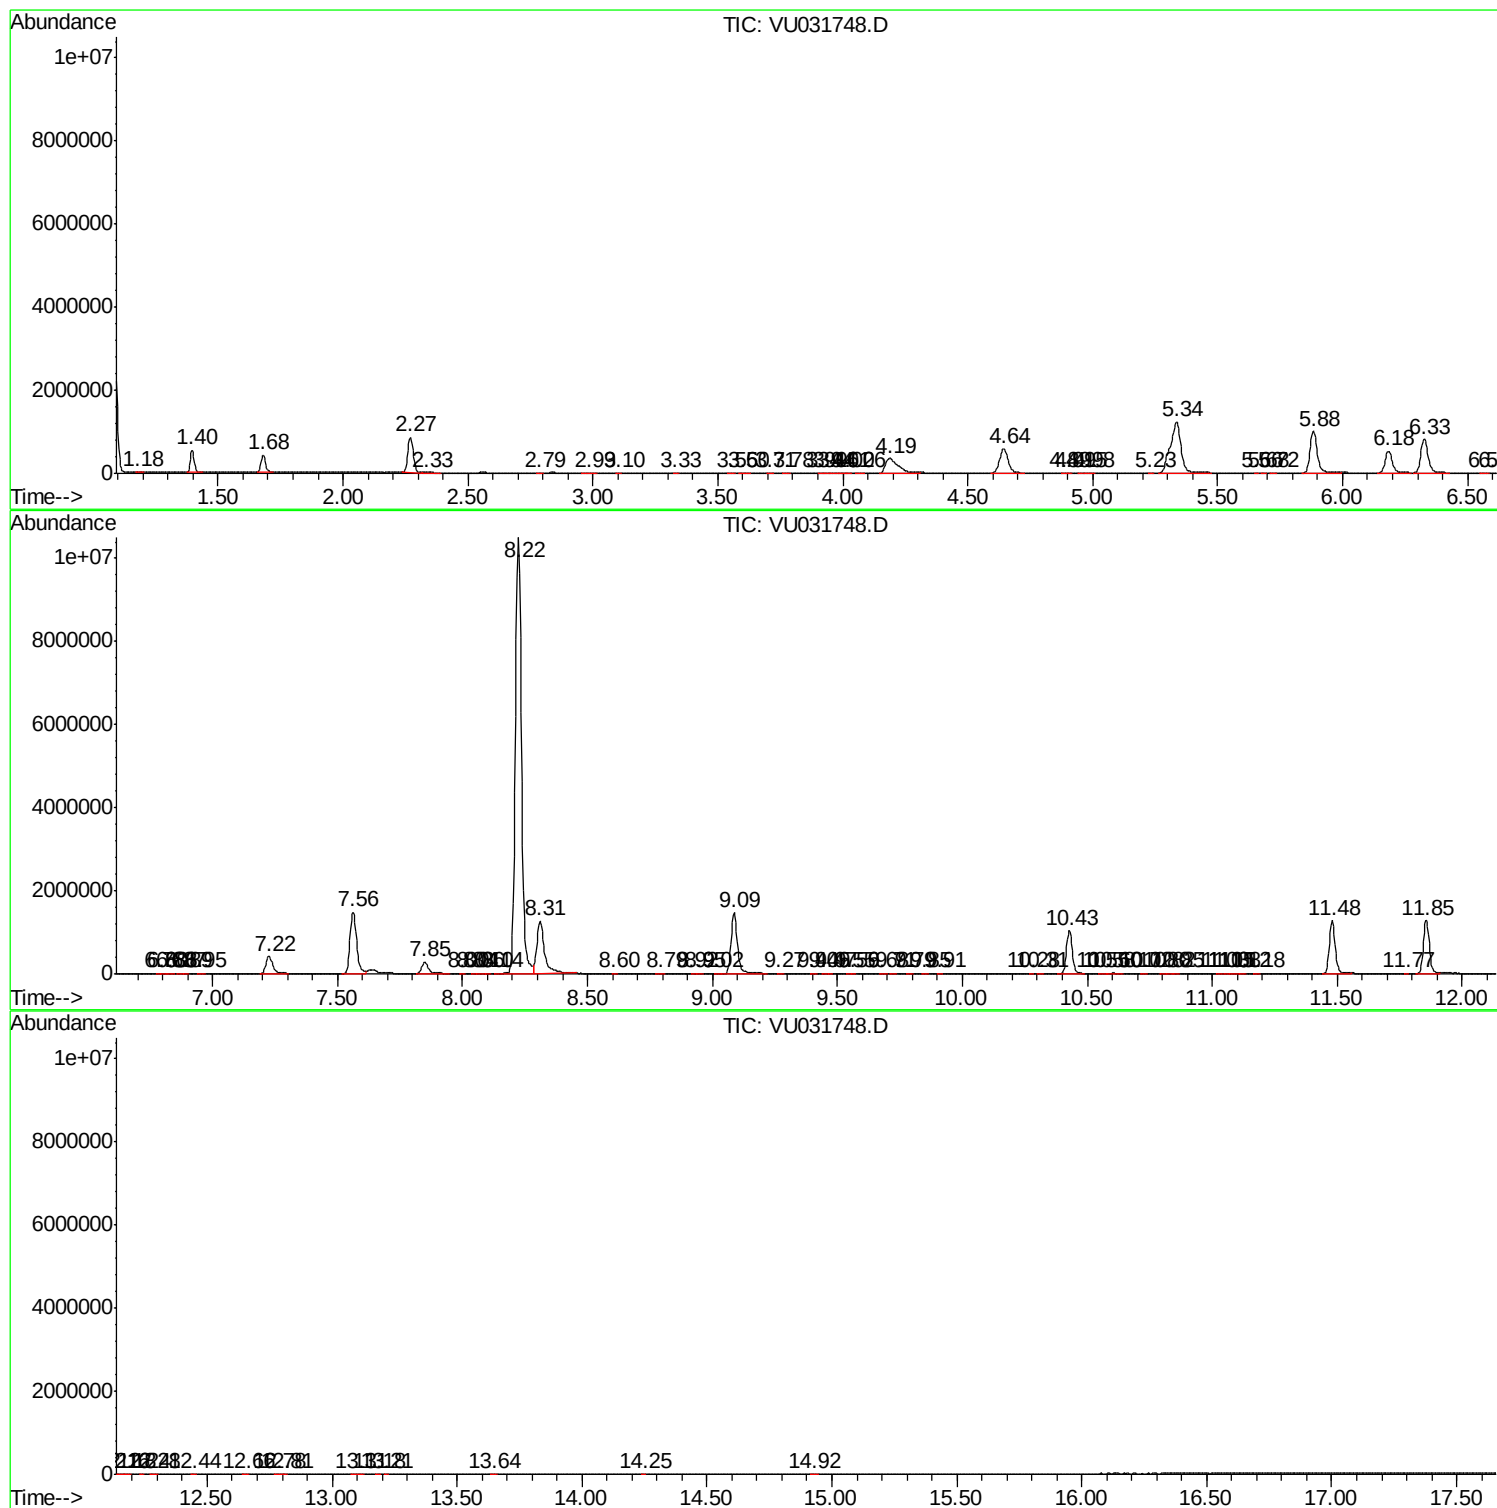

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031748.D
Acq On : 03 May 2019 14:31
Operator : JC/SP
Sample : K2661-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B26

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031748.D
Acq On : 03 May 2019 14:31
Operator : JC/SP
Sample : K2661-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B26

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc