

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031749.D
 Acq On : 03 May 2019 14:54
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	106	rBV	454213	487906	14.47%	1.930%
2	1.678	176	183	194	rBV	354591	434808	12.89%	1.720%
3	2.270	356	367	380	rBV	749232	1133442	33.61%	4.484%
4	2.447	419	422	424	rBV4	1410	973	0.03%	0.004%
5	2.514	440	443	445	rBV2	1215	834	0.02%	0.003%
6	2.569	457	460	463	rBV3	1842	1583	0.05%	0.006%
7	2.701	495	501	505	rBV5	4011	4652	0.14%	0.018%
8	2.762	516	520	522	rBV3	1132	1017	0.03%	0.004%
9	2.810	530	535	538	rBV5	966	938	0.03%	0.004%
10	2.868	551	553	555	rBV2	1431	772	0.02%	0.003%
11	2.897	559	562	566	rVB2	1099	818	0.02%	0.003%
12	2.945	573	577	579	rBV2	1453	1032	0.03%	0.004%
13	3.125	630	633	635	rBV2	799	545	0.02%	0.002%
14	3.219	660	662	666	rVB3	1786	1262	0.04%	0.005%
15	3.244	666	670	677	rBV2	1855	1920	0.06%	0.008%
16	3.280	677	681	685	rBV	1722	1632	0.05%	0.006%
17	3.341	697	700	707	rVB5	1963	2080	0.06%	0.008%
18	3.383	707	713	715	rBV4	1707	1580	0.05%	0.006%
19	3.428	724	727	728	rBV2	1262	593	0.02%	0.002%
20	3.508	750	752	756	rVB3	1007	723	0.02%	0.003%
21	3.547	761	764	770	rVB2	1933	2203	0.07%	0.009%
22	3.579	770	774	776	rBV3	1718	1256	0.04%	0.005%
23	3.604	780	782	785	rVB2	1294	689	0.02%	0.003%
24	3.627	785	789	795	rVB4	891	1010	0.03%	0.004%
25	3.720	812	818	820	rBV2	1374	1220	0.04%	0.005%
26	3.762	829	831	833	rBV2	937	530	0.02%	0.002%
27	3.807	842	845	848	rBV3	916	785	0.02%	0.003%
28	3.839	852	855	857	rBV2	908	629	0.02%	0.002%
29	3.926	879	882	885	rBV	1385	1073	0.03%	0.004%
30	3.955	888	891	892	rBV2	1086	579	0.02%	0.002%
31	3.968	892	895	898	rVV2	743	582	0.02%	0.002%
32	4.032	912	915	916	rBV	1044	609	0.02%	0.002%
33	4.067	923	926	927	rBV	818	539	0.02%	0.002%
34	4.093	931	934	938	rBV2	933	636	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031749.D
 Acq On : 03 May 2019 14:54
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.116	938	941	943	rBV2	859	514	0.02%	0.002%
36	4.186	950	963	1010	rBV	335583	1059724	31.42%	4.192%
37	4.643	1089	1105	1128	rBV	531615	1280905	37.98%	5.067%
38	4.942	1194	1198	1203	rBV6	2160	2379	0.07%	0.009%
39	4.981	1203	1210	1211	rBV6	2230	2379	0.07%	0.009%
40	4.990	1211	1213	1216	rBV3	1491	879	0.03%	0.003%
41	5.093	1242	1245	1249	rBV3	1540	1584	0.05%	0.006%
42	5.170	1264	1269	1271	rBV4	1521	1423	0.04%	0.006%
43	5.247	1290	1293	1297	rBV2	718	644	0.02%	0.003%
44	5.334	1297	1320	1358	rBV2	1100380	3372605	100.00%	13.342%
45	5.637	1412	1414	1417	rBV3	1433	673	0.02%	0.003%
46	5.791	1460	1462	1465	rBV2	1299	752	0.02%	0.003%
47	5.829	1471	1474	1476	rBV2	899	522	0.02%	0.002%
48	5.884	1477	1491	1521	rBV	937176	1930268	57.23%	7.636%
49	6.180	1572	1583	1600	rVB	13532	32546	0.97%	0.129%
50	6.325	1613	1628	1655	rBV	760402	1568264	46.50%	6.204%
51	6.640	1723	1726	1731	rVB3	1544	1324	0.04%	0.005%
52	6.723	1749	1752	1755	rBV5	1355	736	0.02%	0.003%
53	6.781	1767	1770	1774	rVB5	935	603	0.02%	0.002%
54	6.820	1779	1782	1786	rBV3	1353	1248	0.04%	0.005%
55	6.845	1786	1790	1795	rVB4	1619	1611	0.05%	0.006%
56	6.874	1796	1799	1801	rBV3	1344	745	0.02%	0.003%
57	6.890	1801	1804	1805	rBV2	1246	693	0.02%	0.003%
58	6.981	1830	1832	1835	rVB2	1245	684	0.02%	0.003%
59	7.003	1835	1839	1842	rVB5	1364	1035	0.03%	0.004%
60	7.138	1879	1881	1888	rVB4	1952	1643	0.05%	0.006%
61	7.170	1889	1891	1895	rVB3	1208	683	0.02%	0.003%
62	7.225	1895	1908	1941	rBV	387680	753018	22.33%	2.979%
63	7.562	2000	2013	2059	rBV	1301390	2463962	73.06%	9.748%
64	7.849	2091	2102	2127	rBV	253944	482415	14.30%	1.908%
65	8.170	2197	2202	2207	rBV5	3033	3316	0.10%	0.013%
66	8.228	2211	2220	2234	rBV5	26810	49006	1.45%	0.194%
67	8.308	2235	2245	2285	rBV	1123623	2224333	65.95%	8.800%
68	8.714	2368	2371	2374	rBV5	1861	1228	0.04%	0.005%
69	8.797	2393	2397	2400	rVB3	1504	1141	0.03%	0.005%
70	8.816	2400	2403	2405	rBV4	1425	791	0.02%	0.003%
71	9.035	2466	2471	2472	rBV3	1989	1987	0.06%	0.008%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031749.D
 Acq On : 03 May 2019 14:54
 Operator : JC/SP
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.087	2474	2487	2531	rVV	1351093	2391259	70.90%	9.460%
73	9.543	2627	2629	2631	rBV3	1307	720	0.02%	0.003%
74	9.617	2649	2652	2656	rBV5	820	701	0.02%	0.003%
75	9.948	2752	2755	2758	rBV2	1577	1030	0.03%	0.004%
76	10.000	2768	2771	2773	rVB	1091	588	0.02%	0.002%
77	10.016	2773	2776	2777	rBV2	1698	880	0.03%	0.003%
78	10.167	2817	2823	2824	rBV4	2595	2285	0.07%	0.009%
79	10.331	2871	2874	2876	rBV2	1441	965	0.03%	0.004%
80	10.427	2891	2904	2937	rBV	1009611	1642550	48.70%	6.498%
81	10.543	2937	2940	2941	rBV3	1646	997	0.03%	0.004%
82	10.588	2949	2954	2955	rBV3	2592	2137	0.06%	0.008%
83	10.685	2981	2984	2988	rBV4	1571	1230	0.04%	0.005%
84	10.775	3007	3012	3016	rBV2	2131	2174	0.06%	0.009%
85	10.813	3022	3024	3028	rBV3	806	769	0.02%	0.003%
86	10.894	3045	3049	3050	rBV2	1324	1078	0.03%	0.004%
87	10.948	3063	3066	3068	rBV2	1392	735	0.02%	0.003%
88	10.964	3068	3071	3072	rBV2	1011	543	0.02%	0.002%
89	11.048	3095	3097	3099	rBV	1240	556	0.02%	0.002%
90	11.083	3106	3108	3111	rBV2	1435	932	0.03%	0.004%
91	11.131	3120	3123	3126	rBV3	1010	844	0.03%	0.003%
92	11.160	3129	3132	3134	rBV2	1076	635	0.02%	0.003%
93	11.244	3154	3158	3161	rBV2	1527	1146	0.03%	0.005%
94	11.305	3174	3177	3180	rBV3	1480	1009	0.03%	0.004%
95	11.331	3183	3185	3188	rVV4	1341	745	0.02%	0.003%
96	11.479	3220	3231	3254	rBV	1160044	1908268	56.58%	7.549%
97	11.855	3336	3348	3377	rBV	1169059	1968229	58.36%	7.787%
98	12.122	3427	3431	3434	rBV4	2800	2416	0.07%	0.010%
99	13.080	3726	3729	3734	rBV3	1999	1337	0.04%	0.005%
100	13.131	3742	3745	3747	rBV2	1464	756	0.02%	0.003%


Sum of corrected areas: 25277227

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031749.D
Acq On : 03 May 2019 14:54
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

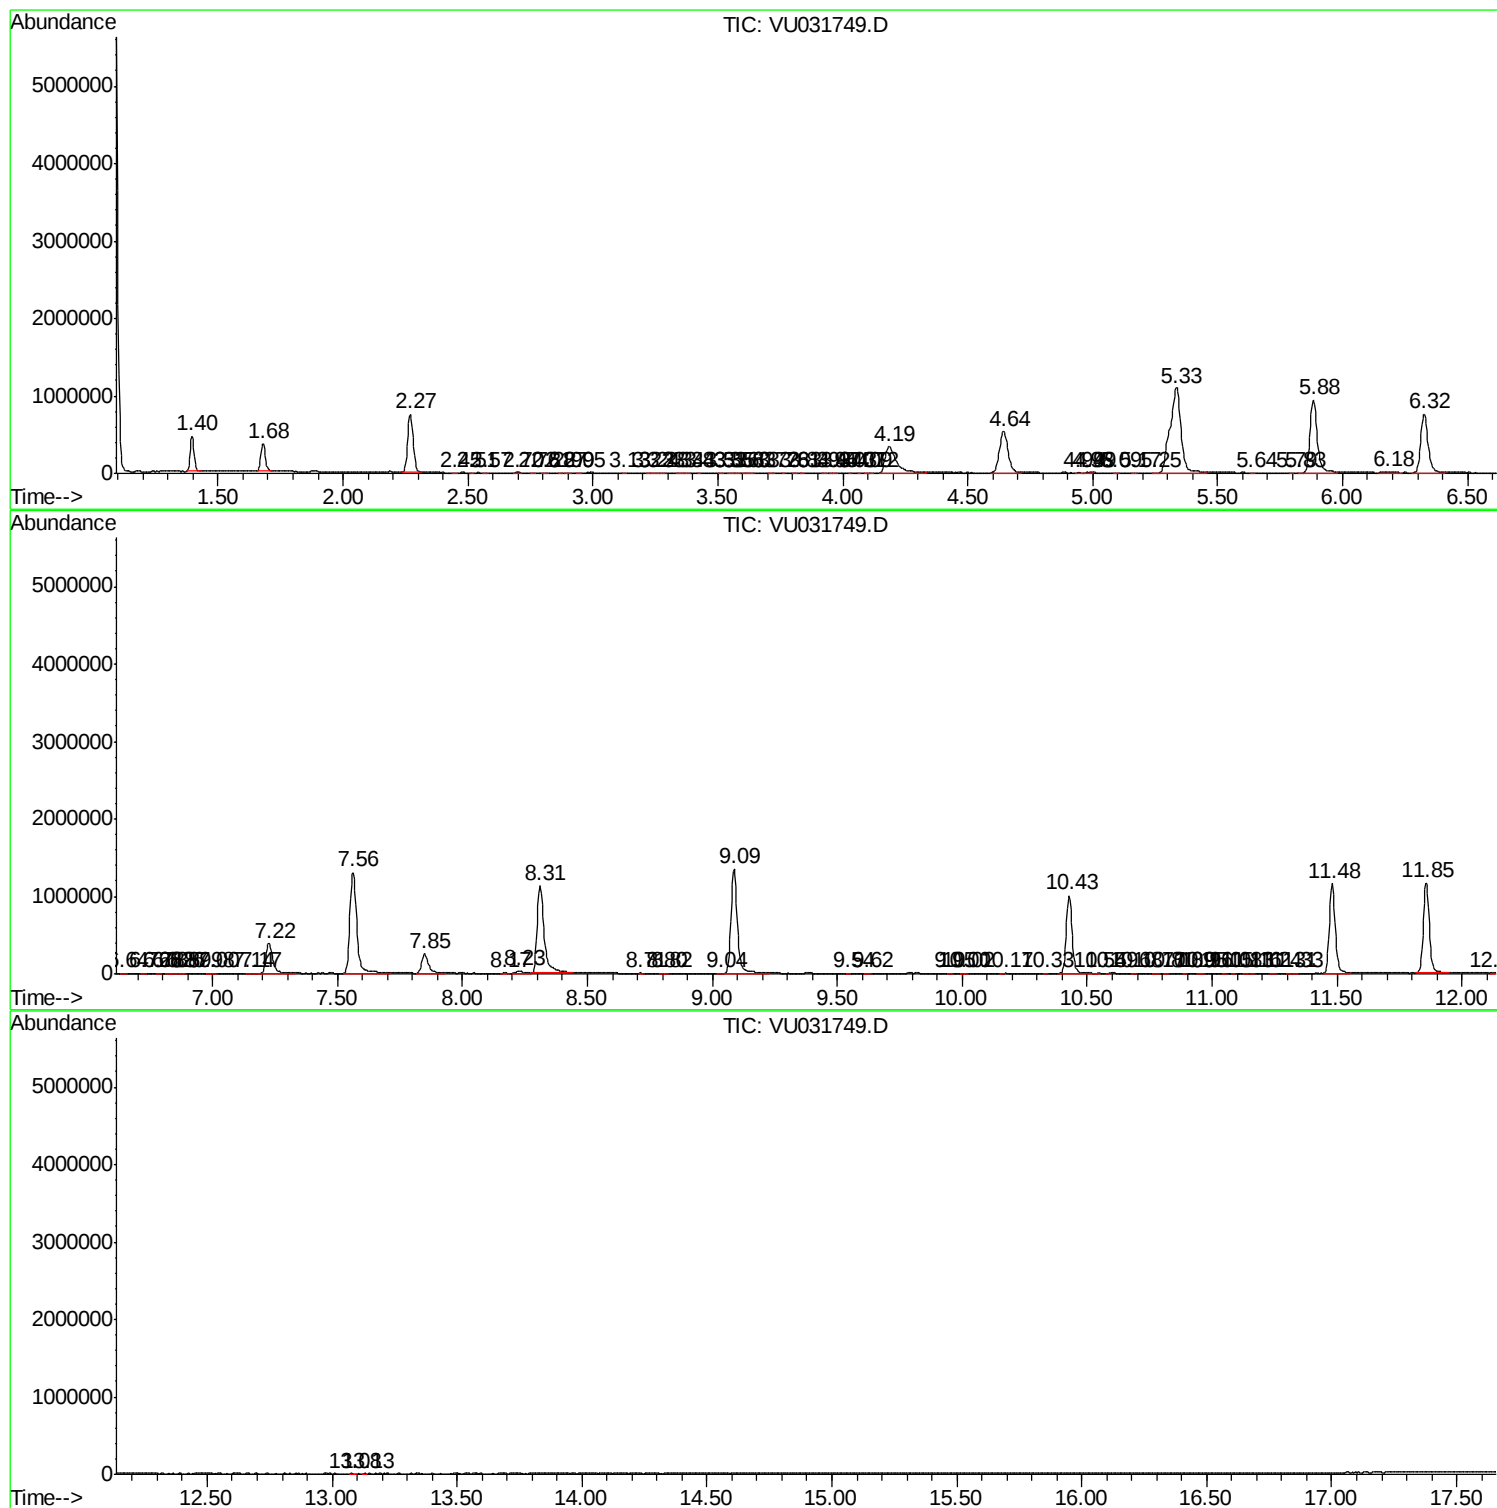

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031749.D
Acq On : 03 May 2019 14:54
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031749.D
Acq On : 03 May 2019 14:54
Operator : JC/SP
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc