

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031758.D
 Acq On : 03 May 2019 18:23
 Operator : JC/SP
 Sample : K2695-04 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	34	rVB	12756	9969	0.30%	0.040%
2	1.396	88	95	111	rBV	466562	511368	15.39%	2.027%
3	1.679	176	183	196	rVB	354925	445883	13.42%	1.768%
4	2.270	356	367	380	rBV	765431	1158076	34.85%	4.591%
5	2.470	425	429	432	rBV5	2766	1732	0.05%	0.007%
6	2.527	443	447	449	rBV	1741	1532	0.05%	0.006%
7	2.601	468	470	477	rVB5	1740	1561	0.05%	0.006%
8	2.633	477	480	485	rBV3	1689	1563	0.05%	0.006%
9	2.691	494	498	499	rBV3	2143	1501	0.05%	0.006%
10	2.849	540	547	552	rBV6	1931	2086	0.06%	0.008%
11	2.978	584	587	590	rVB3	1678	1013	0.03%	0.004%
12	3.132	632	635	640	rBV4	1336	1278	0.04%	0.005%
13	3.170	643	647	651	rBV3	1009	1006	0.03%	0.004%
14	3.222	659	663	667	rVB2	1481	1382	0.04%	0.005%
15	3.251	667	672	674	rBV3	1643	1514	0.05%	0.006%
16	3.309	684	690	697	rVB4	1833	2297	0.07%	0.009%
17	3.450	731	734	739	rVB2	1373	972	0.03%	0.004%
18	3.511	749	753	757	rBV3	1360	1009	0.03%	0.004%
19	3.605	777	782	783	rBV2	1121	988	0.03%	0.004%
20	3.695	803	810	813	rVB4	1302	1250	0.04%	0.005%
21	3.794	838	841	847	rVB4	1492	1308	0.04%	0.005%
22	3.823	847	850	855	rBV4	1719	1822	0.05%	0.007%
23	3.859	855	861	865	rVV3	1326	1443	0.04%	0.006%
24	3.916	875	879	881	rBV3	955	885	0.03%	0.004%
25	3.990	895	902	905	rVB3	1102	1205	0.04%	0.005%
26	4.019	908	911	917	rVB6	1201	1086	0.03%	0.004%
27	4.087	929	932	940	rBV3	1020	1268	0.04%	0.005%
28	4.190	951	964	1010	rBV	302963	1005068	30.25%	3.984%
29	4.643	1087	1105	1129	rBV	529885	1280458	38.53%	5.076%
30	4.955	1199	1202	1205	rBV3	1632	1207	0.04%	0.005%
31	5.087	1241	1243	1246	rVB	1872	999	0.03%	0.004%
32	5.138	1254	1259	1262	rBV3	1579	1466	0.04%	0.006%
33	5.215	1278	1283	1288	rBV5	951	1139	0.03%	0.005%
34	5.334	1297	1320	1346	rBV2	1099152	3323079	100.00%	13.174%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031758.D
 Acq On : 03 May 2019 18:23
 Operator : JC/SP
 Sample : K2695-04 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.736	1440	1445	1450	rVB7	1803	2227	0.07%	0.009%
36	5.765	1450	1454	1458	rBV3	1957	1728	0.05%	0.007%
37	5.788	1458	1461	1463	rVV3	2460	937	0.03%	0.004%
38	5.823	1469	1472	1475	rVB4	1679	1043	0.03%	0.004%
39	5.884	1475	1491	1512	rBV	960994	1957946	58.92%	7.762%
40	6.132	1565	1568	1571	rBV4	1560	957	0.03%	0.004%
41	6.183	1572	1584	1605	rBV3	165322	355000	10.68%	1.407%
42	6.328	1615	1629	1660	rBV	746879	1521319	45.78%	6.031%
43	6.521	1686	1689	1694	rBV6	1346	1421	0.04%	0.006%
44	6.543	1694	1696	1701	rVB4	1725	1404	0.04%	0.006%
45	6.572	1701	1705	1711	rVB7	1523	1734	0.05%	0.007%
46	6.601	1711	1714	1716	rBV3	1484	1001	0.03%	0.004%
47	6.659	1728	1732	1735	rBV5	1037	937	0.03%	0.004%
48	6.733	1751	1755	1758	rVB3	1637	1284	0.04%	0.005%
49	6.759	1758	1763	1768	rBV3	1829	1770	0.05%	0.007%
50	6.977	1827	1831	1837	rVB5	1389	1445	0.04%	0.006%
51	7.071	1857	1860	1864	rVB2	1588	1160	0.03%	0.005%
52	7.103	1868	1870	1874	rBV3	1537	1110	0.03%	0.004%
53	7.164	1881	1889	1894	rBV7	1216	1937	0.06%	0.008%
54	7.225	1895	1908	1941	rBV	366272	717837	21.60%	2.846%
55	7.563	1998	2013	2034	rBV	1312968	2402930	72.31%	9.526%
56	7.849	2091	2102	2124	rBV	249444	463828	13.96%	1.839%
57	8.132	2188	2190	2195	rVB4	1807	1291	0.04%	0.005%
58	8.164	2196	2200	2205	rBV5	1405	1631	0.05%	0.006%
59	8.228	2210	2220	2230	rBV7	13807	24066	0.72%	0.095%
60	8.312	2234	2246	2281	rBV	1070718	2135158	64.25%	8.464%
61	8.775	2383	2390	2394	rVB6	1570	2170	0.07%	0.009%
62	8.804	2394	2399	2404	rBV7	1832	2358	0.07%	0.009%
63	8.887	2420	2425	2428	rBV4	1284	1436	0.04%	0.006%
64	9.087	2474	2487	2530	rBV	1369749	2437892	73.36%	9.665%
65	9.315	2554	2558	2564	rVB6	1573	1571	0.05%	0.006%
66	9.402	2581	2585	2588	rBV3	1188	1062	0.03%	0.004%
67	9.463	2601	2604	2607	rBV2	1898	1230	0.04%	0.005%
68	9.607	2644	2649	2652	rVV2	1526	1589	0.05%	0.006%
69	9.720	2680	2684	2687	rBV4	1420	1188	0.04%	0.005%
70	9.987	2764	2767	2771	rVB3	1331	1031	0.03%	0.004%
71	10.019	2771	2777	2779	rBV3	1189	1225	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031758.D
 Acq On : 03 May 2019 18:23
 Operator : JC/SP
 Sample : K2695-04 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X89

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.077	2790	2795	2799	rBV5	1824	2325	0.07%	0.009%
73	10.231	2839	2843	2845	rBV3	1572	1097	0.03%	0.004%
74	10.286	2857	2860	2865	rVB4	1864	1794	0.05%	0.007%
75	10.427	2890	2904	2931	rBV	963396	1576536	47.44%	6.250%
76	10.720	2992	2995	3002	rVB4	1844	1894	0.06%	0.008%
77	10.778	3010	3013	3017	rVB4	1294	922	0.03%	0.004%
78	10.800	3017	3020	3022	rBV3	1620	1042	0.03%	0.004%
79	10.894	3046	3049	3054	rBV3	1092	1017	0.03%	0.004%
80	10.987	3073	3078	3080	rBV2	1820	1660	0.05%	0.007%
81	11.087	3105	3109	3113	rVB5	2276	2364	0.07%	0.009%
82	11.112	3113	3117	3122	rBV3	1682	1805	0.05%	0.007%
83	11.157	3128	3131	3139	rVB4	1180	1053	0.03%	0.004%
84	11.209	3143	3147	3152	rBV6	1976	1901	0.06%	0.008%
85	11.251	3158	3160	3164	rBV2	1615	1187	0.04%	0.005%
86	11.305	3170	3177	3181	rBV6	2203	2786	0.08%	0.011%
87	11.479	3219	3231	3253	rBV	1159506	1906155	57.36%	7.557%
88	11.855	3336	3348	3373	rBV	1096714	1870022	56.27%	7.413%
89	12.350	3499	3502	3503	rBV2	1787	1009	0.03%	0.004%
90	12.476	3538	3541	3551	rVB6	4823	5746	0.17%	0.023%
91	12.668	3598	3601	3607	rBV5	1722	1845	0.06%	0.007%
92	12.890	3667	3670	3676	rBV4	1074	945	0.03%	0.004%
93	13.080	3723	3729	3734	rBV3	2540	3425	0.10%	0.014%
94	13.170	3752	3757	3761	rBV5	2497	3050	0.09%	0.012%
95	13.485	3852	3855	3858	rBV4	1238	956	0.03%	0.004%
96	13.575	3879	3883	3884	rBV2	1407	1024	0.03%	0.004%
97	13.755	3936	3939	3942	rBV3	1461	1225	0.04%	0.005%
98	13.955	3999	4001	4006	rVB2	1836	1447	0.04%	0.006%
99	13.987	4006	4011	4013	rBV2	1943	1553	0.05%	0.006%
100	14.096	4042	4045	4046	rBV2	1486	928	0.03%	0.004%


Sum of corrected areas: 25224979

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031758.D
Acq On : 03 May 2019 18:23
Operator : JC/SP
Sample : K2695-04 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X89

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

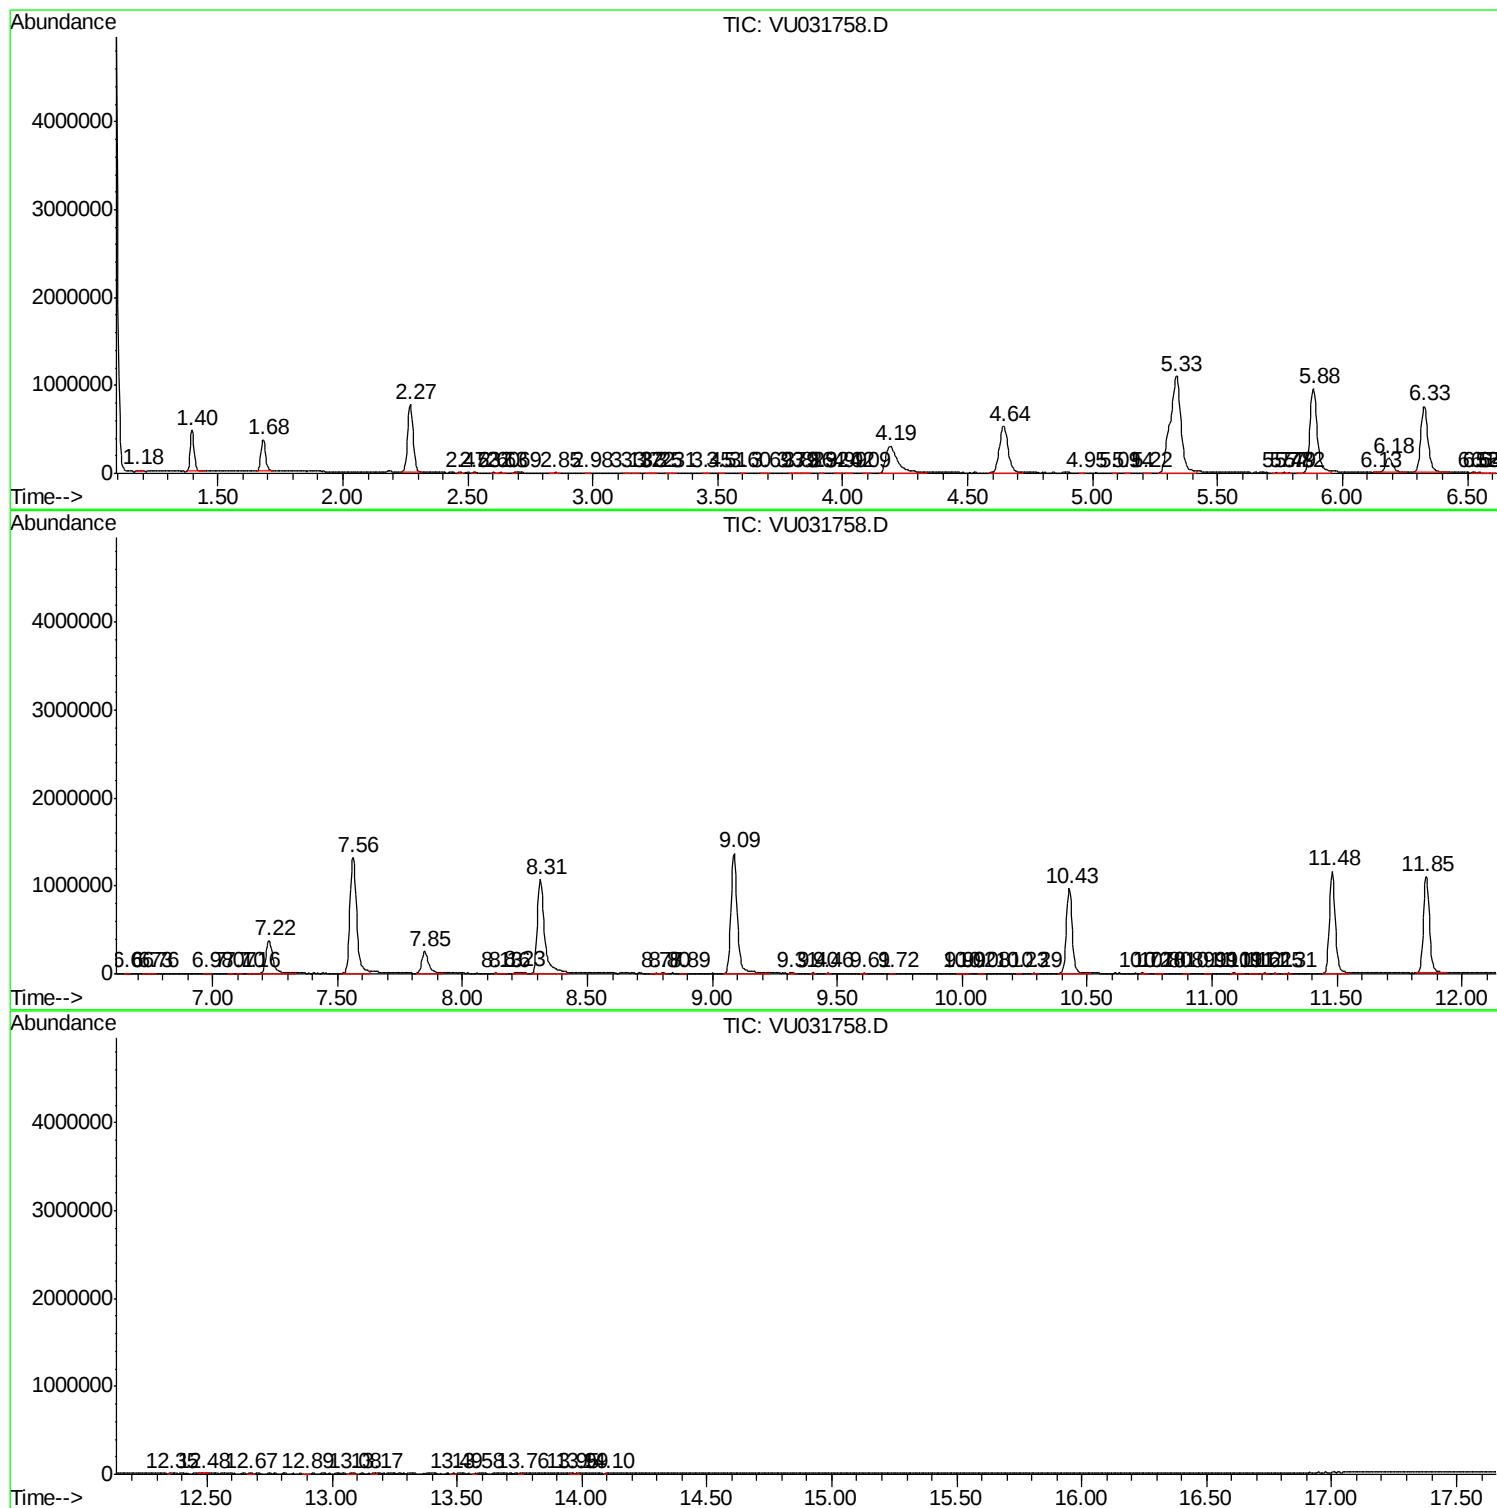

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031758.D
Acq On : 03 May 2019 18:23
Operator : JC/SP
Sample : K2695-04 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X89

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031758.D
Acq On : 03 May 2019 18:23
Operator : JC/SP
Sample : K2695-04 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X89

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc