

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031759.D
 Acq On : 03 May 2019 18:46
 Operator : JC/SP
 Sample : K2695-05 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.396	88	95	109	rBV	490863	529526	15.10%	2.036%
2	1.679	176	183	196	rBV	373151	460753	13.14%	1.772%
3	2.270	356	367	381	rBV	808680	1219133	34.76%	4.688%
4	2.441	417	420	423	rVB2	1426	946	0.03%	0.004%
5	2.556	454	456	460	rBV6	1197	855	0.02%	0.003%
6	2.691	495	498	500	rBV3	2627	1890	0.05%	0.007%
7	2.752	515	517	521	rVB3	1646	1133	0.03%	0.004%
8	2.775	521	524	526	rBV3	1432	873	0.02%	0.003%
9	2.788	526	528	535	rVB4	1165	1128	0.03%	0.004%
10	3.077	612	618	620	rBV3	1598	1396	0.04%	0.005%
11	3.177	641	649	653	rBV4	1036	1665	0.05%	0.006%
12	3.302	685	688	691	rBV2	1013	872	0.02%	0.003%
13	3.360	702	706	711	rBV3	1493	1690	0.05%	0.006%
14	3.386	712	714	717	rVV2	1717	1453	0.04%	0.006%
15	3.418	721	724	728	rVB	1293	973	0.03%	0.004%
16	3.441	728	731	735	rBV	1135	1026	0.03%	0.004%
17	3.518	750	755	756	rBV2	1188	998	0.03%	0.004%
18	3.659	797	799	805	rVB3	1267	874	0.02%	0.003%
19	3.768	830	833	838	rVB2	918	756	0.02%	0.003%
20	3.794	838	841	844	rVB3	1214	875	0.02%	0.003%
21	3.817	844	848	851	rBV2	1554	1299	0.04%	0.005%
22	3.904	872	875	877	rBV3	1297	858	0.02%	0.003%
23	3.920	877	880	883	rVV2	1334	1129	0.03%	0.004%
24	3.974	892	897	901	rBV4	1057	1215	0.03%	0.005%
25	4.055	918	922	924	rBV2	1198	880	0.03%	0.003%
26	4.186	950	963	998	rBV	334680	1039285	29.63%	3.996%
27	4.518	1063	1066	1068	rBV5	1744	871	0.02%	0.003%
28	4.572	1080	1083	1086	rBV4	1320	920	0.03%	0.004%
29	4.643	1088	1105	1134	rVV	558378	1352812	38.57%	5.202%
30	4.878	1175	1178	1181	rBV3	1495	1022	0.03%	0.004%
31	4.971	1204	1207	1210	rBV3	1316	1141	0.03%	0.004%
32	5.003	1215	1217	1221	rVV3	2366	1385	0.04%	0.005%
33	5.116	1249	1252	1255	rVB3	1642	1058	0.03%	0.004%
34	5.154	1255	1264	1269	rBV5	1668	2676	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031759.D
 Acq On : 03 May 2019 18:46
 Operator : JC/SP
 Sample : K2695-05 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.199	1274	1278	1281	rVB5	901	793	0.02%	0.003%
36	5.222	1281	1285	1290	rBV4	1488	1254	0.04%	0.005%
37	5.334	1296	1320	1350	rBV2	1168441	3507223	100.00%	13.486%
38	5.672	1421	1425	1430	rBV6	2388	2379	0.07%	0.009%
39	5.797	1461	1464	1466	rBV3	1460	844	0.02%	0.003%
40	5.813	1466	1469	1472	rVV4	1250	846	0.02%	0.003%
41	5.881	1477	1490	1518	rBV	973339	2016688	57.50%	7.755%
42	6.186	1572	1585	1596	rBV	18349	42890	1.22%	0.165%
43	6.325	1615	1628	1655	rBV	770251	1599974	45.62%	6.152%
44	6.556	1698	1700	1704	rVB3	1606	859	0.02%	0.003%
45	6.723	1749	1752	1755	rVB4	1436	940	0.03%	0.004%
46	6.746	1755	1759	1763	rBV4	1507	1159	0.03%	0.004%
47	6.874	1794	1799	1805	rBV6	1545	1830	0.05%	0.007%
48	6.987	1830	1834	1837	rVV4	1169	889	0.03%	0.003%
49	7.003	1837	1839	1844	rVB2	1358	940	0.03%	0.004%
50	7.067	1855	1859	1860	rBV	1248	1006	0.03%	0.004%
51	7.225	1893	1908	1935	rBV	392859	749460	21.37%	2.882%
52	7.376	1951	1955	1957	rVB4	1178	784	0.02%	0.003%
53	7.563	1999	2013	2064	rBV	1386577	2601704	74.18%	10.004%
54	7.849	2091	2102	2131	rBV	262068	499308	14.24%	1.920%
55	7.984	2139	2144	2146	rBV4	1725	1628	0.05%	0.006%
56	8.154	2193	2197	2201	rBV6	800	845	0.02%	0.003%
57	8.225	2214	2219	2223	rBV5	2939	3342	0.10%	0.013%
58	8.312	2234	2246	2283	rBV	1148558	2257998	64.38%	8.683%
59	8.643	2347	2349	2351	rBV3	1389	866	0.02%	0.003%
60	8.797	2392	2397	2400	rBV5	2178	1912	0.05%	0.007%
61	8.816	2400	2403	2407	rVB4	1232	911	0.03%	0.004%
62	8.926	2434	2437	2441	rBV4	1092	1126	0.03%	0.004%
63	9.035	2463	2471	2474	rBV7	1787	2914	0.08%	0.011%
64	9.087	2474	2487	2514	rBV	1421134	2464976	70.28%	9.479%
65	9.289	2547	2550	2553	rBV3	1646	1406	0.04%	0.005%
66	9.437	2593	2596	2600	rBV4	1925	1643	0.05%	0.006%
67	9.569	2632	2637	2639	rBV4	1580	1240	0.04%	0.005%
68	9.926	2745	2748	2753	rVB2	1973	1506	0.04%	0.006%
69	10.003	2766	2772	2774	rBV5	1224	1213	0.03%	0.005%
70	10.022	2774	2778	2783	rVV2	1547	1580	0.05%	0.006%
71	10.067	2788	2792	2795	rBV3	1691	1734	0.05%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031759.D
 Acq On : 03 May 2019 18:46
 Operator : JC/SP
 Sample : K2695-05 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.135	2810	2813	2818	rVB6	1300	1237	0.04%	0.005%
73	10.215	2833	2838	2842	rVB5	1923	2022	0.06%	0.008%
74	10.241	2842	2846	2849	rBV3	1111	987	0.03%	0.004%
75	10.257	2849	2851	2856	rVB	1455	1165	0.03%	0.004%
76	10.289	2856	2861	2864	rBV2	2788	2414	0.07%	0.009%
77	10.427	2891	2904	2930	rBV	1007719	1641466	46.80%	6.312%
78	10.540	2936	2939	2943	rBV2	1491	1196	0.03%	0.005%
79	10.636	2967	2969	2974	rBV3	1141	792	0.02%	0.003%
80	10.749	3000	3004	3009	rBV6	1544	1400	0.04%	0.005%
81	10.935	3059	3062	3066	rBV3	1400	1261	0.04%	0.005%
82	11.032	3088	3092	3095	rBV4	1853	1283	0.04%	0.005%
83	11.238	3148	3156	3159	rBV5	1588	1955	0.06%	0.008%
84	11.279	3166	3169	3172	rBV3	1386	1105	0.03%	0.004%
85	11.341	3186	3188	3194	rVB3	1512	1167	0.03%	0.004%
86	11.479	3220	3231	3258	rBV	1188348	1947843	55.54%	7.490%
87	11.858	3336	3349	3379	rBV	1150869	1964589	56.02%	7.554%
88	12.315	3486	3491	3495	rBV3	1792	2104	0.06%	0.008%
89	12.424	3523	3525	3527	rBV2	1537	883	0.03%	0.003%
90	12.543	3557	3562	3565	rBV4	1247	1187	0.03%	0.005%
91	12.951	3686	3689	3690	rBV2	1597	925	0.03%	0.004%
92	13.009	3702	3707	3711	rBV4	1649	1769	0.05%	0.007%
93	13.369	3814	3819	3824	rBV4	1544	1777	0.05%	0.007%
94	13.511	3858	3863	3864	rBV3	1242	1170	0.03%	0.004%
95	13.520	3864	3866	3871	rVB4	2209	1743	0.05%	0.007%
96	14.154	4058	4063	4070	rBV5	2805	3620	0.10%	0.014%
97	14.189	4071	4074	4076	rBV	1501	1018	0.03%	0.004%
98	14.234	4085	4088	4090	rBV3	1525	1045	0.03%	0.004%
99	14.729	4239	4242	4243	rBV3	1994	1133	0.03%	0.004%
100	14.887	4288	4291	4295	rBV4	1708	1562	0.04%	0.006%


Sum of corrected areas: 26005794

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031759.D
Acq On : 03 May 2019 18:46
Operator : JC/SP
Sample : K2695-05 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

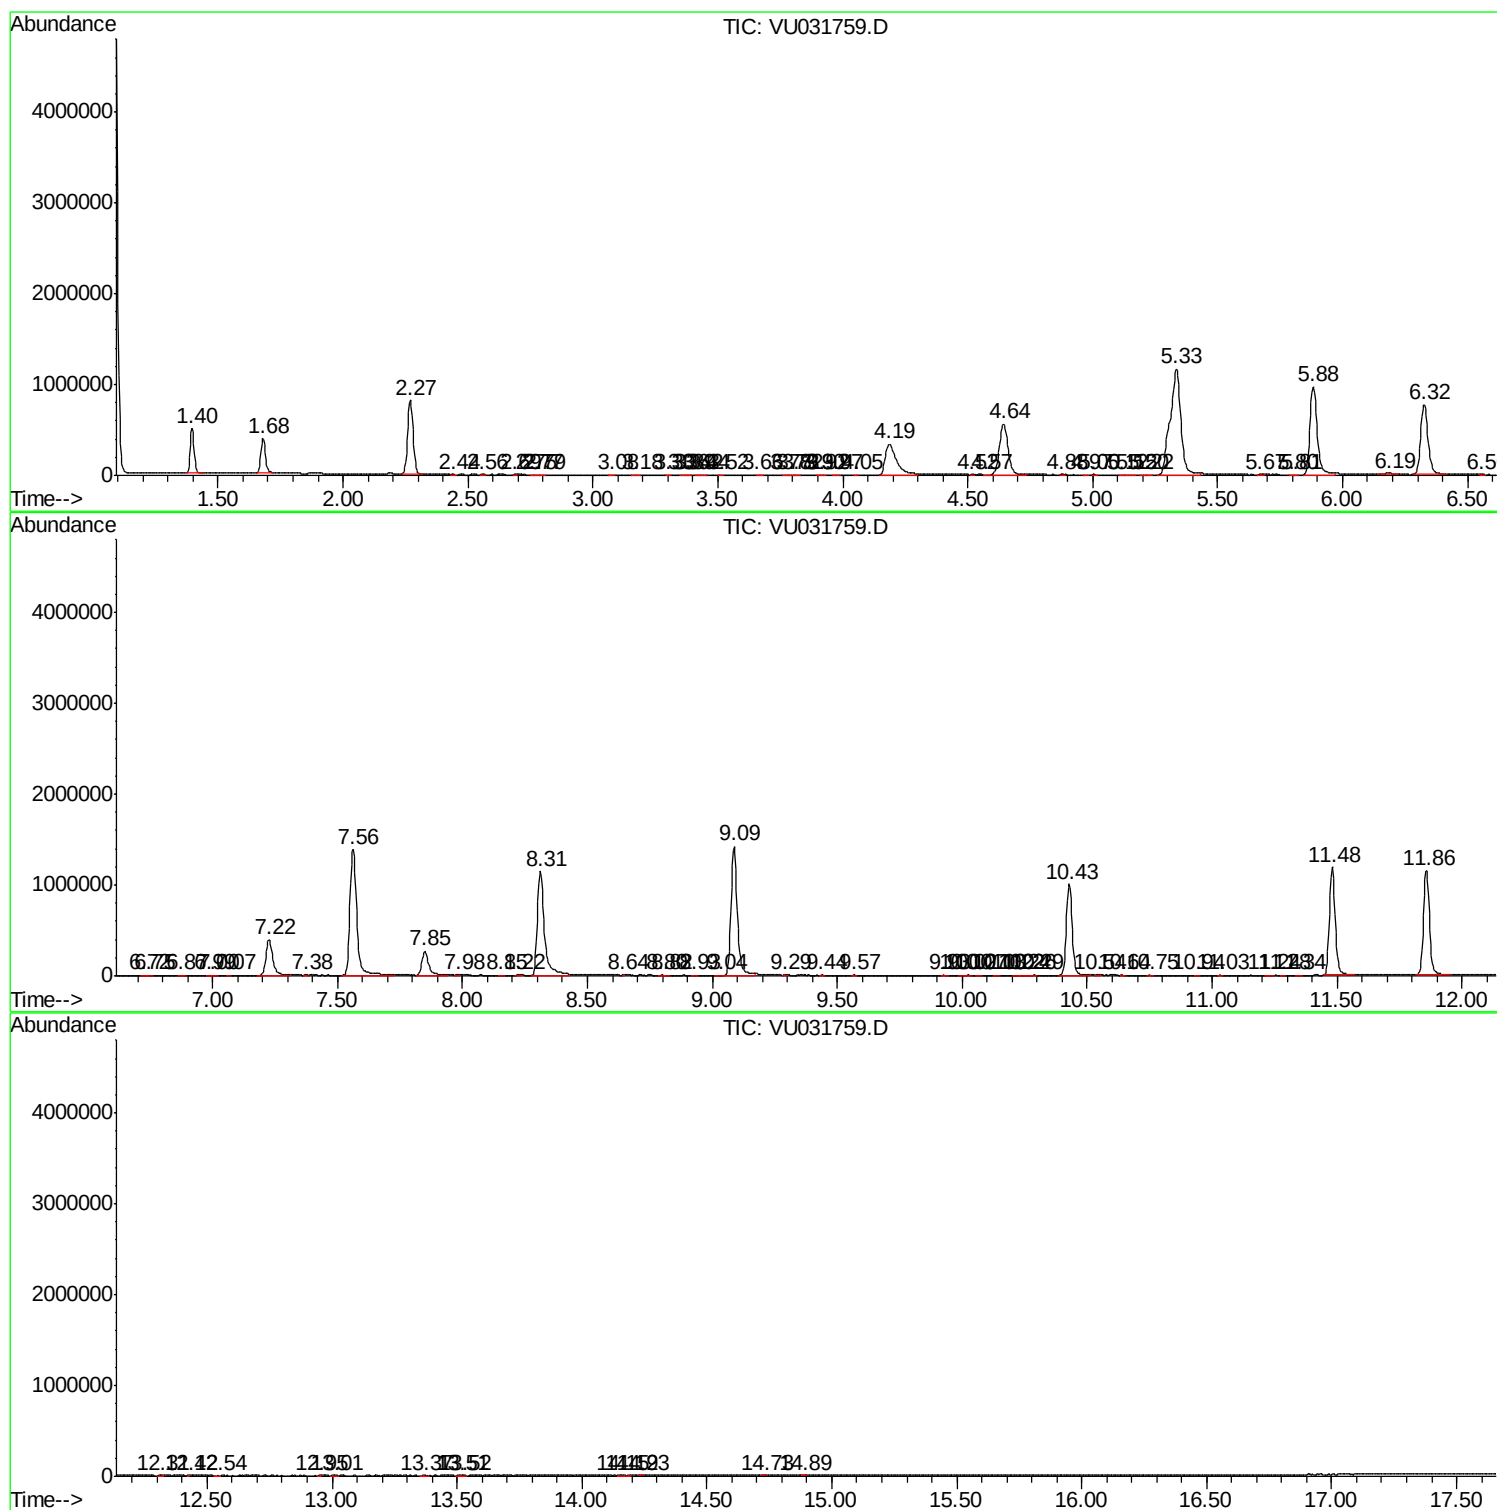

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031759.D
Acq On : 03 May 2019 18:46
Operator : JC/SP
Sample : K2695-05 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU050319\
Data File : VU031759.D
Acq On : 03 May 2019 18:46
Operator : JC/SP
Sample : K2695-05 400X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0XD5

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc