

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031760.D
 Acq On : 03 May 2019 19:10
 Operator : JC/SP
 Sample : K2695-09 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	88	95	108	rVB	482011	511957	14.78%	1.975%
2	1.678	176	183	195	rVB	372712	456848	13.19%	1.762%
3	2.270	356	367	381	rVB	785745	1199144	34.61%	4.625%
4	2.476	427	431	433	rBV5	1829	1117	0.03%	0.004%
5	2.508	438	441	443	rBV2	1732	1218	0.04%	0.005%
6	2.685	493	496	497	rBV2	1463	861	0.02%	0.003%
7	2.788	525	528	530	rBV3	1144	726	0.02%	0.003%
8	2.923	567	570	577	rVB4	1476	1227	0.04%	0.005%
9	3.029	601	603	608	rBV4	944	628	0.02%	0.002%
10	3.087	618	621	624	rBV4	941	613	0.02%	0.002%
11	3.132	632	635	639	rBV3	796	587	0.02%	0.002%
12	3.254	670	673	677	rBV2	1116	936	0.03%	0.004%
13	3.276	677	680	682	rBV3	1135	830	0.02%	0.003%
14	3.331	692	697	700	rBV4	1256	1169	0.03%	0.005%
15	3.498	743	749	752	rBV	1357	1490	0.04%	0.006%
16	3.682	803	806	807	rBV3	1416	711	0.02%	0.003%
17	3.730	818	821	824	rBV3	761	602	0.02%	0.002%
18	3.746	824	826	829	rBV2	744	584	0.02%	0.002%
19	3.784	835	838	843	rVB2	1075	936	0.03%	0.004%
20	3.926	878	882	887	rVB2	2260	2609	0.08%	0.010%
21	3.958	887	892	894	rBV2	1203	843	0.02%	0.003%
22	3.977	894	898	901	rBV5	1323	1082	0.03%	0.004%
23	3.997	901	904	907	rVB	1634	1051	0.03%	0.004%
24	4.042	915	918	922	rVB3	1477	1050	0.03%	0.004%
25	4.074	923	928	930	rBV3	1256	1242	0.04%	0.005%
26	4.186	950	963	997	rBV2	322566	1006714	29.06%	3.883%
27	4.643	1088	1105	1127	rBV	551471	1314429	37.94%	5.070%
28	4.993	1210	1214	1222	rVB6	2384	2613	0.08%	0.010%
29	5.058	1231	1234	1239	rVB3	1900	1581	0.05%	0.006%
30	5.090	1239	1244	1247	rBV6	902	894	0.03%	0.003%
31	5.112	1248	1251	1254	rVV3	944	618	0.02%	0.002%
32	5.334	1297	1320	1356	rBV2	1143169	3464748	100.00%	13.364%
33	5.762	1450	1453	1456	rBV4	2218	1771	0.05%	0.007%
34	5.881	1476	1490	1538	rBV	968103	2042031	58.94%	7.876%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031760.D
 Acq On : 03 May 2019 19:10
 Operator : JC/SP
 Sample : K2695-09 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.183	1572	1584	1605	rBV2	176319	378274	10.92%	1.459%
36	6.325	1615	1628	1659	rBV	764980	1567859	45.25%	6.047%
37	6.566	1701	1703	1707	rBV4	1396	881	0.03%	0.003%
38	6.771	1764	1767	1769	rBV2	1266	778	0.02%	0.003%
39	6.839	1786	1788	1790	rBV2	1237	610	0.02%	0.002%
40	6.910	1806	1810	1812	rBV3	1435	1013	0.03%	0.004%
41	6.952	1820	1823	1824	rBV2	1541	815	0.02%	0.003%
42	6.990	1833	1835	1839	rVB3	1244	758	0.02%	0.003%
43	7.013	1839	1842	1845	rBV2	1255	819	0.02%	0.003%
44	7.035	1845	1849	1857	rBV3	1765	2064	0.06%	0.008%
45	7.071	1857	1860	1864	rVB3	1034	966	0.03%	0.004%
46	7.103	1864	1870	1874	rBV	2957	3230	0.09%	0.012%
47	7.144	1880	1883	1888	rVB4	1302	983	0.03%	0.004%
48	7.225	1896	1908	1938	rBV	382543	735000	21.21%	2.835%
49	7.405	1961	1964	1966	rBV	1210	877	0.03%	0.003%
50	7.562	2000	2013	2057	rBV	1345091	2530477	73.03%	9.760%
51	7.849	2091	2102	2125	rBV	256727	476702	13.76%	1.839%
52	8.067	2167	2170	2173	rBV4	1450	815	0.02%	0.003%
53	8.228	2211	2220	2231	rBV5	14001	24844	0.72%	0.096%
54	8.312	2234	2246	2291	rBV	1101253	2206255	63.68%	8.510%
55	8.787	2389	2394	2397	rBV5	1243	1267	0.04%	0.005%
56	8.861	2415	2417	2420	rVB2	1380	662	0.02%	0.003%
57	8.897	2425	2428	2432	rVV3	1182	891	0.03%	0.003%
58	8.996	2456	2459	2462	rVB5	1049	680	0.02%	0.003%
59	9.022	2462	2467	2469	rBV2	1335	1335	0.04%	0.005%
60	9.086	2474	2487	2515	rBV	1398143	2451882	70.77%	9.457%
61	9.244	2533	2536	2537	rBV2	1433	864	0.02%	0.003%
62	9.405	2582	2586	2590	rVB3	1590	1247	0.04%	0.005%
63	9.485	2608	2611	2615	rVB3	2489	1891	0.05%	0.007%
64	9.575	2636	2639	2641	rBV2	1214	775	0.02%	0.003%
65	9.611	2645	2650	2652	rBV2	1517	1418	0.04%	0.005%
66	9.755	2692	2695	2696	rBV4	1165	578	0.02%	0.002%
67	9.787	2701	2705	2711	rBV5	1391	1584	0.05%	0.006%
68	9.977	2761	2764	2769	rBV3	1085	952	0.03%	0.004%
69	10.025	2776	2779	2782	rVB3	1096	761	0.02%	0.003%
70	10.064	2787	2791	2793	rBV2	1337	1031	0.03%	0.004%
71	10.099	2799	2802	2806	rVB4	1385	1120	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050319\
 Data File : VU031760.D
 Acq On : 03 May 2019 19:10
 Operator : JC/SP
 Sample : K2695-09 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.189	2826	2830	2832	rBV4	1629	1141	0.03%	0.004%
73	10.202	2832	2834	2838	rVV5	1180	905	0.03%	0.003%
74	10.279	2856	2858	2861	rBV3	1283	892	0.03%	0.003%
75	10.427	2889	2904	2929	rBV	986725	1600794	46.20%	6.174%
76	10.611	2954	2961	2970	rBV	2044	3696	0.11%	0.014%
77	10.649	2970	2973	2976	rBV3	1288	1070	0.03%	0.004%
78	10.701	2987	2989	2997	rBV5	1133	1063	0.03%	0.004%
79	10.736	2998	3000	3004	rBV2	1560	1069	0.03%	0.004%
80	10.784	3011	3015	3016	rBV2	2046	1289	0.04%	0.005%
81	10.868	3038	3041	3043	rBV	988	744	0.02%	0.003%
82	10.935	3058	3062	3069	rVB4	1389	1662	0.05%	0.006%
83	10.974	3069	3074	3076	rBV	1417	1569	0.05%	0.006%
84	11.051	3093	3098	3103	rBV5	1441	2071	0.06%	0.008%
85	11.102	3111	3114	3118	rVB2	1141	1008	0.03%	0.004%
86	11.218	3148	3150	3154	rVB2	1397	846	0.02%	0.003%
87	11.331	3182	3185	3187	rBV3	1229	919	0.03%	0.004%
88	11.418	3210	3212	3216	rBV4	1023	782	0.02%	0.003%
89	11.479	3219	3231	3257	rBV	1165516	1926062	55.59%	7.429%
90	11.855	3336	3348	3370	rBV	1137445	1925646	55.58%	7.427%
91	12.479	3533	3542	3549	rBV4	5805	10444	0.30%	0.040%
92	12.549	3562	3564	3566	rBV2	1632	973	0.03%	0.004%
93	12.742	3621	3624	3628	rVB2	1753	1194	0.03%	0.005%
94	12.762	3628	3630	3633	rBV	1305	862	0.02%	0.003%
95	12.826	3647	3650	3655	rBV6	1834	2137	0.06%	0.008%
96	12.945	3684	3687	3693	rBV4	2063	2442	0.07%	0.009%
97	13.019	3707	3710	3712	rBV3	1316	790	0.02%	0.003%
98	13.093	3730	3733	3738	rBV2	1719	1502	0.04%	0.006%
99	14.089	4041	4043	4046	rBV2	1373	696	0.02%	0.003%
100	14.999	4322	4326	4331	rBV4	4023	3694	0.11%	0.014%


Sum of corrected areas: 25926380

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050319\
Data File : VU031760.D
Acq On : 03 May 2019 19:10
Operator : JC/SP
Sample : K2695-09 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

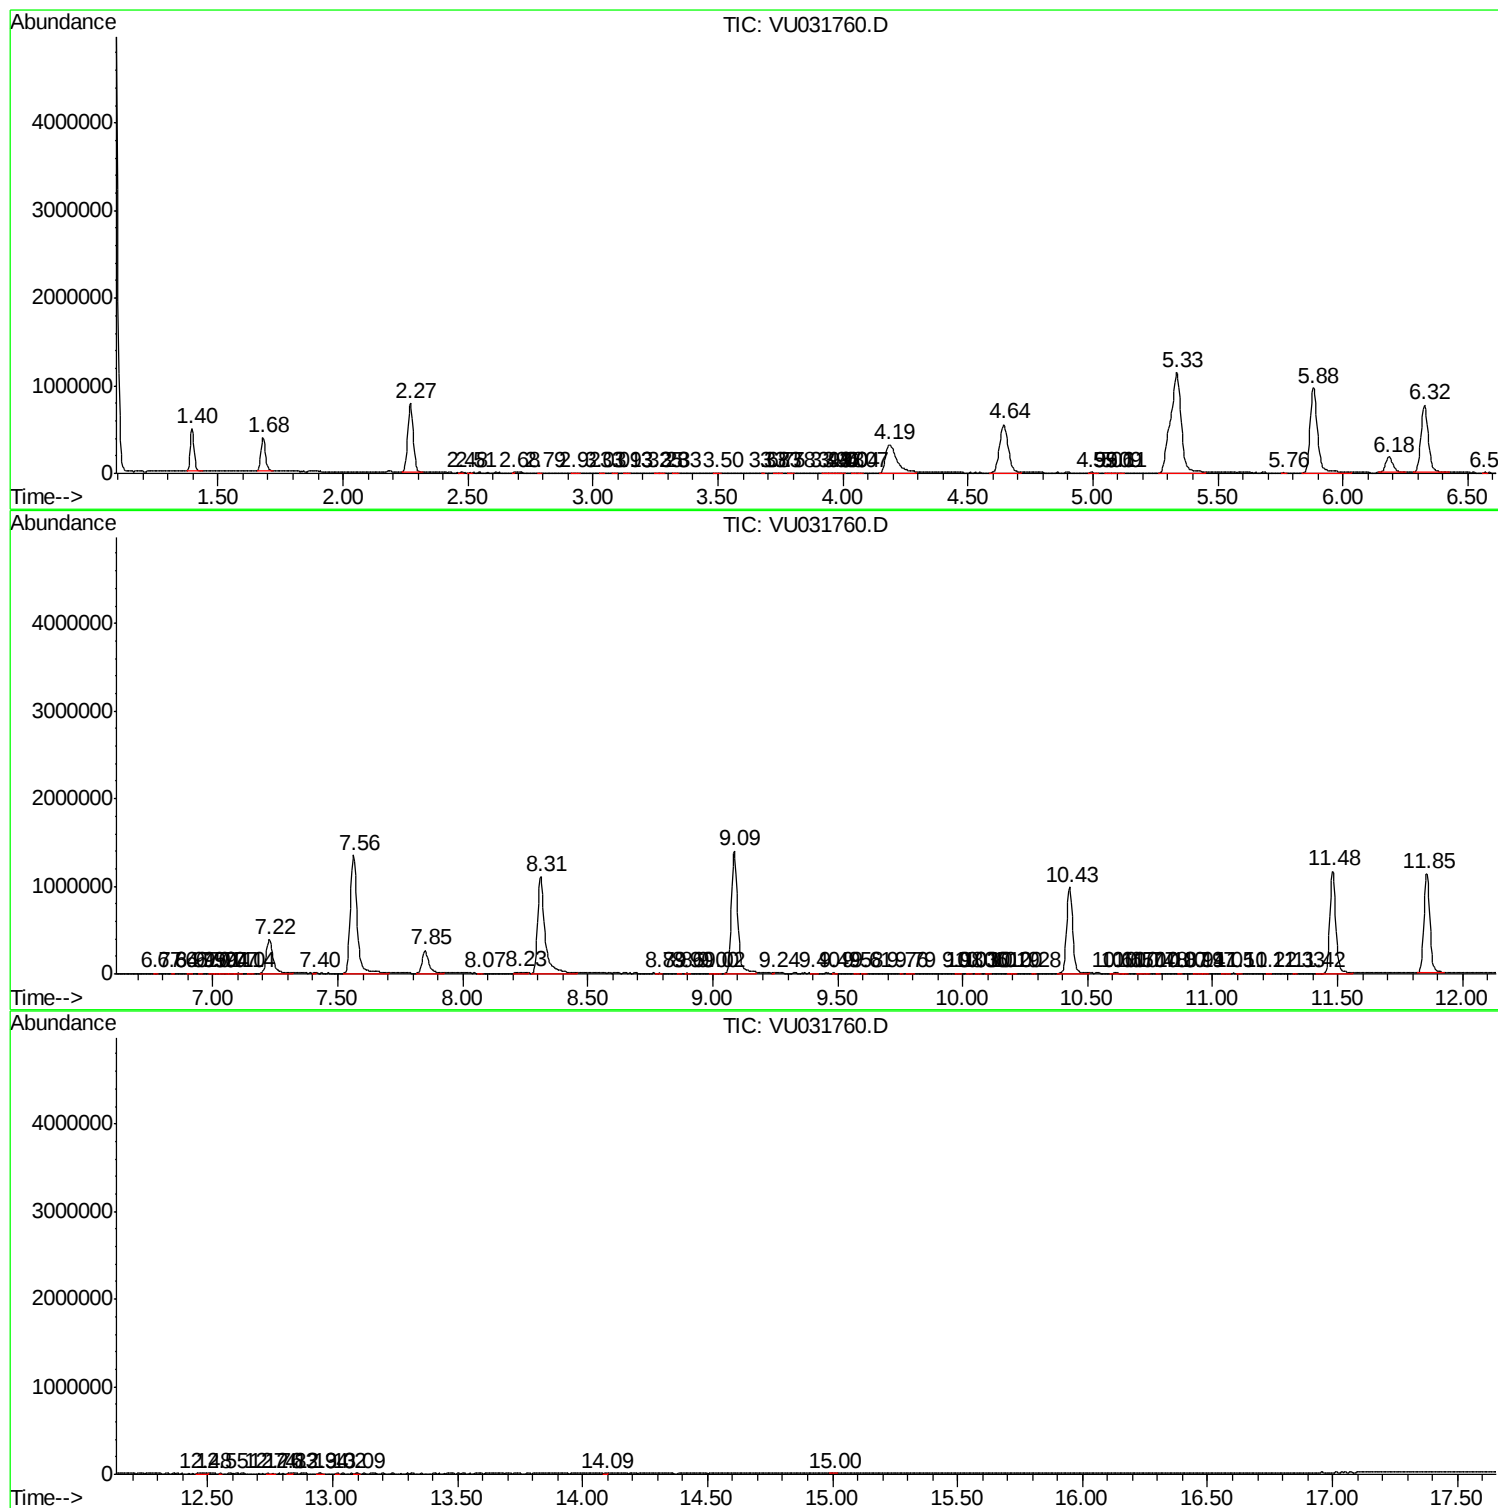

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031760.D
Acq On : 03 May 2019 19:10
Operator : JC/SP
Sample : K2695-09 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050319\
Data File : VU031760.D
Acq On : 03 May 2019 19:10
Operator : JC/SP
Sample : K2695-09 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XH3

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc