


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050319\
 Data File : VU031733.D
 Acq On : 03 May 2019 08:35
 Operator : JC/SP
 Sample : BFB37
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB37

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Sat May 04 02:35:16 2019

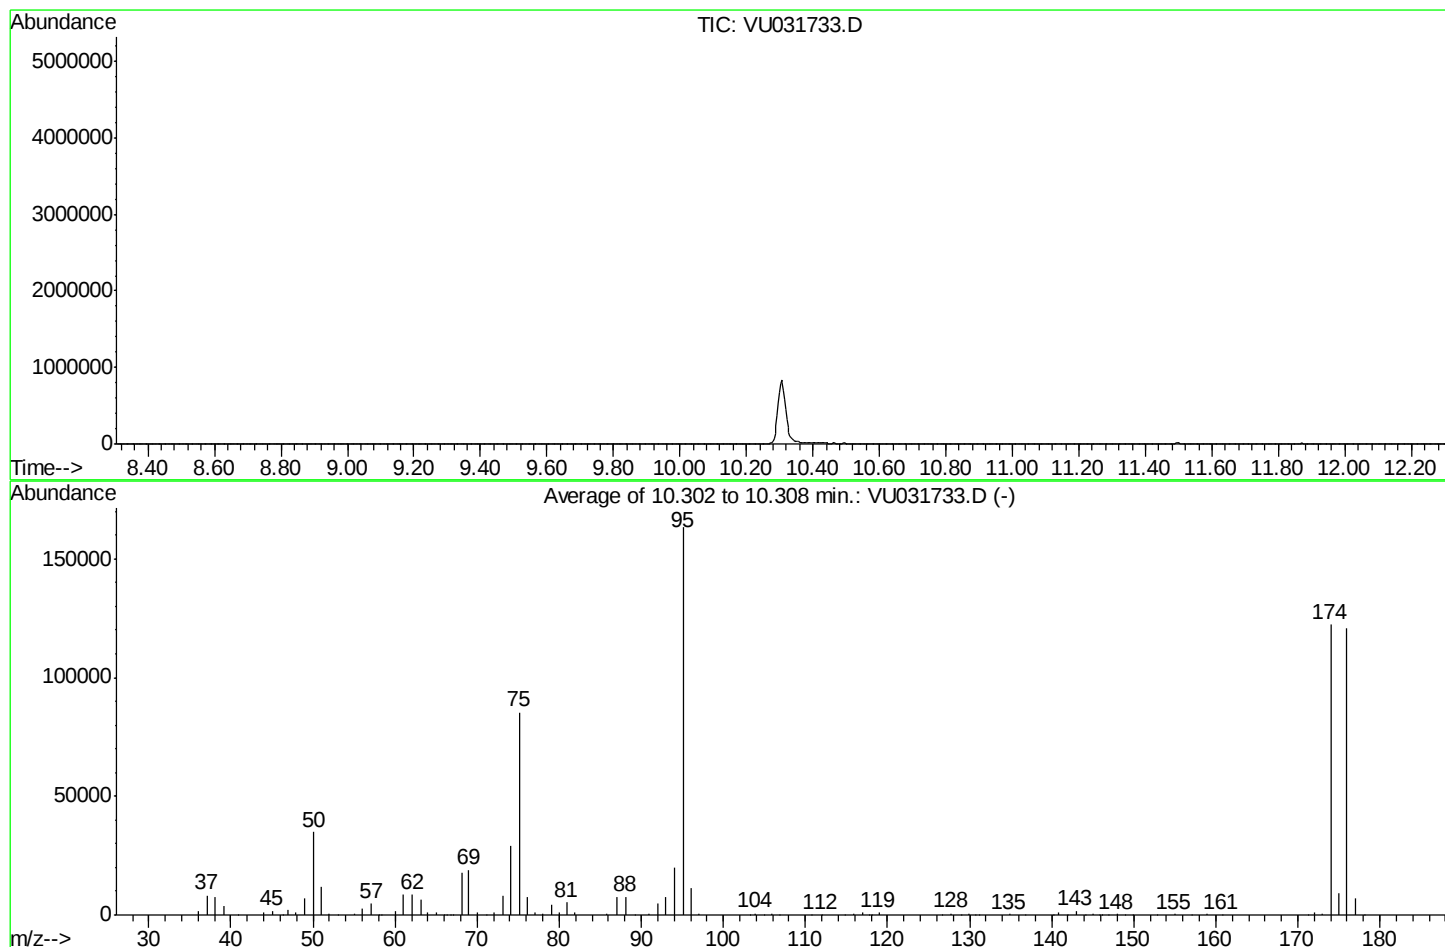

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	34800	PASS
75	95	30	80	52.3	85405	PASS
95	95	100	100	100.0	163242	PASS
96	95	5	9	6.9	11241	PASS
173	174	0.00	2	0.3	385	PASS
174	95	50	120	74.8	122109	PASS
175	174	5	9	7.4	8995	PASS
176	174	95	101	98.9	120810	PASS
177	176	5	9	5.9	7075	PASS

Scan 2853 (10.263 min): VU031733.D
BFB37

m/z	Abundance
40.00	5145.0
40.90	107.0
44.00	1372.0
207.10	237.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.10	1641.0
37.10	8314.0
38.00	7740.0
39.10	3898.0
40.00	4934.0
44.00	2479.0
45.00	1765.0
46.30	167.0
47.00	2317.0
48.00	1063.0
49.00	6943.0
50.10	34120.0
51.00	11781.0
52.00	547.0
53.20	250.0
55.10	539.0
56.00	2693.0
57.10	4591.0
58.00	335.0
60.00	1471.0
61.00	8849.0
62.10	7689.0
63.10	6357.0
64.00	954.0
65.00	1041.0
66.30	140.0
67.10	372.0
68.10	16760.0
69.00	19216.0
70.00	926.0
71.10	120.0
72.00	902.0
73.10	7670.0
74.10	28560.0
75.10	83600.0
76.00	7529.0
77.00	1330.0
78.00	715.0
79.00	4266.0
80.00	1373.0
81.00	5089.0
82.00	1211.0
85.90	237.0
87.00	7649.0
88.10	7398.0
90.90	549.0
92.00	4746.0
93.00	7421.0
94.10	19712.0
95.10	159296.0
96.10	11317.0
97.10	392.0
103.30	150.0
103.90	808.0
104.90	136.0
105.90	517.0
106.90	127.0
110.80	160.0
111.90	212.0
114.80	135.0
115.80	512.0
117.00	829.0
118.00	416.0
119.00	1095.0
127.80	518.0
129.10	221.0
129.90	454.0
130.70	116.0
131.10	180.0
134.90	414.0
136.90	116.0
140.20	121.0
140.90	1322.0
142.00	173.0
143.00	1784.0
144.10	168.0
145.00	380.0
146.20	226.0
146.90	159.0
147.90	398.0
153.00	122.0
154.90	599.0
157.00	243.0
159.00	285.0
160.80	112.0
172.00	1133.0
174.00	118112.0
175.00	9186.0
176.00	114664.0
177.00	6787.0
178.10	198.0
207.10	224.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.00	1757.0
37.10	8432.0
38.00	7585.0
39.10	4132.0
40.00	4998.0
40.90	146.0
44.00	2420.0
45.00	1695.0
46.30	317.0
47.00	2371.0
48.00	1216.0
49.10	7545.0
50.10	35672.0
51.10	12339.0
52.00	558.0
53.10	192.0
55.10	535.0
56.00	2648.0
57.10	4748.0
58.00	225.0
60.00	1640.0
61.00	8668.0
62.10	8803.0
63.10	6923.0
64.00	906.0
65.00	1139.0
66.80	262.0
68.10	18312.0
69.00	19488.0
70.00	1179.0
71.20	204.0
72.00	951.0
73.10	8565.0
74.10	30000.0
75.10	87944.0
76.00	7648.0
77.00	1344.0
78.00	813.0
79.00	4382.0
79.90	1338.0
81.00	5378.0
81.90	1212.0
85.80	346.0
87.00	8043.0
88.00	8153.0
90.90	665.0
92.10	4687.0
93.00	7776.0
94.10	20440.0
95.10	167872.0
96.10	11527.0
97.00	566.0
103.30	141.0
103.90	809.0
104.90	113.0
105.90	457.0
110.80	222.0
111.90	204.0
115.80	578.0
117.00	892.0
118.10	338.0
118.90	1063.0
126.70	144.0
127.80	683.0
129.10	271.0
129.90	525.0
130.70	121.0
131.20	144.0
134.90	406.0
136.80	133.0
140.10	155.0
140.90	1339.0
141.90	166.0
142.90	1948.0
144.10	136.0
145.00	482.0
146.20	342.0
146.90	209.0
148.00	431.0
149.00	171.0
149.90	106.0
152.90	145.0
155.00	521.0
157.00	225.0
159.00	333.0
160.80	147.0
171.30	326.0
172.00	1284.0
172.90	1157.0
174.00	125800.0
175.00	9374.0
176.00	124880.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

177.00	7184.0
178.10	192.0
207.00	181.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

m/z	Abundance
36.00	1755.0
37.00	8381.0
38.00	7099.0
39.10	3670.0
40.00	5083.0
40.90	193.0
44.10	2368.0
45.10	1592.0
46.30	324.0
47.00	2159.0
47.90	1352.0
49.10	7213.0
50.10	34608.0
51.10	11249.0
51.90	554.0
53.00	136.0
55.10	463.0
56.00	2410.0
57.10	4480.0
57.90	124.0
58.40	155.0
60.00	1661.0
61.10	7698.0
62.10	8805.0
63.10	6752.0
64.00	862.0
65.00	1121.0
66.00	121.0
66.70	258.0
68.10	17960.0
69.00	18160.0
70.10	1348.0
71.20	183.0
72.10	983.0
73.10	8198.0
74.10	28512.0
75.10	84672.0
76.10	7420.0
77.00	1209.0
78.00	822.0
79.00	4220.0
79.90	1200.0
80.90	5063.0
81.80	1177.0
85.80	306.0
87.00	7580.0
88.00	7965.0
89.20	118.0
90.90	637.0
92.10	4395.0
93.00	7136.0
94.10	19024.0
95.10	162560.0
96.10	10880.0
97.00	616.0
103.90	675.0
105.90	455.0
110.80	207.0
112.00	207.0
115.90	662.0
117.00	942.0
117.80	250.0
119.00	965.0
126.70	166.0
127.80	651.0
129.00	282.0
130.00	563.0
130.70	119.0
134.80	294.0
136.80	195.0
140.10	143.0
140.90	1414.0
141.80	178.0
142.90	1934.0
145.00	497.0
145.90	250.0
146.20	273.0
146.90	187.0
148.00	449.0
149.00	191.0
149.90	119.0
152.80	119.0
155.10	438.0
157.00	228.0
159.00	305.0
160.80	122.0
171.30	278.0
172.10	1200.0
174.00	122416.0
175.00	8427.0
176.00	122888.0
177.00	7255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37

178.10193.0

206.90144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB37