

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050321\
 Data File : VU043503.D
 Acq On : 03 May 2021 23:53
 Operator : SY/MD
 Sample : M2195-16DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB3J4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043503.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	51846	58261	10.70%	1.493%
2	1.919	171	180	195	rVB	40450	52524	9.65%	1.346%
3	2.572	370	383	400	rBV	91970	149099	27.38%	3.821%
4	3.057	524	534	544	rVB3	4076	7498	1.38%	0.192%
5	3.192	565	576	594	rBV3	2660	5460	1.00%	0.140%
6	4.645	1012	1028	1063	rBV2	57277	192302	35.32%	4.928%
7	5.073	1146	1161	1182	rBV	77770	174001	31.96%	4.459%
8	5.735	1345	1367	1389	rBV2	153077	402732	73.97%	10.320%
9	6.256	1513	1529	1545	rBV	119244	224556	41.24%	5.754%
10	6.700	1653	1667	1689	rBV	102741	199161	36.58%	5.104%
11	7.575	1926	1939	1959	rBV2	49773	87495	16.07%	2.242%
12	7.906	2029	2042	2057	rBV	174915	295697	54.31%	7.577%
13	8.189	2115	2130	2149	rBV2	31853	55523	10.20%	1.423%
14	8.562	2231	2246	2260	rBV	301370	511115	93.88%	13.098%
15	8.645	2260	2272	2313	rVB	257689	544460	100.00%	13.952%
16	9.423	2498	2514	2532	rBV	176139	296502	54.46%	7.598%
17	10.764	2919	2931	2947	rBV	77435	125309	23.02%	3.211%
18	11.819	3247	3259	3274	rBV	160327	254261	46.70%	6.516%
19	12.201	3365	3378	3392	rBV	168657	266366	48.92%	6.826%




Sum of corrected areas: 3902322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050321\
Data File : VU043503.D
Acq On : 03 May 2021 23:53
Operator : SY/MD
Sample : M2195-16DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

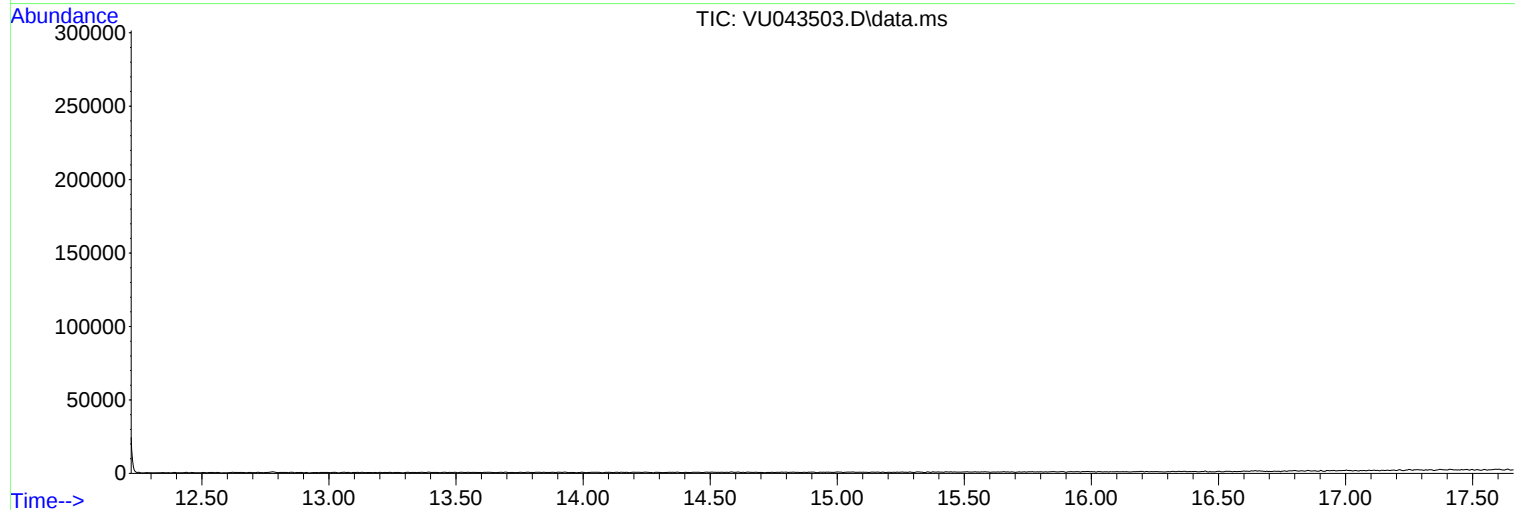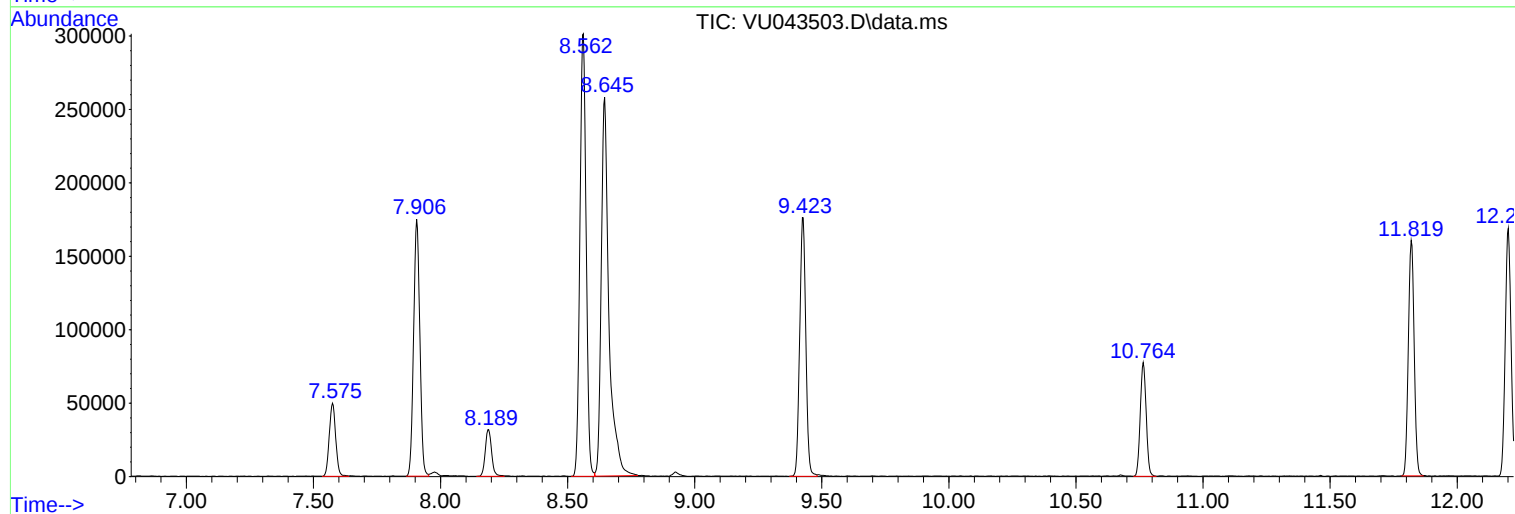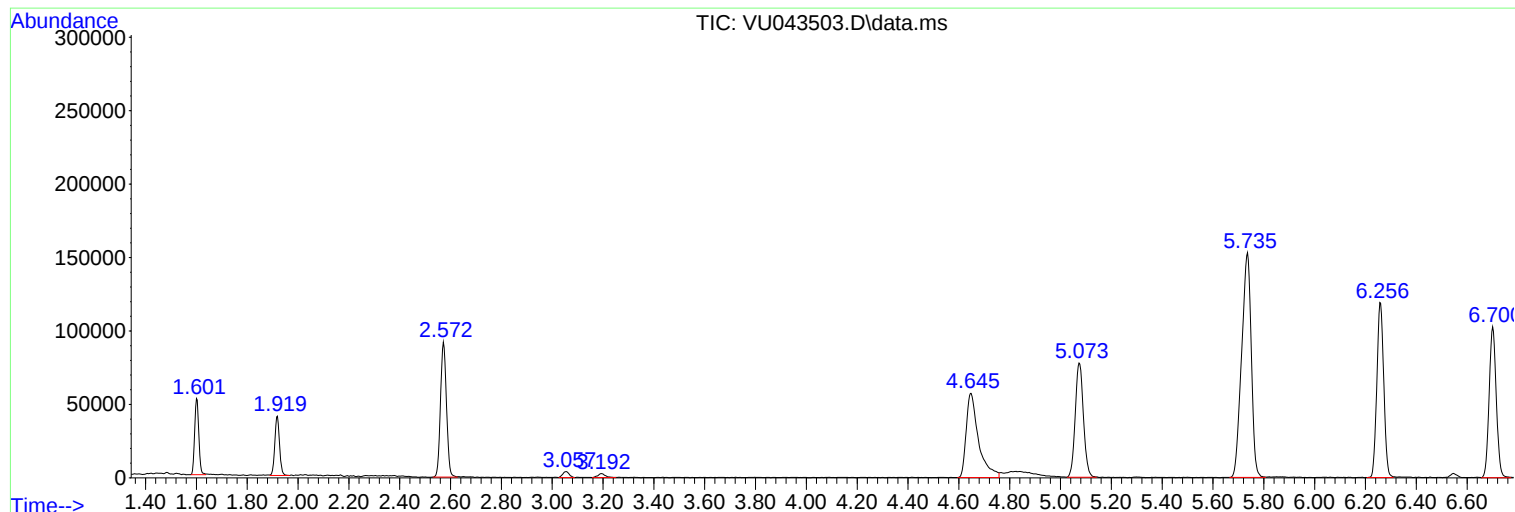

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050321\
Data File : VU043503.D
Acq On : 03 May 2021 23:53
Operator : SY/MD
Sample : M2195-16DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050321\
Data File : VU043503.D
Acq On : 03 May 2021 23:53
Operator : SY/MD
Sample : M2195-16DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB3J4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
