
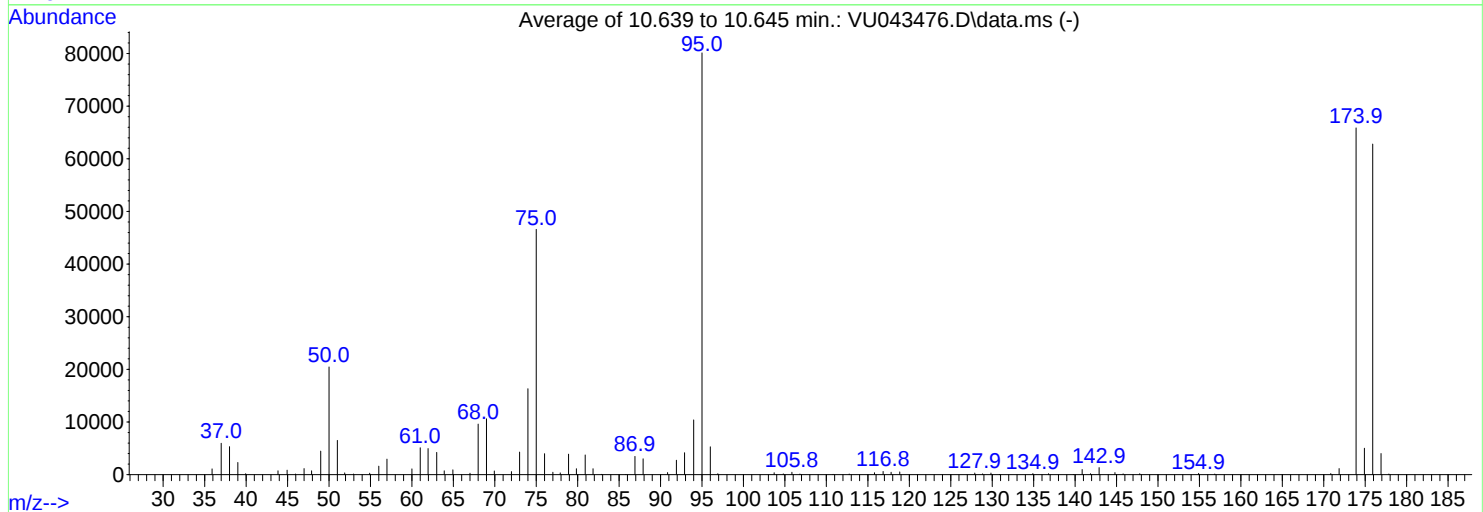


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050321\
 Data File : VU043476.D
 Acq On : 03 May 2021 08:58
 Operator : SY/MD
 Sample : BFB39
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB139

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR050321WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed May 05 08:11:40 2021

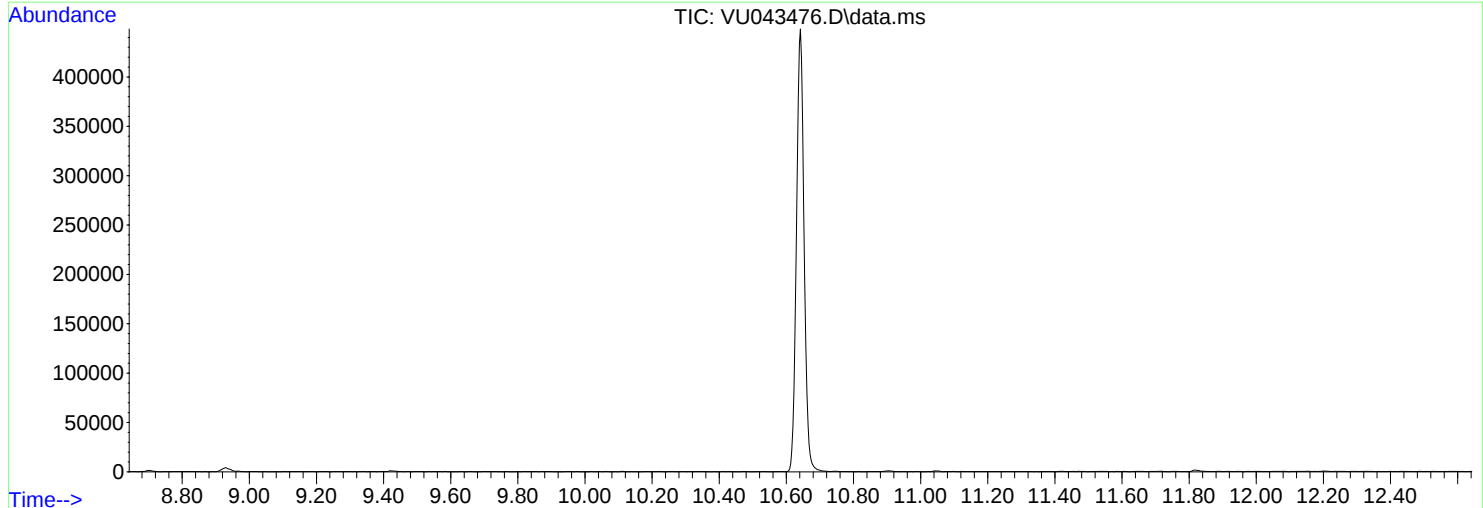

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	20461	PASS
75	95	30	80	58.1	46592	PASS
95	95	100	100	100.0	80133	PASS
96	95	5	9	6.6	5279	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	82.2	65864	PASS
175	174	5	9	7.6	5006	PASS
176	174	95	101	95.4	62811	PASS
177	176	5	9	6.4	4006	PASS

m/z	Abundance
43.80	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	1172.0
37.00	6126.0
38.00	5452.0
39.00	2310.0
40.00	183.0
43.90	1058.0
45.00	837.0
45.90	187.0
47.00	1158.0
47.90	771.0
49.00	4526.0
50.00	20816.0
51.00	6776.0
51.90	333.0
52.90	136.0
54.90	278.0
56.00	1590.0
57.00	2926.0
60.00	1022.0
61.00	5271.0
62.00	4991.0
63.00	4108.0
63.90	798.0
64.90	917.0
67.00	295.0
68.00	9820.0
69.00	10788.0
69.90	744.0
72.00	540.0
73.00	4425.0
74.00	16250.0
75.00	46960.0
76.00	4017.0
77.00	508.0
77.90	383.0
78.90	4114.0
79.90	1155.0
80.90	3909.0
81.80	1172.0
85.80	113.0
86.90	3389.0
87.90	3061.0
90.90	413.0
91.90	2852.0
92.90	4270.0
94.00	10445.0
95.00	80592.0
96.00	5384.0
96.90	202.0
103.70	338.0
104.80	160.0
105.90	351.0
106.80	135.0
110.80	120.0
112.80	116.0
115.80	397.0
116.90	658.0
117.80	440.0
118.90	602.0
127.90	293.0
128.80	126.0
129.80	310.0
134.90	233.0
136.80	224.0
139.80	107.0
140.90	991.0
141.80	188.0
142.90	1455.0
144.80	435.0
145.80	151.0
147.80	168.0
154.90	219.0
156.80	135.0
171.00	189.0
171.90	1147.0
173.90	64592.0
174.90	4893.0
175.90	61168.0
176.90	3938.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	1140.0
37.00	6194.0
38.00	5451.0
39.00	2422.0
39.90	186.0
43.90	1005.0
45.00	867.0
46.00	156.0
47.00	1215.0
47.90	786.0
49.00	4679.0
50.00	21184.0
51.00	6696.0
51.90	357.0
52.90	144.0
54.90	291.0
56.00	1663.0
57.00	3102.0
60.00	1162.0
61.00	5288.0
62.00	5092.0
63.00	4323.0
63.90	771.0
65.00	923.0
67.00	285.0
68.00	9993.0
69.00	11044.0
69.90	713.0
72.00	589.0
73.00	4408.0
74.00	16872.0
75.00	48232.0
76.00	4163.0
77.00	468.0
77.90	348.0
78.90	4014.0
79.90	1159.0
80.90	3782.0
81.90	1193.0
82.90	107.0
86.90	3593.0
87.90	3101.0
90.80	407.0
91.90	2819.0
92.90	4361.0
94.00	10698.0
95.00	82880.0
96.00	5481.0
96.90	182.0
103.70	371.0
104.80	178.0
105.70	331.0
105.90	330.0
106.80	137.0
110.80	108.0
112.80	136.0
115.80	388.0
116.90	632.0
117.80	487.0
118.90	538.0
127.90	359.0
128.90	147.0
129.90	317.0
134.90	255.0
136.80	201.0
140.80	1007.0
141.80	193.0
142.90	1405.0
144.80	422.0
145.80	151.0
147.80	191.0
154.90	247.0
156.80	146.0
170.80	203.0
171.90	1198.0
173.90	68112.0
174.90	5134.0
175.90	64944.0
176.90	4099.0
177.80	124.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139

m/z	Abundance
35.90	1010.0
37.00	5582.0
38.00	5070.0
39.00	2239.0
39.90	188.0
43.90	835.0
44.90	822.0
47.00	1112.0
47.90	685.0
49.00	4220.0
50.00	19384.0
51.00	6020.0
51.90	308.0
53.00	137.0
54.90	272.0
56.00	1572.0
57.00	2818.0
60.00	1099.0
61.00	4731.0
61.90	4794.0
63.00	4224.0
63.90	591.0
65.00	899.0
67.00	249.0
68.00	9033.0
69.00	9996.0
70.00	654.0
72.00	562.0
73.00	4018.0
74.00	15834.0
75.00	44584.0
76.00	3732.0
77.00	443.0
77.90	295.0
78.90	3576.0
79.80	1026.0
80.90	3494.0
81.90	1059.0
82.90	113.0
86.90	3452.0
87.90	2899.0
90.90	365.0
91.90	2552.0
92.90	3869.0
94.00	10102.0
95.00	76928.0
96.00	4973.0
96.90	156.0
103.70	377.0
104.80	130.0
105.80	368.0
106.80	127.0
112.70	122.0
115.80	324.0
116.80	581.0
117.80	458.0
118.80	464.0
127.90	318.0
128.90	175.0
129.80	299.0
130.90	114.0
134.90	172.0
136.80	144.0
140.80	921.0
141.90	180.0
142.90	1201.0
144.80	353.0
145.80	143.0
147.80	214.0
154.90	243.0
156.90	130.0
170.80	227.0
171.80	1146.0
173.90	64888.0
174.90	4991.0
175.90	62320.0
176.90	3982.0
177.80	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB139