

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048390.D
 Acq On : 03 May 2022 15:07
 Operator : SY/MD
 Sample : N2668-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :


Quant Time: May 04 01:39:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 04 01:37:47 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	432979	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	422388	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	201318	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	210429	52.851	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.700%
7) Chloroethane-d5	1.903	69	165473	59.207	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	118.420%
11) 1,1-Dichloroethene-d2	2.565	63	254285	39.859	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	79.720%
21) 2-Butanone-d5	4.623	46	291241	85.763	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	85.760%
24) Chloroform-d	5.066	84	337747	46.767	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.540%
26) 1,2-Dichloroethane-d4	5.703	65	209450	48.880	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.760%
32) Benzene-d6	5.729	84	724399	54.378	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.760%
36) 1,2-Dichloropropane-d6	6.690	67	229043	52.006	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.020%
41) Toluene-d8	7.899	98	634735	52.565	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.140%
43) trans-1,3-Dichloroprop...	8.179	79	93911	48.324	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.640%
47) 2-Hexanone-d5	8.636	63	212255	89.328	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	89.330%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	350898	45.429	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.860%
66) 1,2-Dichlorobenzene-d4	12.192	152	244466	53.981	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.960%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.565	101	2621	0.804	ug/L #	18
12) 1,1-Dichloroethene	2.568	96	2174	0.764	ug/L #	1
37) 1,2-Dichloropropane	6.693	63	22615	6.356	ug/L #	88
60) 1,2,3-Trichloropropane	11.812	75	20145	4.289	ug/L #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 04 01:39:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 04 01:37:47 2022
Response via : Initial Calibration







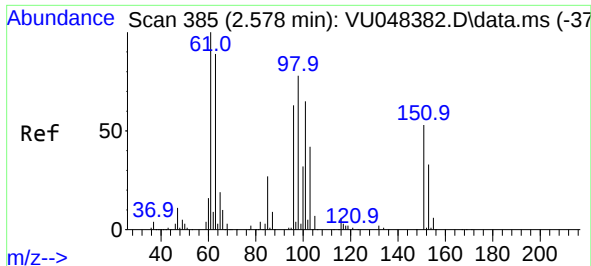

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.804 ug/L
 RT: 2.565 min Scan# 381
 Delta R.T. -0.013 min
 Lab File: VU048390.D
 Acq: 03 May 2022 15:07




Instrument :
 MSVOA_U
 ClientSampleId :


Tgt Ion:101 Resp: 2621
 Ion Ratio Lower Upper
 101 100
 85 0.0 32.6 48.8#
 151 0.0 64.1 96.1#

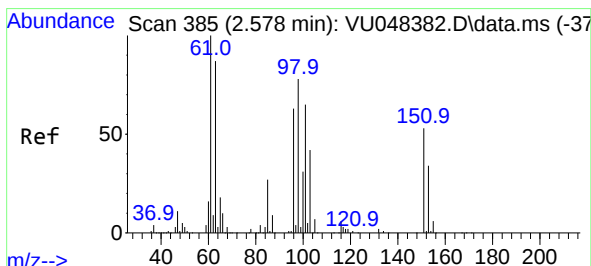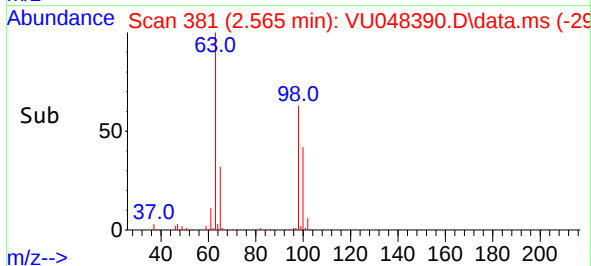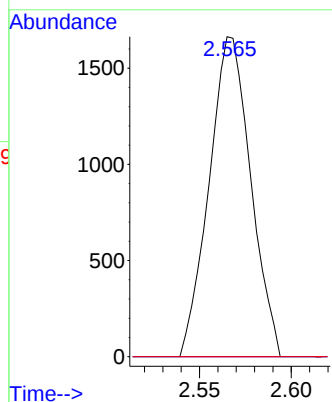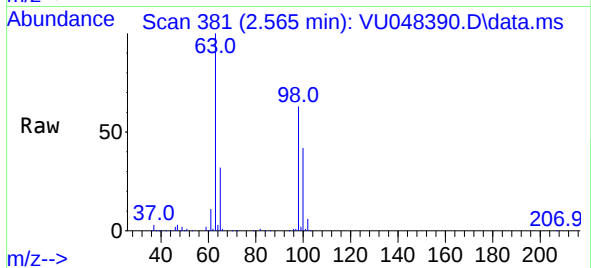

#12
 1,1-Dichloroethene
 Concen: 0.764 ug/L
 RT: 2.568 min Scan# 382
 Delta R.T. -0.010 min
 Lab File: VU048390.D
 Acq: 03 May 2022 15:07

Tgt Ion: 96 Resp: 2174
 Ion Ratio Lower Upper
 96 100
 61 1221.5 107.9 200.3#
 63 10914.4 80.3 149.1#


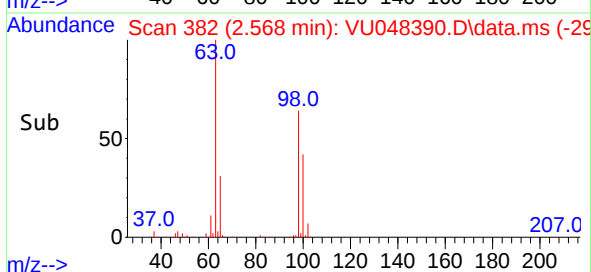
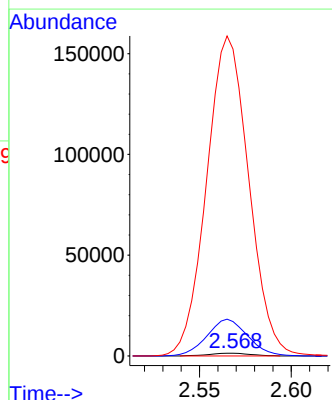
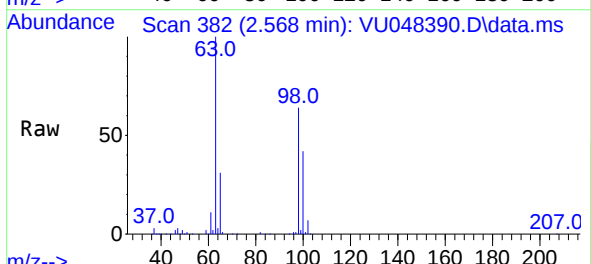


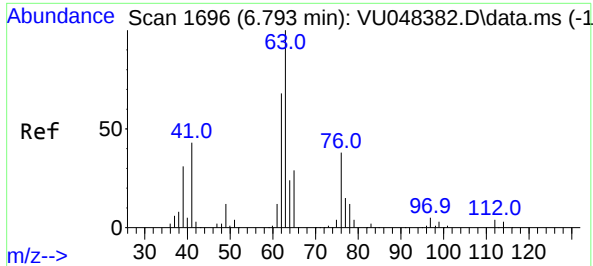

#37
1,2-Dichloropropane
Concen: 6.356 ug/L
RT: 6.693 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU048390.D
Acq: 03 May 2022 15:07

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 22615
Ion Ratio Lower Upper
63 100
112 0.0 3.1 4.7#

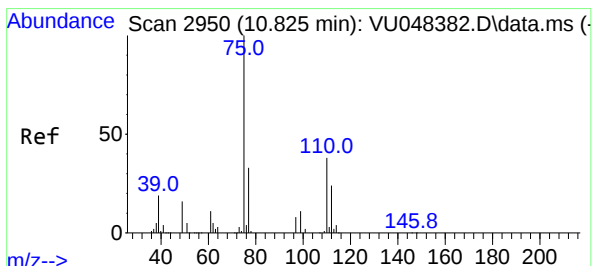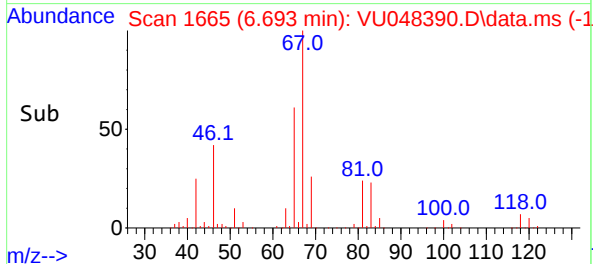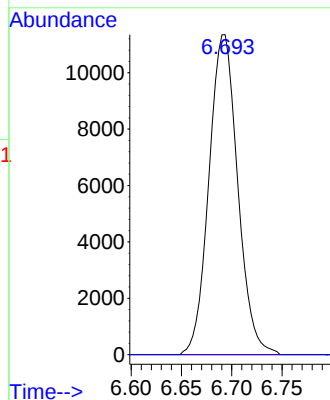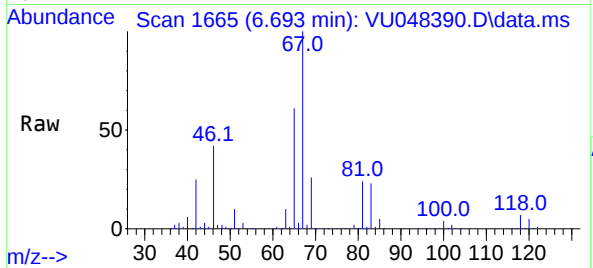

#60
1,2,3-Trichloropropane
Concen: 4.289 ug/L
RT: 11.812 min Scan# 3257
Delta R.T. 0.987 min
Lab File: VU048390.D
Acq: 03 May 2022 15:07

Tgt Ion: 75 Resp: 20145
Ion Ratio Lower Upper
75 100
77 30.4 25.8 38.8
110 2.6 29.9 44.9#

