




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048392.D
 Acq On : 03 May 2022 15:54
 Operator : SY/MD
 Sample : N2668-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL67

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:40:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 04 01:37:47 2022
 Response via : Initial Calibration

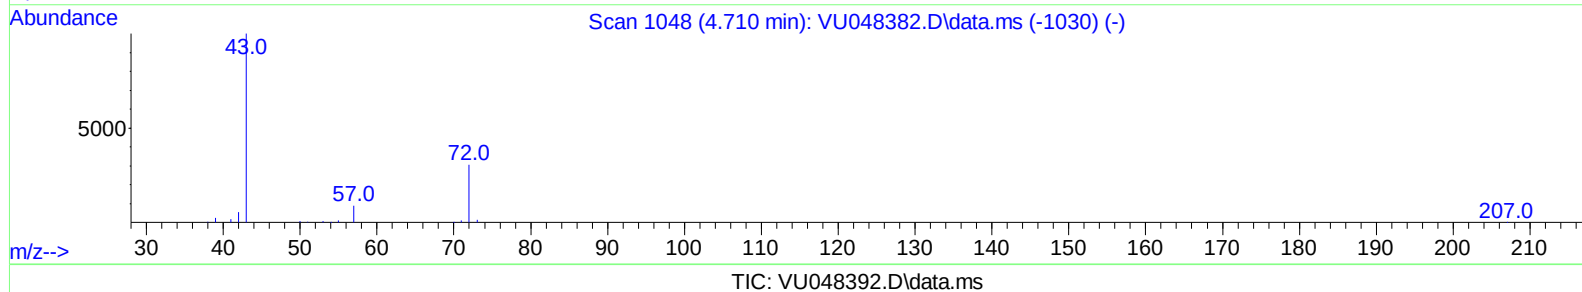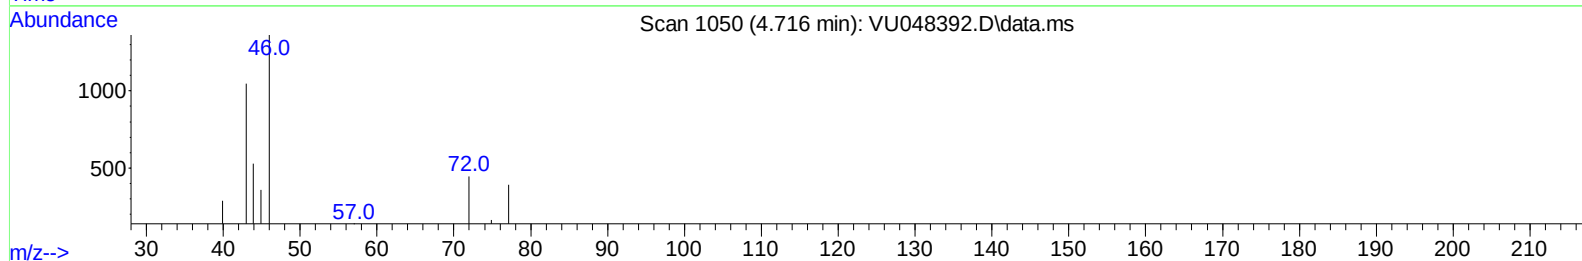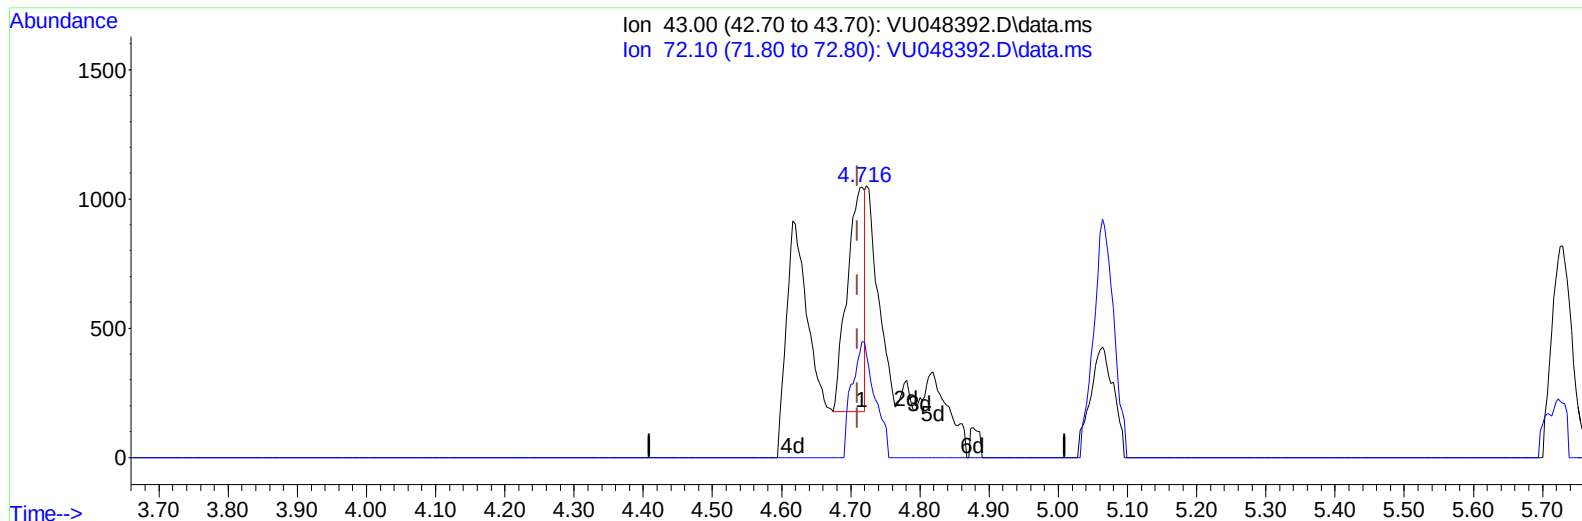

(22) 2-Butanone (T)

4.716min (+ 0.007) 0.46 ug/L

response 1489

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.20	68.03#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048392.D
Acq On : 03 May 2022 15:54
Operator : SY/MD
Sample : N2668-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL67

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

Quant Time: May 04 01:40:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 04 01:37:47 2022
Response via : Initial Calibration

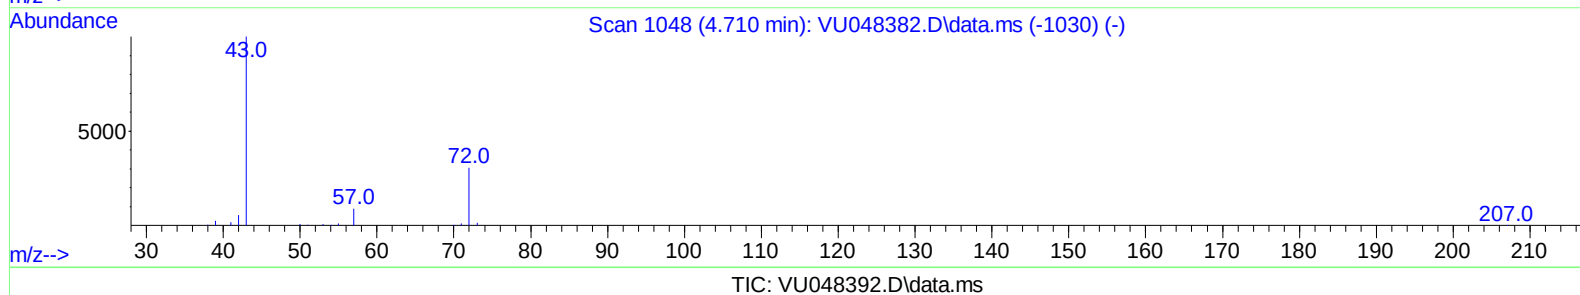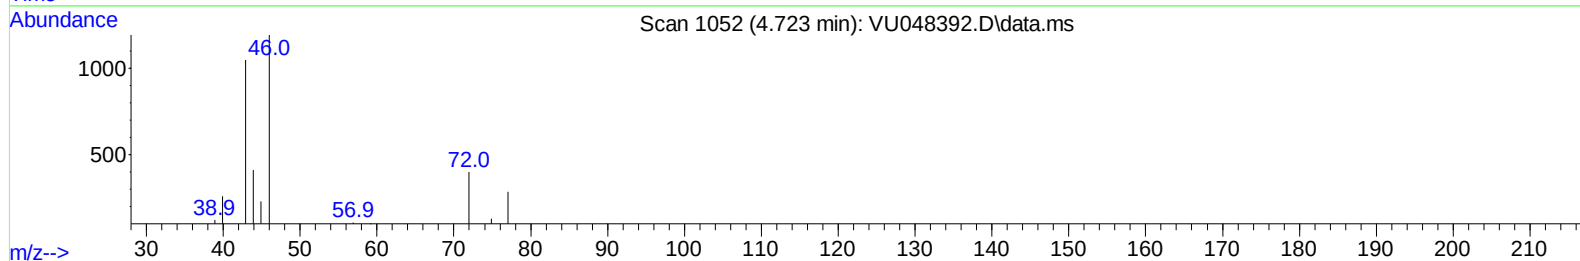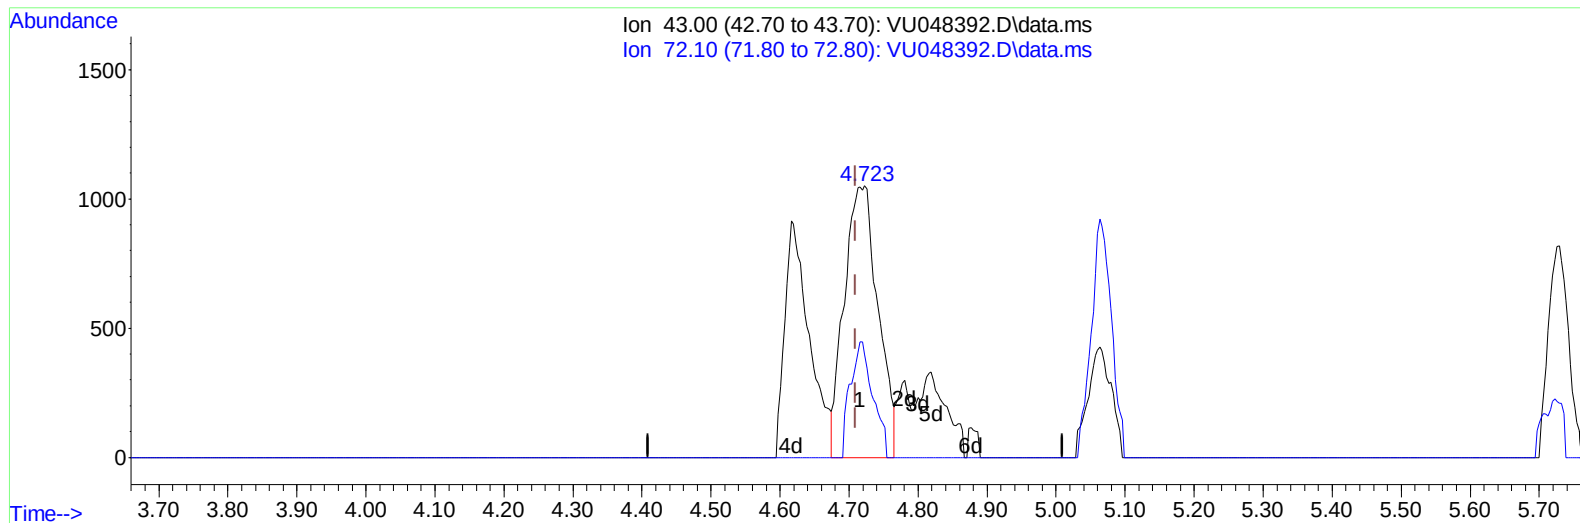**(22) 2-Butanone (T)**

4.723min (+ 0.013) 1.10 ug/L m

response 3547

Ion	Exp%	Act%
43.00	100.00	100.00
72.10	29.20	28.56
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048392.D
 Acq On : 03 May 2022 15:54
 Operator : SY/MD
 Sample : N2668-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL67

Manual IntegrationsAPPROVED

Quant Time: May 04 01:40:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 04 01:37:47 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	434190	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	431748	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	200485	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	214689	53.771	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	107.540%	
7) Chloroethane-d5	1.900	69	153302	54.699	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	109.400%	
11) 1,1-Dichloroethene-d2	2.562	63	251277	39.278	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	78.560%	
21) 2-Butanone-d5	4.620	46	303484	89.119	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	89.120%	
24) Chloroform-d	5.063	84	342717	47.323	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	94.640%	
26) 1,2-Dichloroethane-d4	5.700	65	213785	49.753	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	99.500%	
32) Benzene-d6	5.726	84	728002	53.464	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	106.920%	
36) 1,2-Dichloropropane-d6	6.690	67	232902	51.736	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	103.480%	
41) Toluene-d8	7.899	98	637962	51.687	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	103.380%	
43) trans-1,3-Dichloroprop...	8.179	79	97092	48.878	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	97.760%	
47) 2-Hexanone-d5	8.632	63	216664	89.207	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	89.210%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	356369	45.137	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	90.280%	
66) 1,2-Dichlorobenzene-d4	12.195	152	242321	53.730	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	107.460%	
Target Compounds						
						Qvalue
22) 2-Butanone	4.723	43	3547m	1.097	ug/L	
38) Bromodichloromethane	7.105	83	2244	0.489	ug/L	81
46) Tetrachloroethene	8.552	164	18614	6.922	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048392.D
Acq On : 03 May 2022 15:54
Operator : SY/MD
Sample : N2668-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 3

Instrument :
MSVOA_U
ClientSampleId :
EXL67

Manual IntegrationsAPPROVED

Quant Time: May 04 01:40:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 04 01:37:47 2022
Response via : Initial Calibration

Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

