

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048387.D
 Acq On : 03 May 2022 13:30
 Operator : SY/MD
 Sample : N2603-09ME
 Misc : 5.86g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW490ME

Quant Time: May 04 01:39:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 04 01:37:47 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 05/04/2022
 Supervised By : Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	467888	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.424	117	477884	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	250978	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	103150m	23.974	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	47.940%#		
7) Chloroethane-d5	1.874	69	23476	7.773	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	15.540%#		
11) 1,1-Dichloroethene-d2	2.533	63	154034	22.343	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	44.680%#		
21) 2-Butanone-d5	4.636	46	285379	77.767	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	77.770%		
24) Chloroform-d	5.064	84	280549	35.949	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	71.900%		
26) 1,2-Dichloroethane-d4	5.703	65	183285	39.583	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	79.160%		
32) Benzene-d6	5.723	84	580642	38.525	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	77.060%		
36) 1,2-Dichloropropane-d6	6.690	67	196723	39.481	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	78.960%		
41) Toluene-d8	7.899	98	530739	38.849	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	77.700%#		
43) trans-1,3-Dichloroprop...	8.186	79	86621	39.397	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.800%		
47) 2-Hexanone-d5	8.661	63	215555	80.182	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.180%		
56) 1,1,2,2-Tetrachloroeth...	10.768	84	338245	38.706	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	77.420%		
66) 1,2-Dichlorobenzene-d4	12.198	152	243441	43.119	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.240%		
Target Compounds					Qvalue	
22) 2-Butanone	4.723	43	37094	10.648	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048387.D
Acq On : 03 May 2022 13:30
Operator : SY/MD
Sample : N2603-09ME
Misc : 5.86g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
EW490ME

Quant Time: May 04 01:39:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 04 01:37:47 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

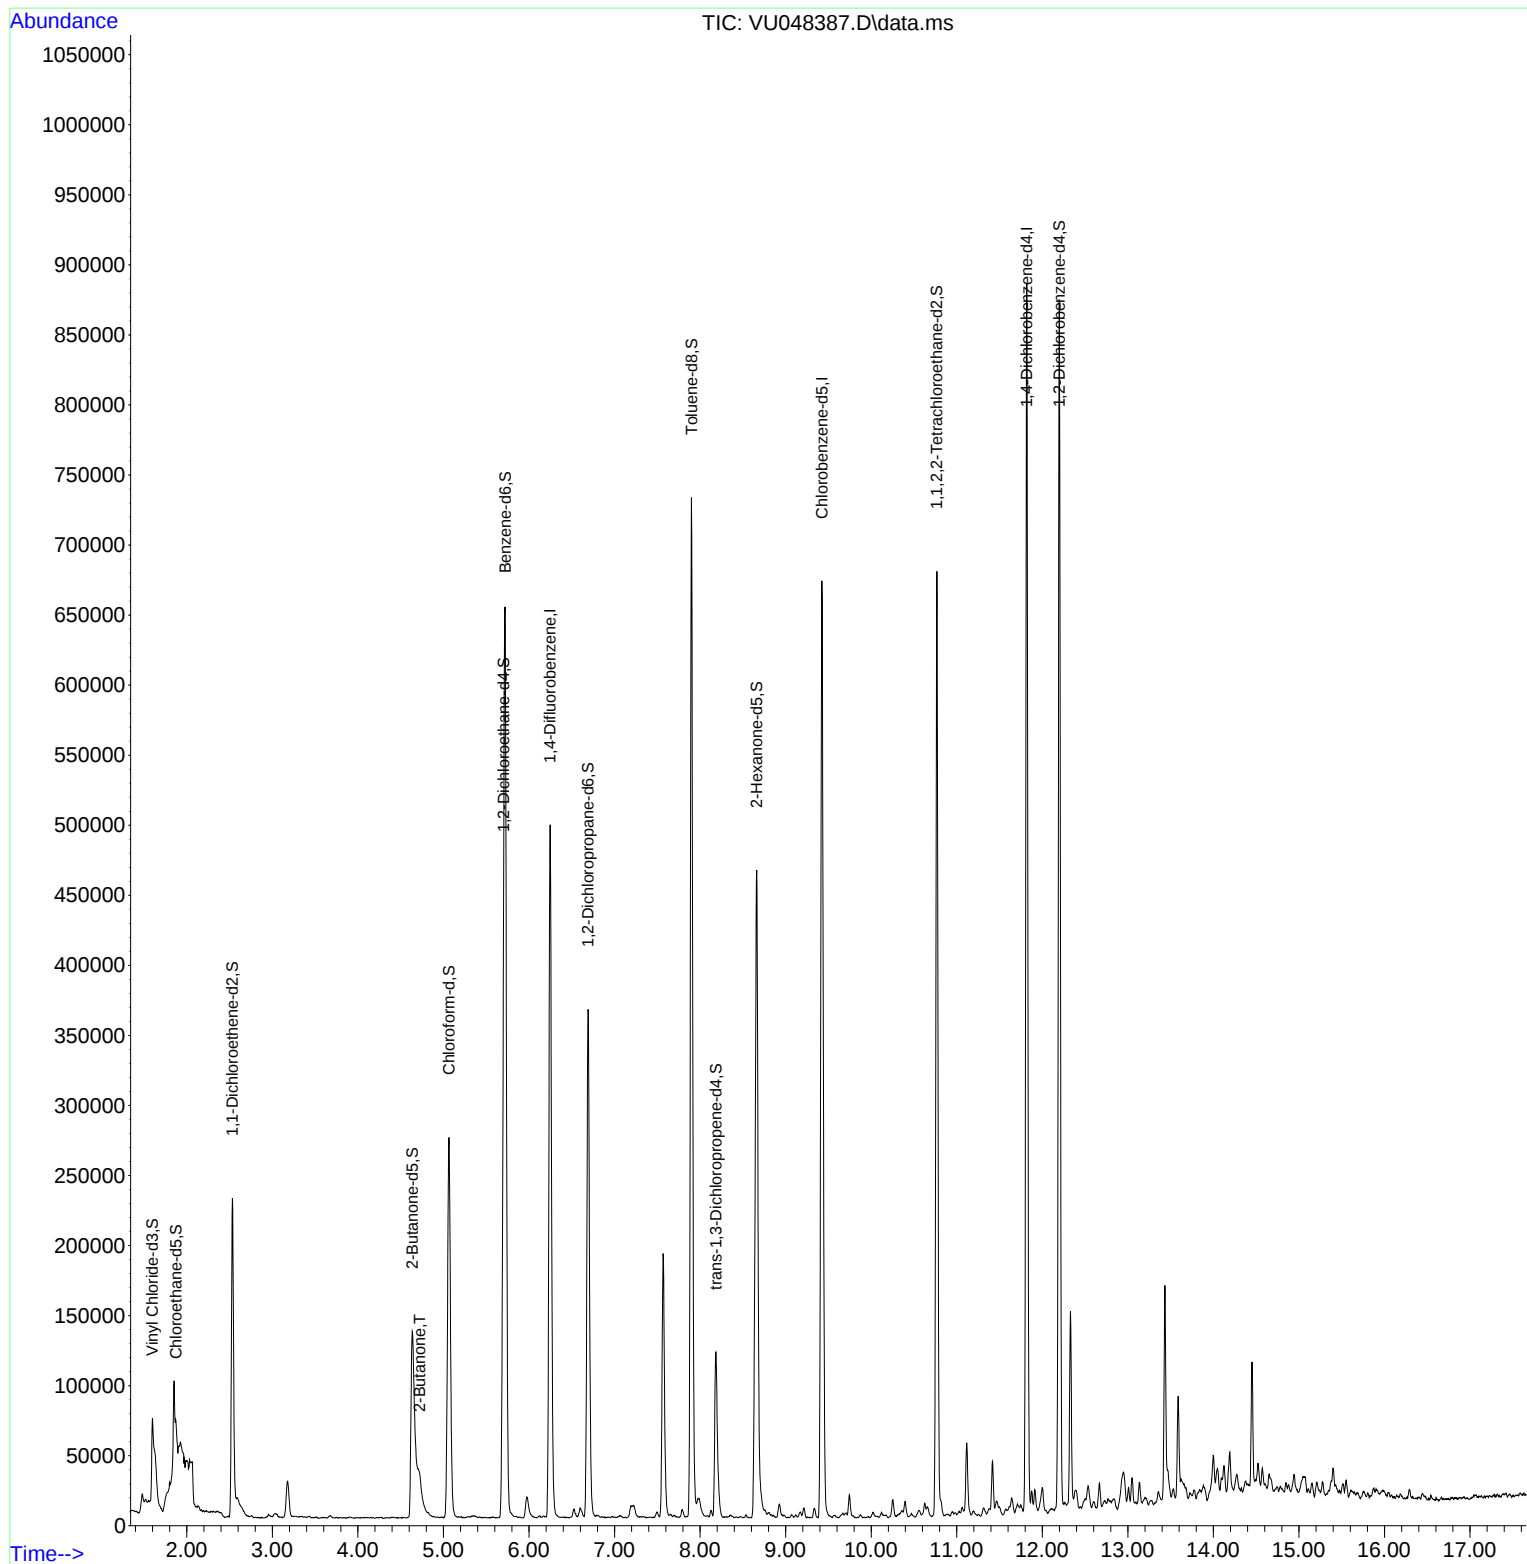

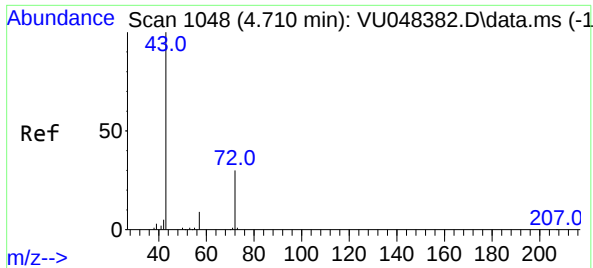

#22
 2-Butanone
 Concen: 10.648 ug/L
 RT: 4.723 min Scan# 1052
 Delta R.T. 0.013 min
 Lab File: VU048387.D
 Acq: 03 May 2022 13:30

Instrument :
 MSVOA_U
 ClientSampleId :
 EW490ME

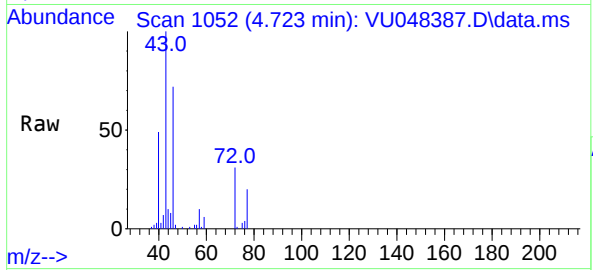

Tgt Ion: 43 Resp: 37094
 Ion Ratio Lower Upper
 43 100
 72 30.6 14.6 43.8

Manual Integrations
 APPROVED

Reviewed By :John Carlone 05/04/2022
 Supervised By :Mahesh Dadoda 05/04/2022

