

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048388.D
 Acq On : 03 May 2022 13:54
 Operator : SY/MD
 Sample : N2603-10ME
 Misc : 7.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW491ME

Quant Time: May 04 01:39:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed May 04 01:37:47 2022
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 05/04/2022
 Supervised By : Mahesh Dadoda 05/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	484909	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117	488514	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	242774	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	98967m	22.194	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	44.380%#		
7) Chloroethane-d5	1.874	69	24031	7.678	ug/L	-0.03
Spiked Amount 50.000	Range 70 - 130		Recovery =	15.360%#		
11) 1,1-Dichloroethene-d2	2.533	63	145528	20.369	ug/L	-0.03
Spiked Amount 50.000	Range 60 - 125		Recovery =	40.740%#		
21) 2-Butanone-d5	4.636	46	284323	74.759	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	74.760%		
24) Chloroform-d	5.063	84	268226	33.163	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	66.320%#		
26) 1,2-Dichloroethane-d4	5.700	65	178398	37.175	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	74.340%		
32) Benzene-d6	5.719	84	555080	36.028	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	72.060%		
36) 1,2-Dichloropropane-d6	6.690	67	189539	37.211	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	74.420%		
41) Toluene-d8	7.896	98	499163	35.742	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	71.480%#		
43) trans-1,3-Dichloroprop...	8.182	79	82068	36.514	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.020%		
47) 2-Hexanone-d5	8.658	63	212872	77.461	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	77.460%		
56) 1,1,2,2-Tetrachloroeth...	10.764	84	321575	35.997	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	72.000%		
66) 1,2-Dichlorobenzene-d4	12.198	152	221680	40.591	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	81.180%		
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.957	43	5532	1.141	ug/L	91
22) 2-Butanone	4.722	43	35938	9.954	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048388.D
Acq On : 03 May 2022 13:54
Operator : SY/MD
Sample : N2603-10ME
Misc : 7.46g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
EW491ME

Quant Time: May 04 01:39:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Wed May 04 01:37:47 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : John Carlone 05/04/2022
Supervised By : Mahesh Dadoda 05/04/2022

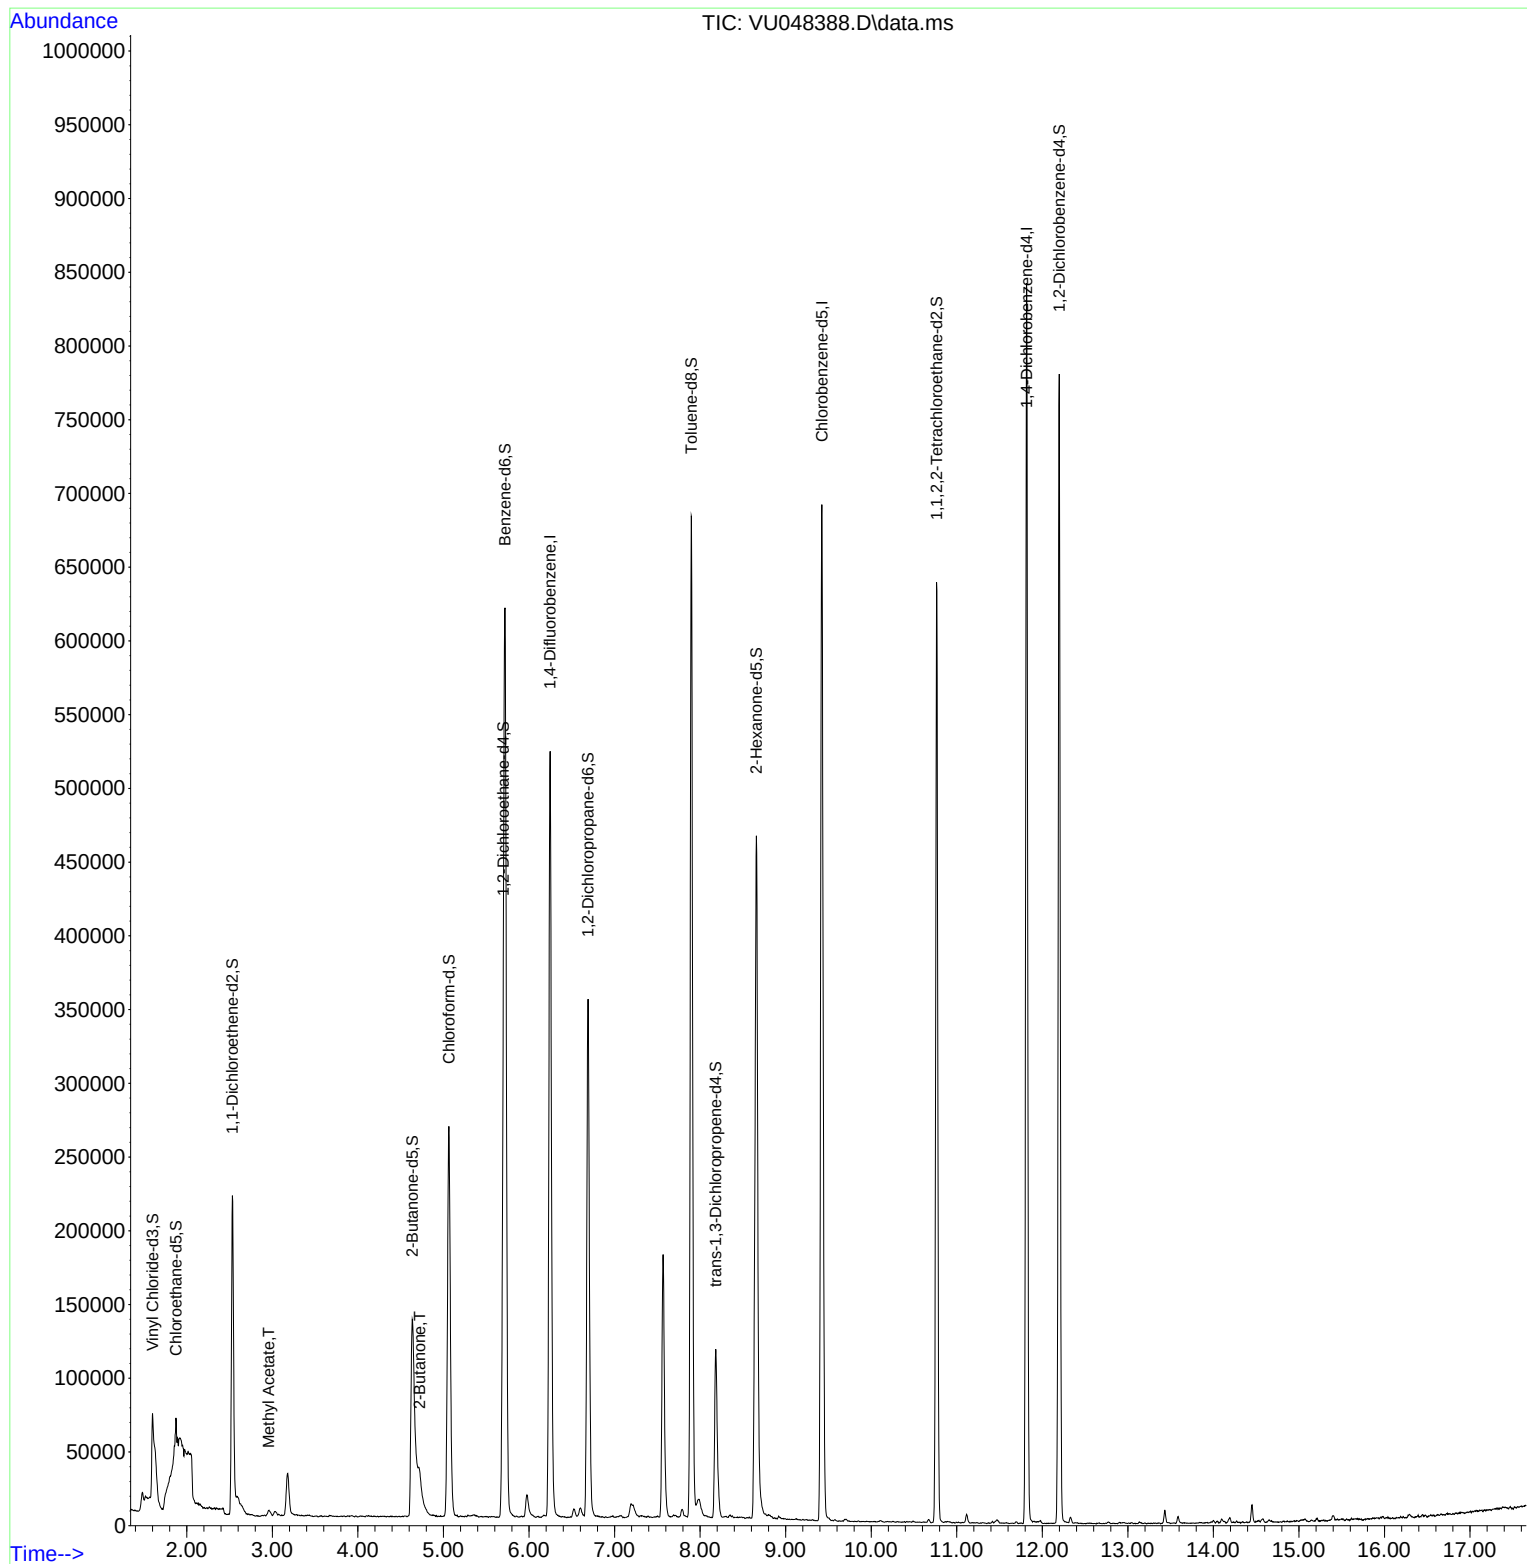

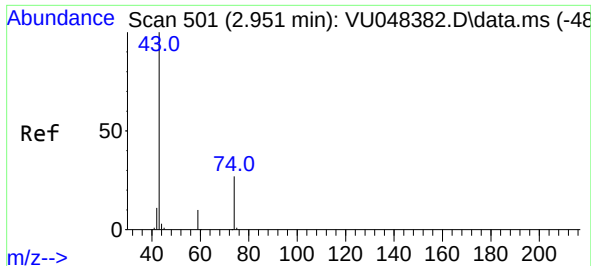

#15
Methyl Acetate
Concen: 1.141 ug/L
RT: 2.957 min Scan# 501
Delta R.T. 0.006 min
Lab File: VU048388.D
Acq: 03 May 2022 13:54




Instrument :
MSVOA_U
ClientSampleId :
EW491ME

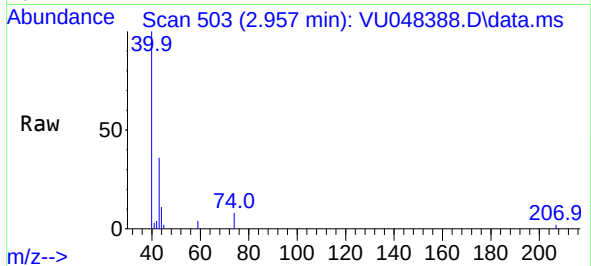


Tgt Ion: 43 Resp: 5532
Ion Ratio Lower Upper
43 100
74 21.7 21.0 31.6

Manual Integrations
APPROVED

Reviewed By :John Carlone 05/04/2022
Supervised By :Mahesh Dadoda 05/04/2022

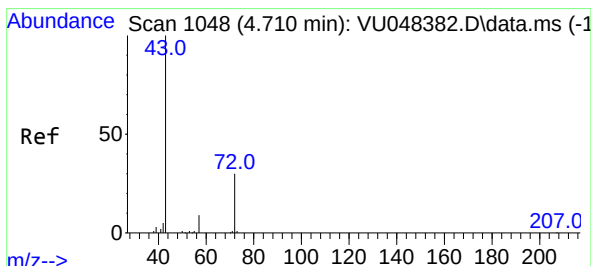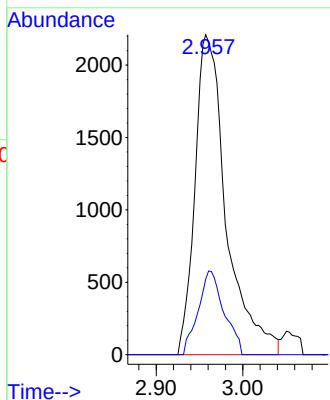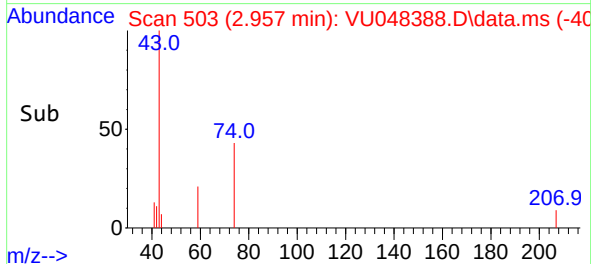

#22
2-Butanone
Concen: 9.954 ug/L
RT: 4.722 min Scan# 1052
Delta R.T. 0.013 min
Lab File: VU048388.D
Acq: 03 May 2022 13:54

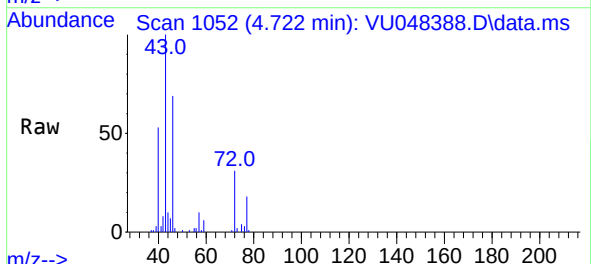

Tgt Ion: 43 Resp: 35938
Ion Ratio Lower Upper
43 100
72 31.0 14.6 43.8

