

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048383.D
 Acq On : 03 May 2022 10:30
 Operator : SY/MD
 Sample : VU0503MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	53	rBV4	5835	8398	0.43%	0.058%
2	1.600	73	81	100	rBV	263024	333513	16.97%	2.298%
3	1.893	163	172	188	rBV	168687	252878	12.87%	1.742%
4	2.562	367	380	403	rBV	430339	712206	36.24%	4.907%
5	2.729	430	432	434	rBV2	420	274	0.01%	0.002%
6	2.835	462	465	476	rVB3	816	713	0.04%	0.005%
7	2.877	476	478	481	rBV	402	222	0.01%	0.002%
8	2.903	483	486	492	rVB	616	482	0.02%	0.003%
9	3.051	527	532	543	rVB7	1981	3114	0.16%	0.021%
10	3.096	543	546	548	rBV	428	220	0.01%	0.002%
11	3.121	548	554	562	rBV2	571	836	0.04%	0.006%
12	3.179	562	572	575	rBV3	2402	3439	0.18%	0.024%
13	3.305	606	611	615	rVB	641	599	0.03%	0.004%
14	3.337	618	621	624	rBV2	499	417	0.02%	0.003%
15	3.359	624	628	631	rVV3	713	633	0.03%	0.004%
16	3.420	645	647	650	rVB	529	277	0.01%	0.002%
17	3.446	650	655	658	rBV2	400	394	0.02%	0.003%
18	3.536	680	683	686	rBV	600	371	0.02%	0.003%
19	3.613	703	707	710	rBV3	415	372	0.02%	0.003%
20	3.652	716	719	722	rBV2	434	297	0.02%	0.002%
21	3.681	725	728	731	rBV2	343	281	0.01%	0.002%
22	3.784	755	760	763	rBV2	462	502	0.03%	0.003%
23	3.819	768	771	775	rBV	458	405	0.02%	0.003%
24	3.848	778	780	782	rVV	506	256	0.01%	0.002%
25	3.861	782	784	791	rVB4	476	439	0.02%	0.003%
26	3.893	791	794	797	rBV	287	192	0.01%	0.001%
27	3.941	806	809	813	rVB	749	494	0.03%	0.003%
28	3.964	813	816	818	rBV2	348	239	0.01%	0.002%
29	3.980	818	821	824	rVV2	350	249	0.01%	0.002%
30	3.999	824	827	829	rVV	384	255	0.01%	0.002%
31	4.018	829	833	836	rVV	224	217	0.01%	0.001%
32	4.044	836	841	847	rVB	595	576	0.03%	0.004%
33	4.076	847	851	854	rBV2	311	204	0.01%	0.001%
34	4.102	855	859	863	rBV	343	389	0.02%	0.003%
35	4.153	871	875	877	rBV	432	306	0.02%	0.002%
36	4.170	877	880	885	rVB2	314	239	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048383.D
 Acq On : 03 May 2022 10:30
 Operator : SY/MD
 Sample : VU0503MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	4.195	886	888	891	rVB2	382	184	0.01%	0.001%
38	4.218	891	895	896	rBV	409	292	0.01%	0.002%
39	4.263	906	909	911	rBV2	421	292	0.01%	0.002%
40	4.308	917	923	926	rBV	768	669	0.03%	0.005%
41	4.337	926	932	935	rBV2	620	532	0.03%	0.004%
42	4.353	935	937	941	rBV	325	218	0.01%	0.002%
43	4.375	941	944	946	rBV	387	214	0.01%	0.001%
44	4.407	952	954	957	rBV2	391	267	0.01%	0.002%
45	4.430	957	961	965	rVV2	463	437	0.02%	0.003%
46	4.472	972	974	977	rBV	304	154	0.01%	0.001%
47	4.533	988	993	1000	rVB	716	882	0.04%	0.006%
48	4.571	1001	1005	1006	rBV	432	284	0.01%	0.002%
49	4.620	1006	1020	1045	rBV	205234	497453	25.31%	3.427%
50	4.867	1094	1097	1103	rBV2	590	653	0.03%	0.004%
51	4.928	1113	1116	1118	rBV2	505	315	0.02%	0.002%
52	4.944	1118	1121	1125	rVV2	689	556	0.03%	0.004%
53	4.973	1128	1130	1136	rVB2	768	587	0.03%	0.004%
54	4.999	1136	1138	1140	rBV	241	134	0.01%	0.001%
55	5.063	1140	1158	1186	rVV	344948	757312	38.54%	5.218%
56	5.173	1186	1192	1196	rBV2	719	766	0.04%	0.005%
57	5.211	1201	1204	1205	rBV2	396	235	0.01%	0.002%
58	5.247	1211	1215	1220	rVB2	812	715	0.04%	0.005%
59	5.292	1225	1229	1231	rBV2	453	391	0.02%	0.003%
60	5.420	1265	1269	1270	rBV	379	271	0.01%	0.002%
61	5.430	1270	1272	1274	rVV2	393	253	0.01%	0.002%
62	5.443	1274	1276	1278	rVV	452	290	0.01%	0.002%
63	5.456	1278	1280	1283	rVV	599	389	0.02%	0.003%
64	5.472	1283	1285	1287	rVV2	390	210	0.01%	0.001%
65	5.485	1287	1289	1291	rVV	324	196	0.01%	0.001%
66	5.501	1291	1294	1296	rVV	522	294	0.01%	0.002%
67	5.523	1296	1301	1307	rVB3	838	959	0.05%	0.007%
68	5.549	1307	1309	1312	rVB	605	270	0.01%	0.002%
69	5.578	1316	1318	1321	rVB	523	293	0.01%	0.002%
70	5.613	1321	1329	1332	rBV2	552	793	0.04%	0.005%
71	5.726	1342	1364	1398	rBV2	735702	1965113	100.00%	13.539%
72	5.951	1431	1434	1435	rBV	446	260	0.01%	0.002%
73	5.967	1435	1439	1456	rVB5	1264	2353	0.12%	0.016%
74	6.031	1456	1459	1464	rBV4	657	744	0.04%	0.005%
75	6.141	1491	1493	1495	rBV	422	213	0.01%	0.001%
76	6.157	1495	1498	1502	rVV2	519	442	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048383.D
 Acq On : 03 May 2022 10:30
 Operator : SY/MD
 Sample : VU0503MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	6.250	1512	1527	1549	rBV	445225	845692	43.04%	5.827%
78	6.539	1606	1617	1625	rBV6	3040	5404	0.27%	0.037%
79	6.587	1630	1632	1635	rVB3	1029	550	0.03%	0.004%
80	6.690	1649	1664	1682	rBV	446135	863646	43.95%	5.950%
81	6.838	1708	1710	1711	rBV2	504	223	0.01%	0.002%
82	7.565	1923	1936	1955	rBV	238697	416159	21.18%	2.867%
83	7.899	2026	2040	2057	rBV	907628	1576451	80.22%	10.861%
84	8.179	2115	2127	2145	rBV	170474	285575	14.53%	1.968%
85	8.468	2214	2217	2221	rBV2	815	819	0.04%	0.006%
86	8.636	2256	2269	2315	rBV	638997	1190683	60.59%	8.204%
87	9.417	2499	2512	2541	rBV	663522	1108171	56.39%	7.635%
88	9.574	2555	2561	2569	rVB5	1718	2341	0.12%	0.016%
89	9.690	2593	2597	2606	rVB5	2171	3314	0.17%	0.023%
90	10.298	2784	2786	2789	rBV	835	524	0.03%	0.004%
91	10.758	2915	2929	2946	rBV	733310	1186529	60.38%	8.175%
92	11.465	3142	3149	3164	rVB8	3441	6934	0.35%	0.048%
93	11.742	3232	3235	3238	rBV4	1779	1381	0.07%	0.010%
94	11.812	3244	3257	3281	rBV	646790	1032400	52.54%	7.113%
95	12.076	3336	3339	3341	rBV	760	517	0.03%	0.004%
96	12.195	3363	3376	3395	rBV	844632	1383158	70.39%	9.530%
97	13.224	3692	3696	3706	rVB6	3006	4208	0.21%	0.029%
98	13.848	3883	3890	3901	rVB5	5649	8408	0.43%	0.058%
99	14.092	3959	3966	3978	rVB2	11069	18087	0.92%	0.125%
100	14.330	4034	4040	4054	rVB5	6425	11295	0.57%	0.078%




Sum of corrected areas: 14514252

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048383.D
Acq On : 03 May 2022 10:30
Operator : SY/MD
Sample : VU0503MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

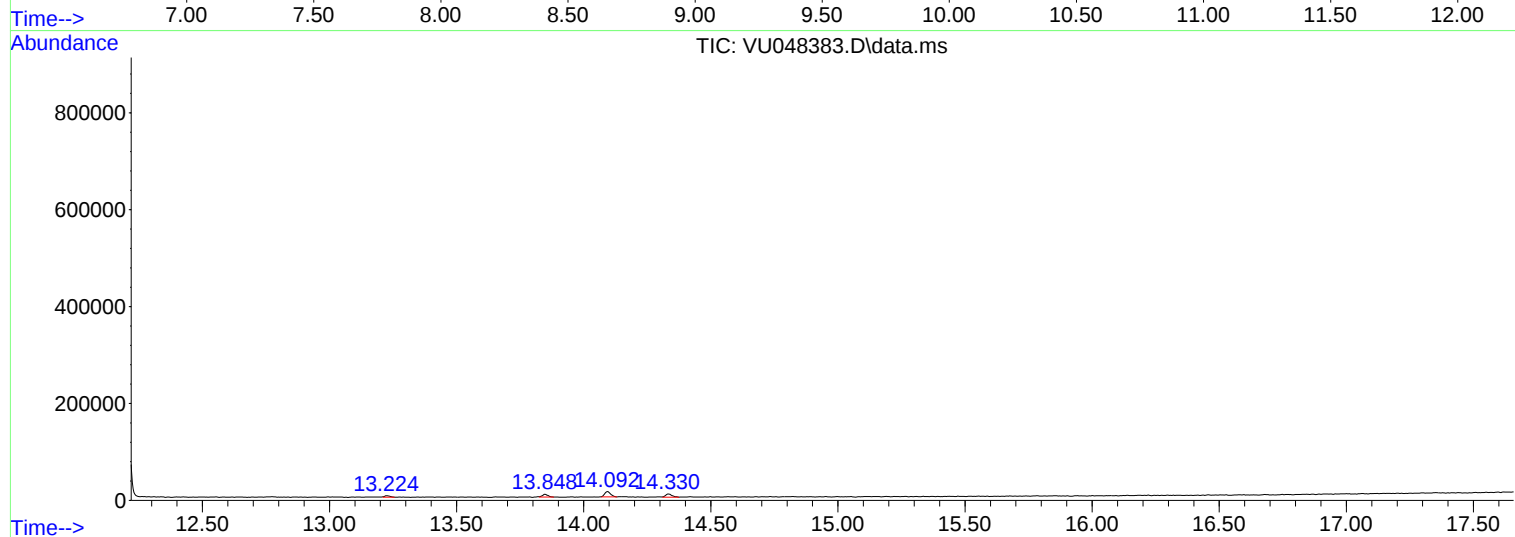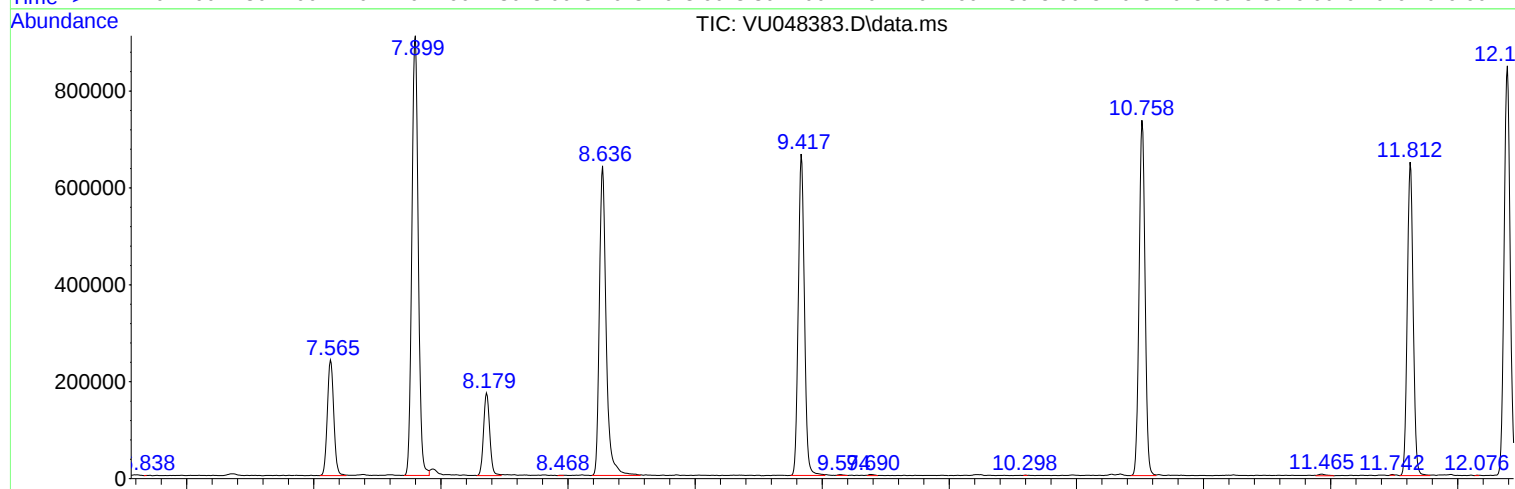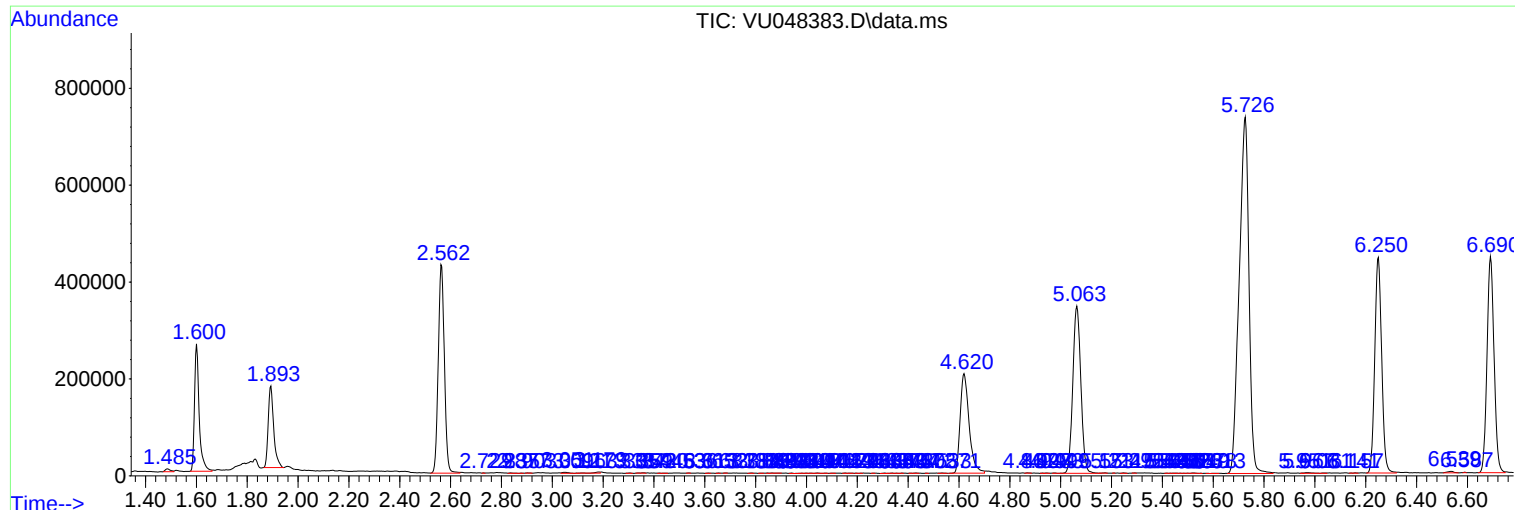

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048383.D
Acq On : 03 May 2022 10:30
Operator : SY/MD
Sample : VU0503MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048383.D
Acq On : 03 May 2022 10:30
Operator : SY/MD
Sample : VU0503MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
