

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048384.D
 Acq On : 03 May 2022 11:14
 Operator : SY/MD
 Sample : VU0503WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	51	rBV3	6019	8691	0.43%	0.057%
2	1.601	73	81	102	rBV	255130	332530	16.52%	2.188%
3	1.887	162	170	190	rVB	170936	269586	13.39%	1.774%
4	2.514	362	365	367	rBV	1096	613	0.03%	0.004%
5	2.562	367	380	401	rVV	440066	722560	35.89%	4.755%
6	2.906	483	487	490	rBV	792	727	0.04%	0.005%
7	3.186	571	574	580	rVB2	2136	1758	0.09%	0.012%
8	3.440	650	653	655	rBV	712	523	0.03%	0.003%
9	4.099	853	858	860	rBV	666	703	0.03%	0.005%
10	4.237	898	901	903	rBV2	670	494	0.02%	0.003%
11	4.298	918	920	922	rBV2	559	333	0.02%	0.002%
12	4.488	976	979	981	rBV	877	579	0.03%	0.004%
13	4.620	1006	1020	1056	rBV	204623	507880	25.23%	3.342%
14	4.925	1112	1115	1120	rBV2	656	528	0.03%	0.003%
15	5.063	1142	1158	1178	rVB	352966	763639	37.93%	5.025%
16	5.575	1314	1317	1319	rBV2	884	592	0.03%	0.004%
17	5.723	1342	1363	1393	rBV2	755430	2013386	100.00%	13.250%
18	6.018	1452	1455	1459	rBV	627	516	0.03%	0.003%
19	6.247	1512	1526	1545	rBV	497645	938376	46.61%	6.175%
20	6.690	1649	1664	1685	rBV	457887	889485	44.18%	5.854%
21	6.989	1754	1757	1762	rBV2	596	756	0.04%	0.005%
22	7.176	1807	1815	1829	rVB8	3744	7766	0.39%	0.051%
23	7.314	1853	1858	1862	rBV	562	767	0.04%	0.005%
24	7.565	1923	1936	1955	rBV	240727	418153	20.77%	2.752%
25	7.758	1993	1996	2000	rBV3	669	641	0.03%	0.004%
26	7.848	2019	2024	2026	rBV2	824	817	0.04%	0.005%
27	7.896	2026	2039	2056	rBV	938034	1623865	80.65%	10.686%
28	8.115	2105	2107	2112	rBV2	402	291	0.01%	0.002%
29	8.179	2115	2127	2144	rBV	170579	285279	14.17%	1.877%
30	8.314	2167	2169	2172	rBV	566	355	0.02%	0.002%
31	8.468	2214	2217	2219	rBV2	605	401	0.02%	0.003%
32	8.636	2255	2269	2298	rVV	663702	1217668	60.48%	8.013%
33	8.867	2337	2341	2346	rBV3	767	591	0.03%	0.004%
34	8.976	2367	2375	2383	rVB2	1174	1962	0.10%	0.013%
35	9.012	2383	2386	2389	rBV2	756	702	0.03%	0.005%
36	9.073	2402	2405	2407	rBV	292	224	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048384.D
 Acq On : 03 May 2022 11:14
 Operator : SY/MD
 Sample : VU0503WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	9.095	2408	2412	2418	rVB2	533	625	0.03%	0.004%
38	9.121	2418	2420	2423	rBV3	413	233	0.01%	0.002%
39	9.160	2428	2432	2435	rBV2	968	837	0.04%	0.006%
40	9.208	2444	2447	2450	rVB2	536	366	0.02%	0.002%
41	9.237	2450	2456	2461	rBV2	591	584	0.03%	0.004%
42	9.275	2461	2468	2471	rBV2	676	727	0.04%	0.005%
43	9.320	2477	2482	2483	rBV	536	428	0.02%	0.003%
44	9.417	2498	2512	2545	rBV	730867	1226886	60.94%	8.074%
45	9.555	2553	2555	2557	rBV	723	450	0.02%	0.003%
46	9.610	2569	2572	2576	rBV2	494	342	0.02%	0.002%
47	9.629	2576	2578	2581	rVV	377	215	0.01%	0.001%
48	9.648	2581	2584	2587	rVB2	556	406	0.02%	0.003%
49	9.693	2591	2598	2605	rVB5	992	1274	0.06%	0.008%
50	9.745	2609	2614	2617	rVB	458	423	0.02%	0.003%
51	9.767	2617	2621	2625	rBV2	563	392	0.02%	0.003%
52	9.851	2644	2647	2650	rBV	298	215	0.01%	0.001%
53	9.890	2656	2659	2664	rVB2	404	314	0.02%	0.002%
54	9.919	2665	2668	2671	rVV	497	352	0.02%	0.002%
55	9.964	2675	2682	2685	rVB2	652	626	0.03%	0.004%
56	10.002	2690	2694	2700	rBV2	599	754	0.04%	0.005%
57	10.054	2706	2710	2715	rVB	893	676	0.03%	0.004%
58	10.079	2715	2718	2721	rBV2	357	252	0.01%	0.002%
59	10.118	2724	2730	2737	rVB4	977	1200	0.06%	0.008%
60	10.150	2737	2740	2743	rVB2	831	493	0.02%	0.003%
61	10.185	2743	2751	2753	rBV2	552	748	0.04%	0.005%
62	10.227	2760	2764	2766	rBV2	314	274	0.01%	0.002%
63	10.362	2800	2806	2810	rBV2	947	974	0.05%	0.006%
64	10.423	2822	2825	2830	rVB2	436	306	0.02%	0.002%
65	10.452	2830	2834	2838	rBV2	593	605	0.03%	0.004%
66	10.472	2838	2840	2842	rBV	438	248	0.01%	0.002%
67	10.488	2842	2845	2849	rVB2	925	673	0.03%	0.004%
68	10.513	2850	2853	2854	rBV2	391	228	0.01%	0.002%
69	10.568	2867	2870	2875	rVV2	339	396	0.02%	0.003%
70	10.639	2888	2892	2895	rBV2	700	584	0.03%	0.004%
71	10.668	2895	2901	2914	rVB4	3779	6086	0.30%	0.040%
72	10.758	2914	2929	2950	rBV	747353	1215555	60.37%	7.999%
73	10.957	2988	2991	2999	rVB2	610	767	0.04%	0.005%
74	11.021	3008	3011	3014	rBV	464	301	0.01%	0.002%
75	11.115	3035	3040	3049	rVB5	1366	1885	0.09%	0.012%
76	11.179	3054	3060	3063	rVB2	758	672	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048384.D
 Acq On : 03 May 2022 11:14
 Operator : SY/MD
 Sample : VU0503WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.198	3063	3066	3068	rBV2	557	302	0.01%	0.002%
78	11.214	3068	3071	3077	rBV3	426	428	0.02%	0.003%
79	11.269	3085	3088	3094	rBV2	581	558	0.03%	0.004%
80	11.317	3100	3103	3106	rBV3	530	429	0.02%	0.003%
81	11.459	3140	3147	3160	rVB7	2294	4690	0.23%	0.031%
82	11.542	3169	3173	3177	rBV	524	436	0.02%	0.003%
83	11.571	3177	3182	3188	rVB2	817	975	0.05%	0.006%
84	11.613	3193	3195	3200	rVB	424	316	0.02%	0.002%
85	11.645	3203	3205	3212	rVB2	342	264	0.01%	0.002%
86	11.687	3213	3218	3220	rBV4	1176	1062	0.05%	0.007%
87	11.748	3233	3237	3244	rVB4	933	978	0.05%	0.006%
88	11.812	3244	3257	3275	rBV	762329	1203791	59.79%	7.922%
89	12.037	3322	3327	3330	rBV2	743	705	0.04%	0.005%
90	12.082	3339	3341	3344	rVB2	922	473	0.02%	0.003%
91	12.192	3362	3375	3394	rBV	907780	1489096	73.96%	9.799%
92	12.674	3521	3525	3526	rBV2	496	393	0.02%	0.003%
93	12.764	3549	3553	3561	rBV3	1124	1512	0.08%	0.010%
94	12.825	3568	3572	3573	rBV	760	512	0.03%	0.003%
95	12.941	3604	3608	3616	rBV2	763	1181	0.06%	0.008%
96	12.976	3616	3619	3622	rBV2	796	609	0.03%	0.004%
97	13.063	3644	3646	3649	rBV2	517	364	0.02%	0.002%
98	13.304	3718	3721	3726	rBV2	787	810	0.04%	0.005%
99	13.925	3911	3914	3917	rBV2	961	729	0.04%	0.005%
100	14.336	4039	4042	4052	rVB3	1903	2016	0.10%	0.013%




Sum of corrected areas: 15195738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048384.D
Acq On : 03 May 2022 11:14
Operator : SY/MD
Sample : VU0503WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

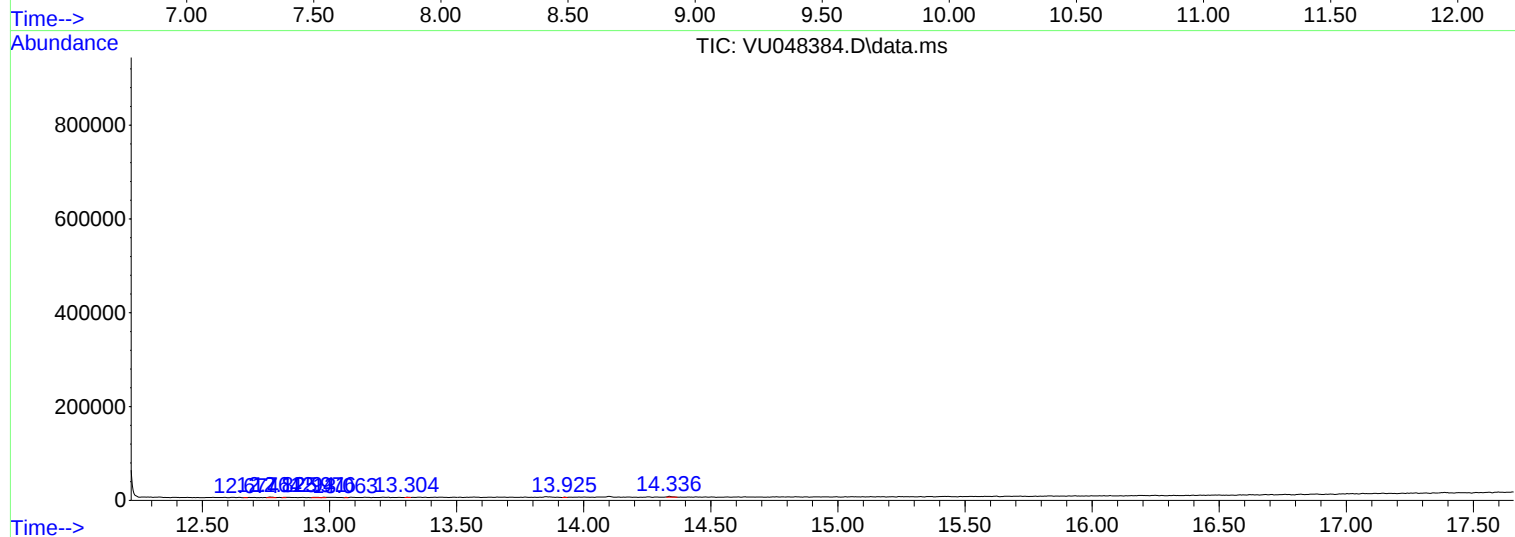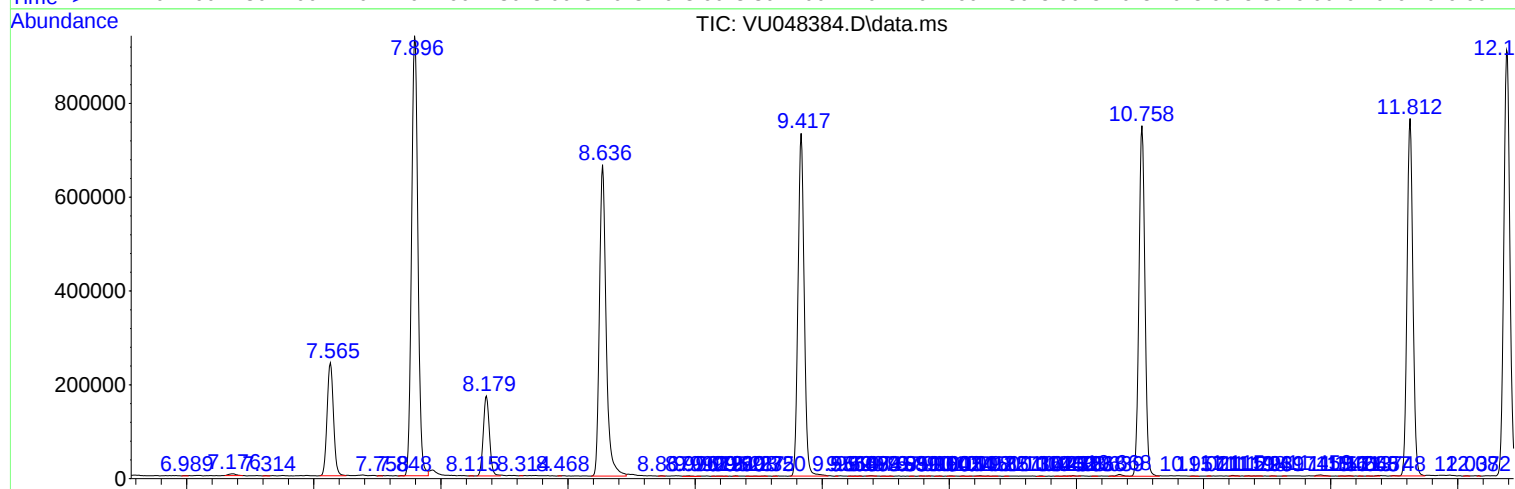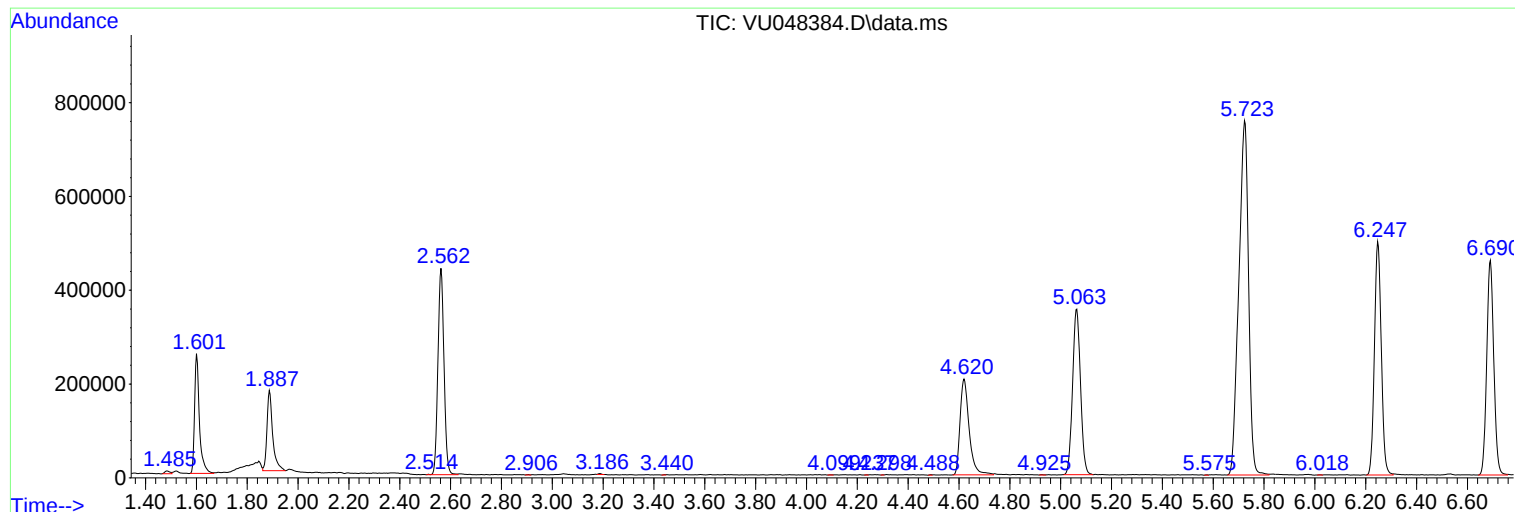

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048384.D
Acq On : 03 May 2022 11:14
Operator : SY/MD
Sample : VU0503WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048384.D
Acq On : 03 May 2022 11:14
Operator : SY/MD
Sample : VU0503WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc