

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048390.D
 Acq On : 03 May 2022 15:07
 Operator : SY/MD
 Sample : N2668-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	104	rBV	258792	337795	16.86%	2.277%
2	1.903	166	175	210	rVB	183538	292870	14.62%	1.974%
3	2.565	368	381	397	rBV	444056	721260	36.01%	4.862%
4	2.793	435	452	471	rVV2	5664	17070	0.85%	0.115%
5	2.861	471	473	477	rVV2	554	335	0.02%	0.002%
6	2.954	498	502	504	rBV2	227	187	0.01%	0.001%
7	3.047	525	531	534	rBV2	880	1002	0.05%	0.007%
8	3.189	559	575	599	rBV	19291	52749	2.63%	0.356%
9	3.378	632	634	638	rVV	227	190	0.01%	0.001%
10	3.407	641	643	647	rVV2	320	255	0.01%	0.002%
11	3.430	648	650	654	rVV	320	227	0.01%	0.002%
12	3.459	655	659	664	rVB2	262	233	0.01%	0.002%
13	3.674	724	726	734	rVB	298	298	0.01%	0.002%
14	3.710	734	737	742	rBV	220	201	0.01%	0.001%
15	3.771	751	756	758	rBV2	203	187	0.01%	0.001%
16	3.845	773	779	782	rVV2	162	211	0.01%	0.001%
17	4.089	849	855	858	rVV	283	250	0.01%	0.002%
18	4.623	1005	1021	1054	rBV	203634	507150	25.32%	3.419%
19	4.915	1109	1112	1114	rBV2	274	180	0.01%	0.001%
20	5.063	1142	1158	1183	rBV	353947	767900	38.34%	5.177%
21	5.279	1222	1225	1227	rBV2	409	326	0.02%	0.002%
22	5.330	1236	1241	1246	rBV3	610	868	0.04%	0.006%
23	5.726	1342	1364	1398	rBV2	752449	2003025	100.00%	13.503%
24	5.886	1411	1414	1424	rVB6	982	1062	0.05%	0.007%
25	5.948	1430	1433	1435	rBV	335	221	0.01%	0.001%
26	5.967	1435	1439	1441	rBV3	493	364	0.02%	0.002%
27	6.034	1456	1460	1462	rBV3	437	327	0.02%	0.002%
28	6.108	1480	1483	1486	rBV2	262	187	0.01%	0.001%
29	6.144	1491	1494	1497	rBV3	449	351	0.02%	0.002%
30	6.173	1500	1503	1508	rVB2	390	309	0.02%	0.002%
31	6.250	1508	1527	1558	rBV	499876	950819	47.47%	6.410%
32	6.427	1580	1582	1587	rVB3	317	192	0.01%	0.001%
33	6.475	1591	1597	1602	rBV3	267	299	0.01%	0.002%
34	6.529	1606	1614	1625	rBV5	2051	4195	0.21%	0.028%
35	6.578	1628	1629	1632	rVB	576	291	0.01%	0.002%
36	6.600	1632	1636	1640	rBV4	754	699	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048390.D
 Acq On : 03 May 2022 15:07
 Operator : SY/MD
 Sample : N2668-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.690	1646	1664	1684	rBV	452005	886205	44.24%	5.974%
38	6.800	1694	1698	1700	rBV3	857	657	0.03%	0.004%
39	6.947	1738	1744	1745	rVV2	293	242	0.01%	0.002%
40	7.034	1763	1771	1772	rBV2	400	366	0.02%	0.002%
41	7.115	1794	1796	1802	rBV2	246	257	0.01%	0.002%
42	7.179	1806	1816	1830	rBV7	3880	8206	0.41%	0.055%
43	7.301	1850	1854	1857	rBV	245	211	0.01%	0.001%
44	7.446	1897	1899	1906	rBV2	261	297	0.01%	0.002%
45	7.565	1919	1936	1964	rBV	234914	419687	20.95%	2.829%
46	7.687	1969	1974	1985	rVB6	1721	2752	0.14%	0.019%
47	7.755	1991	1995	1999	rVB4	342	281	0.01%	0.002%
48	7.803	2002	2010	2013	rBV2	377	499	0.02%	0.003%
49	7.835	2017	2020	2023	rVB2	431	233	0.01%	0.002%
50	7.899	2023	2040	2056	rBV	917204	1584500	79.11%	10.682%
51	8.179	2116	2127	2153	rVV	163859	280097	13.98%	1.888%
52	8.407	2196	2198	2207	rVB5	435	308	0.02%	0.002%
53	8.475	2209	2219	2230	rVB	4953	9266	0.46%	0.062%
54	8.542	2238	2240	2247	rVB	501	434	0.02%	0.003%
55	8.574	2247	2250	2253	rBV	324	178	0.01%	0.001%
56	8.636	2253	2269	2296	rBV	617187	1132451	56.54%	7.634%
57	8.880	2341	2345	2348	rBV3	227	199	0.01%	0.001%
58	8.992	2378	2380	2385	rVB	354	244	0.01%	0.002%
59	9.121	2417	2420	2423	rVB2	324	205	0.01%	0.001%
60	9.169	2430	2435	2441	rVB3	503	660	0.03%	0.004%
61	9.365	2493	2496	2499	rBV2	262	206	0.01%	0.001%
62	9.417	2499	2512	2552	rVV	705310	1177429	58.78%	7.937%
63	9.629	2575	2578	2580	rVV3	263	183	0.01%	0.001%
64	9.648	2581	2584	2587	rVV	504	326	0.02%	0.002%
65	9.664	2587	2589	2592	rVV	321	200	0.01%	0.001%
66	9.693	2592	2598	2606	rVV4	839	1113	0.06%	0.008%
67	9.963	2679	2682	2683	rBV	381	191	0.01%	0.001%
68	10.066	2711	2714	2718	rVB2	222	179	0.01%	0.001%
69	10.201	2753	2756	2760	rVB2	272	180	0.01%	0.001%
70	10.227	2760	2764	2774	rVB2	350	357	0.02%	0.002%
71	10.343	2796	2800	2808	rVB2	325	468	0.02%	0.003%
72	10.488	2837	2845	2846	rBV	261	279	0.01%	0.002%
73	10.587	2872	2876	2878	rBV2	311	197	0.01%	0.001%
74	10.671	2894	2902	2911	rBV4	3147	4371	0.22%	0.029%
75	10.758	2916	2929	2951	rBV	701342	1123493	56.09%	7.574%
76	10.893	2961	2971	2986	rVB2	10018	16859	0.84%	0.114%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048390.D
 Acq On : 03 May 2022 15:07
 Operator : SY/MD
 Sample : N2668-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL46

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.951	2986	2989	2993	rVB3	380	238	0.01%	0.002%
78	11.111	3036	3039	3043	rBV2	739	668	0.03%	0.005%
79	11.153	3049	3052	3055	rVB2	302	191	0.01%	0.001%
80	11.188	3061	3063	3067	rBV2	207	201	0.01%	0.001%
81	11.455	3138	3146	3157	rBV6	2361	3669	0.18%	0.025%
82	11.693	3216	3220	3229	rVB5	1294	1842	0.09%	0.012%
83	11.748	3233	3237	3243	rVB3	388	319	0.02%	0.002%
84	11.812	3243	3257	3274	rBV	697766	1107101	55.27%	7.463%
85	11.973	3304	3307	3314	rVB3	2694	2880	0.14%	0.019%
86	12.005	3314	3317	3319	rBV3	287	184	0.01%	0.001%
87	12.092	3341	3344	3348	rVB3	364	281	0.01%	0.002%
88	12.134	3355	3357	3360	rBV2	253	205	0.01%	0.001%
89	12.192	3360	3375	3391	rBV	865357	1386097	69.20%	9.344%
90	12.323	3414	3416	3422	rBV6	531	478	0.02%	0.003%
91	12.397	3437	3439	3442	rBV	370	252	0.01%	0.002%
92	12.574	3488	3494	3496	rBV2	468	395	0.02%	0.003%
93	12.639	3511	3514	3522	rVB3	456	516	0.03%	0.003%
94	12.770	3547	3555	3564	rBV3	3890	5612	0.28%	0.038%
95	13.436	3757	3762	3770	rVB5	767	789	0.04%	0.005%
96	13.574	3802	3805	3810	rBV3	413	407	0.02%	0.003%
97	14.024	3942	3945	3947	rBV	345	258	0.01%	0.002%
98	14.455	4072	4079	4088	rVB6	1372	2124	0.11%	0.014%
99	14.552	4107	4109	4111	rVB2	635	193	0.01%	0.001%
100	14.960	4234	4236	4239	rBV2	645	371	0.02%	0.003%




Sum of corrected areas: 14833822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048390.D
Acq On : 03 May 2022 15:07
Operator : SY/MD
Sample : N2668-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

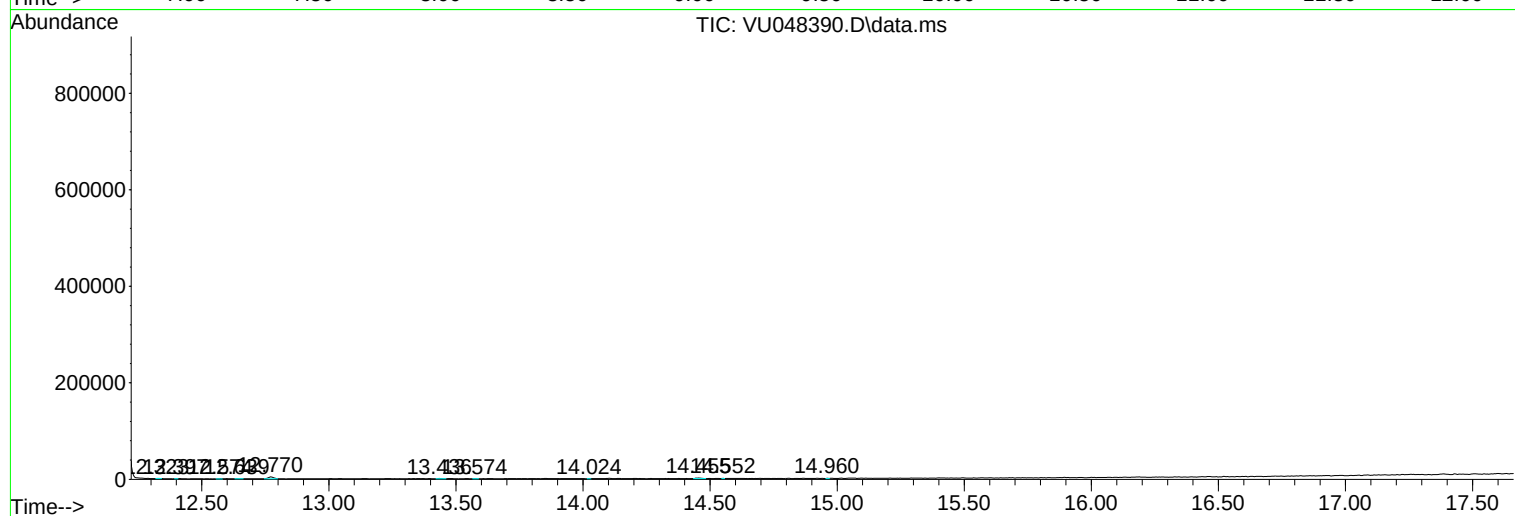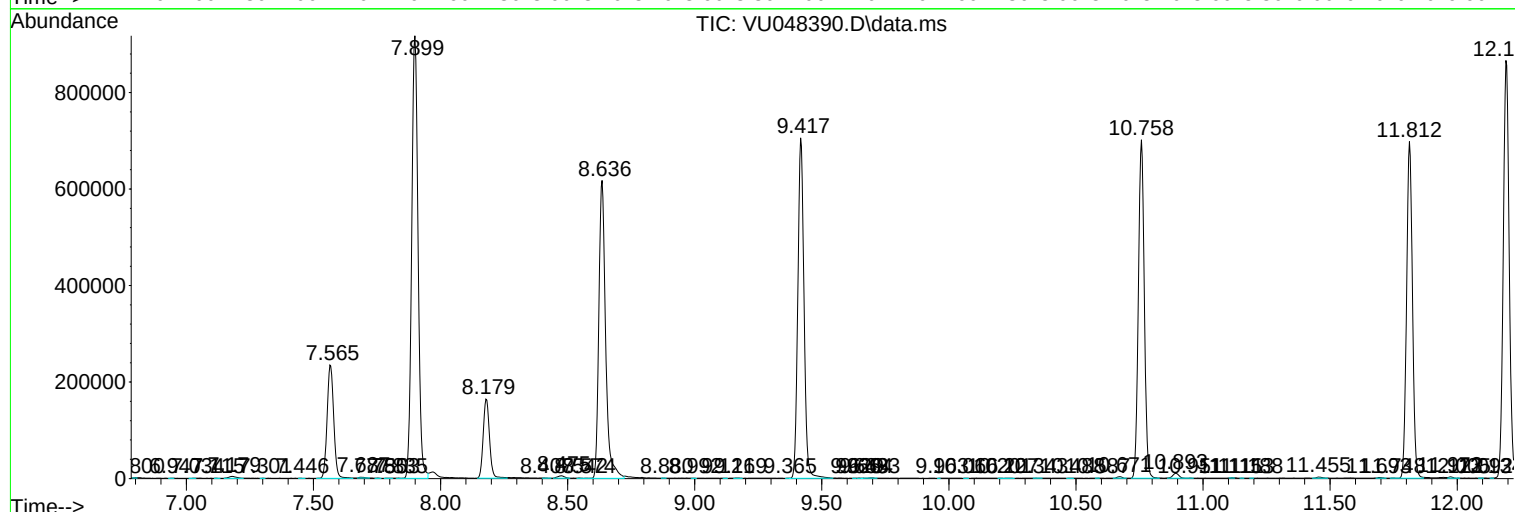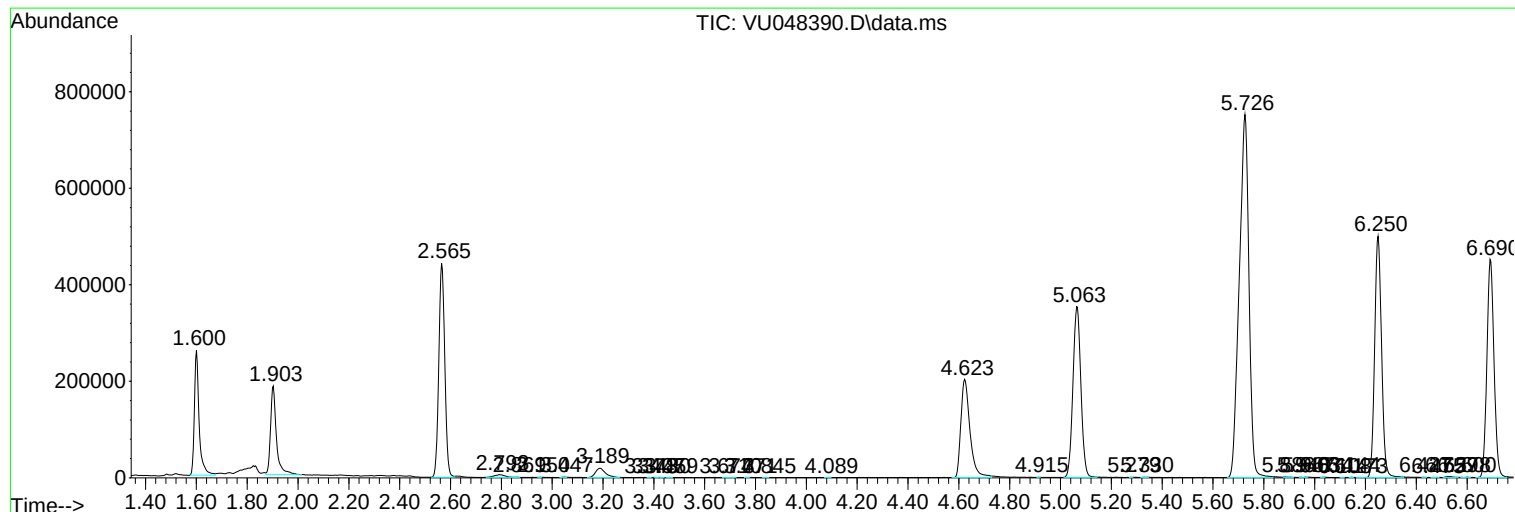

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048390.D
Acq On : 03 May 2022 15:07
Operator : SY/MD
Sample : N2668-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048390.D
Acq On : 03 May 2022 15:07
Operator : SY/MD
Sample : N2668-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------