

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048391.D
 Acq On : 03 May 2022 15:31
 Operator : SY/MD
 Sample : N2668-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	41	46	51	rBV3	4831	5080	0.25%	0.034%
2	1.601	73	81	98	rBV	267378	342868	16.98%	2.319%
3	1.900	166	174	189	rBV	178612	262330	12.99%	1.774%
4	2.565	367	381	398	rBV	444925	722367	35.77%	4.885%
5	2.684	416	418	420	rBV2	444	238	0.01%	0.002%
6	2.716	424	428	432	rBV4	440	382	0.02%	0.003%
7	2.761	436	442	445	rBV2	363	469	0.02%	0.003%
8	2.774	445	446	448	rBV2	339	173	0.01%	0.001%
9	2.819	458	460	465	rVB3	217	184	0.01%	0.001%
10	2.851	465	470	471	rBV	296	233	0.01%	0.002%
11	2.909	485	488	491	rVB2	252	153	0.01%	0.001%
12	2.954	499	502	505	rBV2	379	283	0.01%	0.002%
13	3.038	521	528	531	rBV4	745	907	0.04%	0.006%
14	3.109	547	550	553	rBV	242	174	0.01%	0.001%
15	3.182	560	573	589	rVB2	3568	8229	0.41%	0.056%
16	3.263	594	598	602	rVV	297	248	0.01%	0.002%
17	3.285	602	605	607	rVV2	250	157	0.01%	0.001%
18	3.301	607	610	614	rVV	293	226	0.01%	0.002%
19	3.340	617	622	626	rBV	177	155	0.01%	0.001%
20	3.398	638	640	645	rVB2	348	273	0.01%	0.002%
21	3.433	645	651	653	rBV2	256	243	0.01%	0.002%
22	3.600	699	703	707	rBV2	241	278	0.01%	0.002%
23	3.723	737	741	745	rVV3	192	176	0.01%	0.001%
24	4.215	889	894	897	rBV2	199	159	0.01%	0.001%
25	4.536	991	994	998	rBV2	184	172	0.01%	0.001%
26	4.620	1005	1020	1047	rBV	209084	499414	24.73%	3.377%
27	4.819	1079	1082	1084	rBV2	350	240	0.01%	0.002%
28	5.063	1140	1158	1185	rBV	357011	778226	38.54%	5.263%
29	5.276	1220	1224	1225	rBV	537	345	0.02%	0.002%
30	5.507	1292	1296	1298	rBV	204	161	0.01%	0.001%
31	5.565	1309	1314	1316	rBV2	165	160	0.01%	0.001%
32	5.613	1325	1329	1335	rVB2	287	267	0.01%	0.002%
33	5.726	1341	1364	1403	rBV2	753465	2019508	100.00%	13.658%
34	5.970	1436	1440	1452	rVB6	875	1393	0.07%	0.009%
35	6.028	1454	1458	1460	rBV2	298	278	0.01%	0.002%
36	6.108	1479	1483	1484	rBV2	247	156	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048391.D
 Acq On : 03 May 2022 15:31
 Operator : SY/MD
 Sample : N2668-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.250	1509	1527	1549	rBV	493656	943058	46.70%	6.378%
38	6.404	1571	1575	1578	rVB3	383	322	0.02%	0.002%
39	6.420	1578	1580	1585	rVB3	275	204	0.01%	0.001%
40	6.449	1586	1589	1596	rVB2	267	248	0.01%	0.002%
41	6.530	1608	1614	1622	rVB6	1779	2480	0.12%	0.017%
42	6.591	1629	1633	1636	rBV3	670	409	0.02%	0.003%
43	6.690	1649	1664	1686	rBV	458438	890949	44.12%	6.025%
44	6.803	1694	1699	1701	rBV5	928	851	0.04%	0.006%
45	6.983	1753	1755	1759	rBV2	182	168	0.01%	0.001%
46	7.070	1778	1782	1789	rVB3	424	535	0.03%	0.004%
47	7.182	1804	1817	1827	rBV5	3587	7641	0.38%	0.052%
48	7.256	1838	1840	1847	rVB2	204	182	0.01%	0.001%
49	7.398	1881	1884	1889	rBV2	203	205	0.01%	0.001%
50	7.565	1922	1936	1956	rBV	247339	425603	21.07%	2.878%
51	7.694	1964	1976	1988	rVB6	2244	4805	0.24%	0.032%
52	7.761	1991	1997	2001	rBV3	463	500	0.02%	0.003%
53	7.787	2001	2005	2008	rVB3	461	280	0.01%	0.002%
54	7.899	2025	2040	2057	rBV	923448	1605075	79.48%	10.855%
55	8.115	2105	2107	2112	rVB3	258	195	0.01%	0.001%
56	8.179	2112	2127	2149	rBV	172301	286837	14.20%	1.940%
57	8.282	2157	2159	2161	rBV	569	247	0.01%	0.002%
58	8.353	2178	2181	2185	rBV2	764	676	0.03%	0.005%
59	8.411	2196	2199	2202	rBV2	316	198	0.01%	0.001%
60	8.475	2209	2219	2229	rVB3	5083	9053	0.45%	0.061%
61	8.632	2253	2268	2308	rBV	618013	1144077	56.65%	7.737%
62	8.951	2365	2367	2372	rVB3	513	302	0.01%	0.002%
63	8.980	2372	2376	2377	rBV2	310	198	0.01%	0.001%
64	9.089	2407	2410	2416	rVB3	315	340	0.02%	0.002%
65	9.124	2416	2421	2427	rBV3	344	380	0.02%	0.003%
66	9.250	2456	2460	2462	rBV2	212	187	0.01%	0.001%
67	9.320	2478	2482	2486	rBV2	322	300	0.01%	0.002%
68	9.417	2495	2512	2537	rBV	705295	1182851	58.57%	8.000%
69	9.652	2583	2585	2587	rVV	326	157	0.01%	0.001%
70	9.690	2591	2597	2607	rBV3	833	1163	0.06%	0.008%
71	9.758	2615	2618	2622	rVB2	226	149	0.01%	0.001%
72	9.848	2644	2646	2652	rVB2	270	158	0.01%	0.001%
73	9.909	2662	2665	2674	rVB	263	274	0.01%	0.002%
74	9.951	2674	2678	2679	rBV	217	151	0.01%	0.001%
75	10.182	2748	2750	2754	rVB2	286	150	0.01%	0.001%
76	10.269	2772	2777	2779	rBV2	257	192	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048391.D
 Acq On : 03 May 2022 15:31
 Operator : SY/MD
 Sample : N2668-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.591	2874	2877	2881	rBV2	281	262	0.01%	0.002%
78	10.671	2895	2902	2913	rVB5	2875	4540	0.22%	0.031%
79	10.758	2916	2929	2951	rVV	698250	1123773	55.65%	7.600%
80	10.848	2955	2957	2958	rVV	347	167	0.01%	0.001%
81	10.896	2959	2972	2985	rVB2	10225	18468	0.91%	0.125%
82	11.111	3035	3039	3040	rBV2	608	413	0.02%	0.003%
83	11.333	3102	3108	3112	rBV2	375	420	0.02%	0.003%
84	11.410	3124	3132	3135	rBV4	723	794	0.04%	0.005%
85	11.455	3141	3146	3158	rVB6	2177	3547	0.18%	0.024%
86	11.571	3178	3182	3184	rBV2	448	329	0.02%	0.002%
87	11.626	3196	3199	3204	rVB	307	217	0.01%	0.001%
88	11.693	3213	3220	3226	rBV4	1443	1772	0.09%	0.012%
89	11.742	3233	3235	3239	rVB3	570	382	0.02%	0.003%
90	11.764	3239	3242	3244	rBV	316	198	0.01%	0.001%
91	11.812	3244	3257	3276	rBV	679158	1088078	53.88%	7.359%
92	12.063	3330	3335	3336	rBV3	1885	1380	0.07%	0.009%
93	12.195	3359	3376	3394	rBV	843330	1376274	68.15%	9.308%
94	12.336	3415	3420	3422	rBV5	546	516	0.03%	0.003%
95	12.407	3440	3442	3446	rVB3	351	173	0.01%	0.001%
96	12.500	3469	3471	3475	rVB	322	173	0.01%	0.001%
97	12.584	3494	3497	3501	rBV2	426	413	0.02%	0.003%
98	12.774	3549	3556	3564	rVB2	3910	5729	0.28%	0.039%
99	12.973	3615	3618	3619	rBV	322	201	0.01%	0.001%
100	13.282	3711	3714	3716	rBV	304	228	0.01%	0.002%




Sum of corrected areas: 14786502

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048391.D
Acq On : 03 May 2022 15:31
Operator : SY/MD
Sample : N2668-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

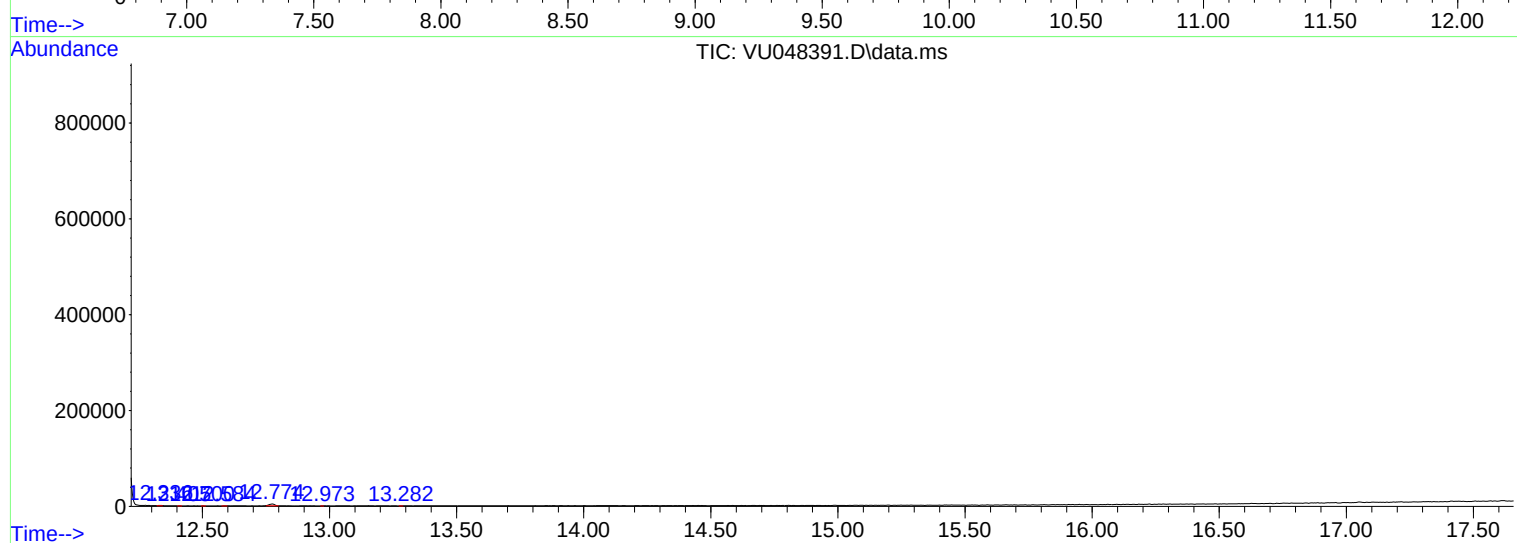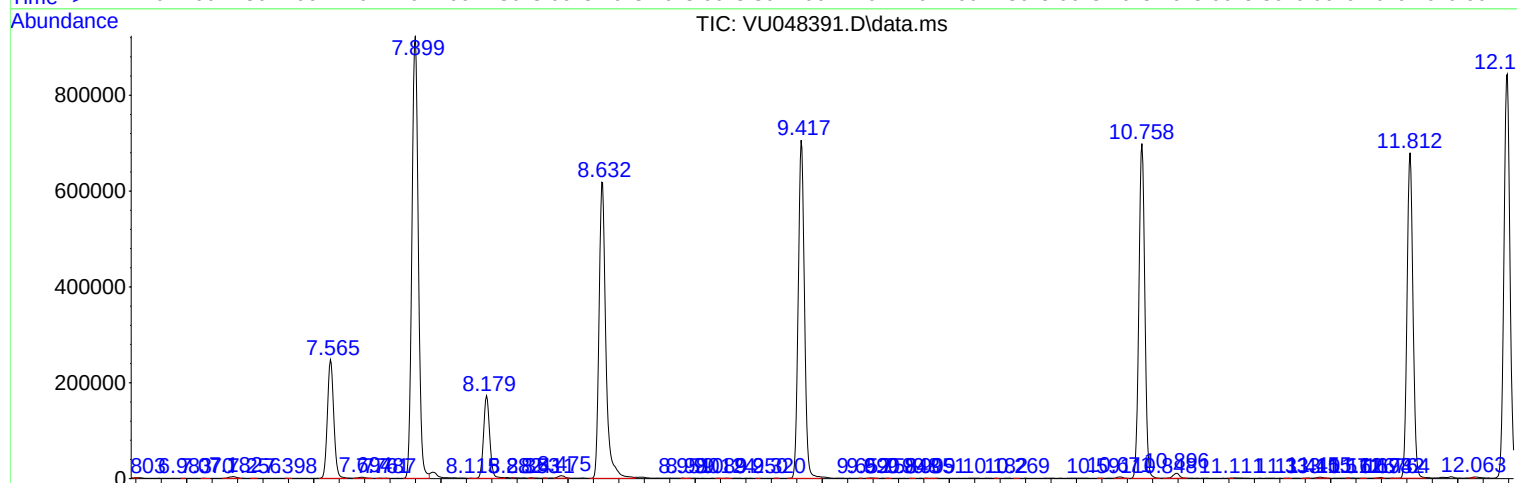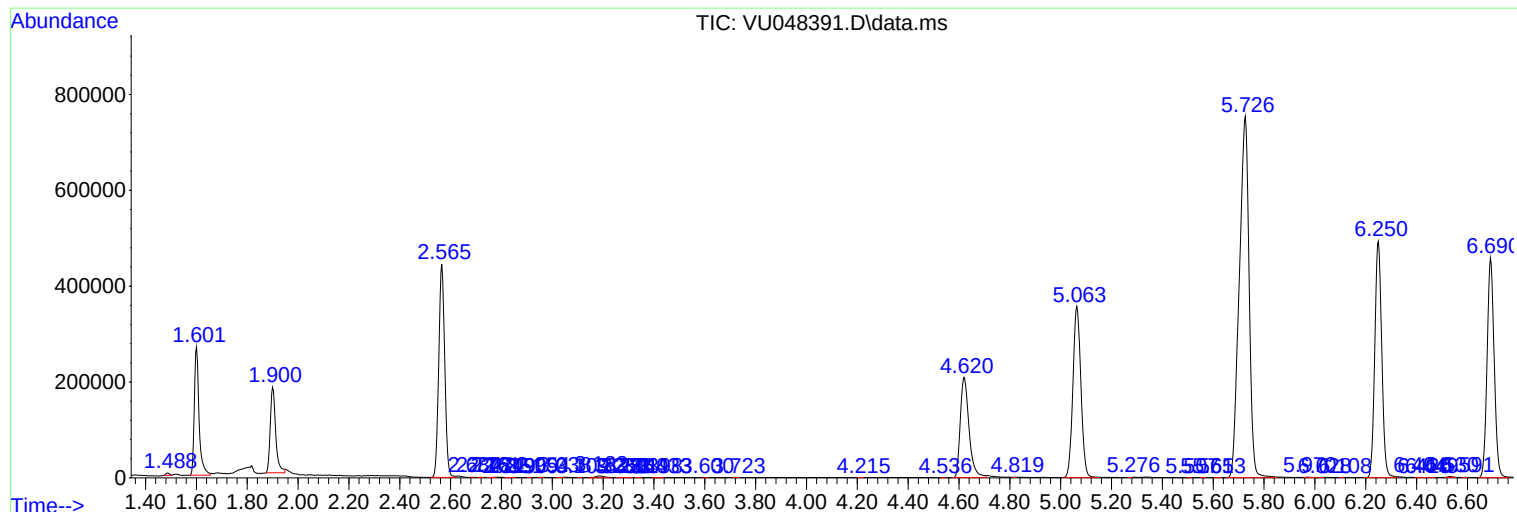

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048391.D
Acq On : 03 May 2022 15:31
Operator : SY/MD
Sample : N2668-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048391.D
Acq On : 03 May 2022 15:31
Operator : SY/MD
Sample : N2668-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------