

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048392.D
 Acq On : 03 May 2022 15:54
 Operator : SY/MD
 Sample : N2668-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	51	rBV2	6939	7644	0.38%	0.051%
2	1.601	73	81	102	rBV	269579	347418	17.22%	2.304%
3	1.900	165	174	185	rBV	175572	257564	12.77%	1.708%
4	2.565	367	381	396	rBV	435224	717716	35.57%	4.761%
5	2.716	425	428	430	rBV2	438	324	0.02%	0.002%
6	2.771	431	445	462	rVB3	4445	11505	0.57%	0.076%
7	2.954	499	502	507	rVB2	389	291	0.01%	0.002%
8	3.041	525	529	530	rBV2	663	514	0.03%	0.003%
9	3.112	548	551	554	rVB	356	277	0.01%	0.002%
10	3.186	559	574	599	rVB	16212	39516	1.96%	0.262%
11	3.363	623	629	633	rBV2	322	231	0.01%	0.002%
12	3.388	633	637	641	rVB2	262	237	0.01%	0.002%
13	3.417	641	646	649	rBV2	318	302	0.01%	0.002%
14	3.456	654	658	661	rBV2	266	207	0.01%	0.001%
15	3.575	686	695	699	rBV3	211	255	0.01%	0.002%
16	3.594	699	701	705	rVB2	314	219	0.01%	0.001%
17	3.684	726	729	732	rVB	406	262	0.01%	0.002%
18	3.713	732	738	744	rVB2	331	377	0.02%	0.003%
19	4.060	840	846	848	rBV2	235	223	0.01%	0.001%
20	4.289	912	917	920	rVB2	265	230	0.01%	0.002%
21	4.311	920	924	926	rBV2	234	204	0.01%	0.001%
22	4.401	945	952	957	rVB2	206	288	0.01%	0.002%
23	4.620	1007	1020	1055	rBV	211762	515368	25.54%	3.418%
24	4.880	1098	1101	1104	rVB3	343	281	0.01%	0.002%
25	4.954	1119	1124	1126	rBV2	334	279	0.01%	0.002%
26	5.063	1141	1158	1184	rBV	361186	824814	40.88%	5.471%
27	5.211	1199	1204	1208	rBV4	454	391	0.02%	0.003%
28	5.253	1213	1217	1221	rBV2	292	209	0.01%	0.001%
29	5.272	1221	1223	1225	rBV2	394	221	0.01%	0.001%
30	5.337	1239	1243	1252	rVB2	1220	1695	0.08%	0.011%
31	5.530	1298	1303	1306	rBV2	339	245	0.01%	0.002%
32	5.726	1340	1364	1397	rBV2	747542	2017547	100.00%	13.382%
33	5.967	1435	1439	1441	rBV2	614	546	0.03%	0.004%
34	6.047	1459	1464	1471	rVB3	767	1010	0.05%	0.007%
35	6.096	1476	1479	1481	rBV2	320	222	0.01%	0.001%
36	6.160	1495	1499	1501	rBV2	315	260	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048392.D
 Acq On : 03 May 2022 15:54
 Operator : SY/MD
 Sample : N2668-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.247	1511	1526	1552	rBV	505526	954469	47.31%	6.331%
38	6.391	1565	1571	1573	rBV3	274	293	0.01%	0.002%
39	6.469	1590	1595	1599	rBV	350	386	0.02%	0.003%
40	6.539	1605	1617	1627	rVB7	4141	8854	0.44%	0.059%
41	6.591	1627	1633	1636	rBV3	573	596	0.03%	0.004%
42	6.690	1649	1664	1690	rBV	466552	897359	44.48%	5.952%
43	6.803	1696	1699	1700	rBV2	815	472	0.02%	0.003%
44	7.041	1770	1773	1779	rBV3	591	658	0.03%	0.004%
45	7.105	1784	1793	1806	rVB2	3059	5150	0.26%	0.034%
46	7.182	1806	1817	1826	rBV5	3887	8656	0.43%	0.057%
47	7.295	1845	1852	1855	rBV3	298	288	0.01%	0.002%
48	7.333	1860	1864	1868	rVB2	288	230	0.01%	0.002%
49	7.565	1922	1936	1955	rBV	241704	423834	21.01%	2.811%
50	7.694	1968	1976	1984	rVV5	1591	2897	0.14%	0.019%
51	7.764	1995	1998	2002	rVB2	399	262	0.01%	0.002%
52	7.784	2002	2004	2006	rBV	326	207	0.01%	0.001%
53	7.819	2011	2015	2019	rVB2	290	282	0.01%	0.002%
54	7.899	2025	2040	2057	rBV	913962	1599748	79.29%	10.611%
55	8.179	2114	2127	2145	rBV	170408	285100	14.13%	1.891%
56	8.475	2209	2219	2222	rBV4	1737	2503	0.12%	0.017%
57	8.552	2229	2243	2256	rBV	75556	129366	6.41%	0.858%
58	8.632	2256	2268	2302	rBV	631610	1158524	57.42%	7.684%
59	8.906	2351	2353	2359	rVV3	314	260	0.01%	0.002%
60	9.050	2396	2398	2401	rVV2	367	233	0.01%	0.002%
61	9.105	2412	2415	2418	rBV2	398	244	0.01%	0.002%
62	9.166	2429	2434	2439	rBV3	594	548	0.03%	0.004%
63	9.231	2450	2454	2458	rVB2	264	247	0.01%	0.002%
64	9.317	2478	2481	2487	rVB3	312	238	0.01%	0.002%
65	9.417	2499	2512	2547	rBV	721021	1201380	59.55%	7.969%
66	9.558	2552	2556	2559	rBV2	324	223	0.01%	0.001%
67	9.604	2568	2570	2574	rVB3	304	204	0.01%	0.001%
68	9.629	2574	2578	2579	rBV3	484	316	0.02%	0.002%
69	9.642	2580	2582	2588	rVV3	755	630	0.03%	0.004%
70	9.694	2591	2598	2606	rVV2	1026	1512	0.07%	0.010%
71	9.774	2618	2623	2625	rBV2	294	242	0.01%	0.002%
72	9.845	2643	2645	2652	rVB3	361	366	0.02%	0.002%
73	9.880	2652	2656	2661	rBV2	469	410	0.02%	0.003%
74	9.951	2674	2678	2686	rVB2	412	466	0.02%	0.003%
75	10.423	2822	2825	2830	rVB2	301	219	0.01%	0.001%
76	10.536	2856	2860	2863	rBV	263	222	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048392.D
 Acq On : 03 May 2022 15:54
 Operator : SY/MD
 Sample : N2668-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL67

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.587	2871	2876	2882	rVB3	326	375	0.02%	0.002%
78	10.671	2893	2902	2911	rVB4	2874	3904	0.19%	0.026%
79	10.758	2915	2929	2947	rBV	697864	1142442	56.63%	7.578%
80	10.893	2960	2971	2984	rVB3	4233	7305	0.36%	0.048%
81	11.118	3035	3041	3046	rVB5	750	972	0.05%	0.006%
82	11.459	3140	3147	3159	rVB4	1824	3116	0.15%	0.021%
83	11.517	3159	3165	3168	rBV2	367	421	0.02%	0.003%
84	11.581	3180	3185	3191	rVB2	436	501	0.02%	0.003%
85	11.693	3216	3220	3226	rBV4	1049	949	0.05%	0.006%
86	11.751	3235	3238	3242	rVB2	550	348	0.02%	0.002%
87	11.812	3244	3257	3277	rBV	693611	1104295	54.73%	7.325%
88	11.973	3302	3307	3314	rVB5	1843	2456	0.12%	0.016%
89	12.073	3335	3338	3340	rBV3	389	244	0.01%	0.002%
90	12.115	3347	3351	3354	rBV2	555	423	0.02%	0.003%
91	12.195	3361	3376	3399	rBV	833988	1365853	67.70%	9.060%
92	12.330	3414	3418	3424	rVB3	958	939	0.05%	0.006%
93	12.391	3434	3437	3442	rVB4	516	309	0.02%	0.002%
94	12.488	3464	3467	3469	rBV	295	216	0.01%	0.001%
95	12.603	3500	3503	3507	rBV2	348	267	0.01%	0.002%
96	12.636	3507	3513	3517	rBV2	614	587	0.03%	0.004%
97	12.706	3530	3535	3539	rBV3	377	485	0.02%	0.003%
98	12.771	3548	3555	3567	rBV4	1424	2039	0.10%	0.014%
99	15.070	4267	4270	4273	rBV2	769	514	0.03%	0.003%
100	15.163	4297	4299	4305	rBV2	598	431	0.02%	0.003%




Sum of corrected areas: 15076377

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048392.D
Acq On : 03 May 2022 15:54
Operator : SY/MD
Sample : N2668-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

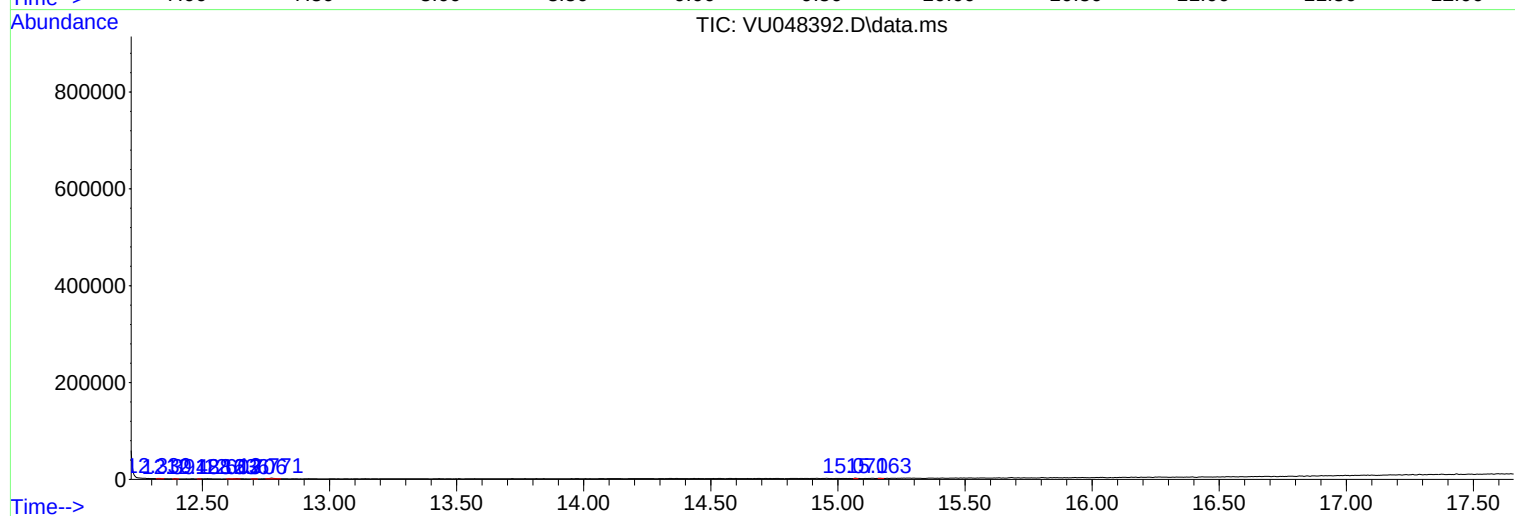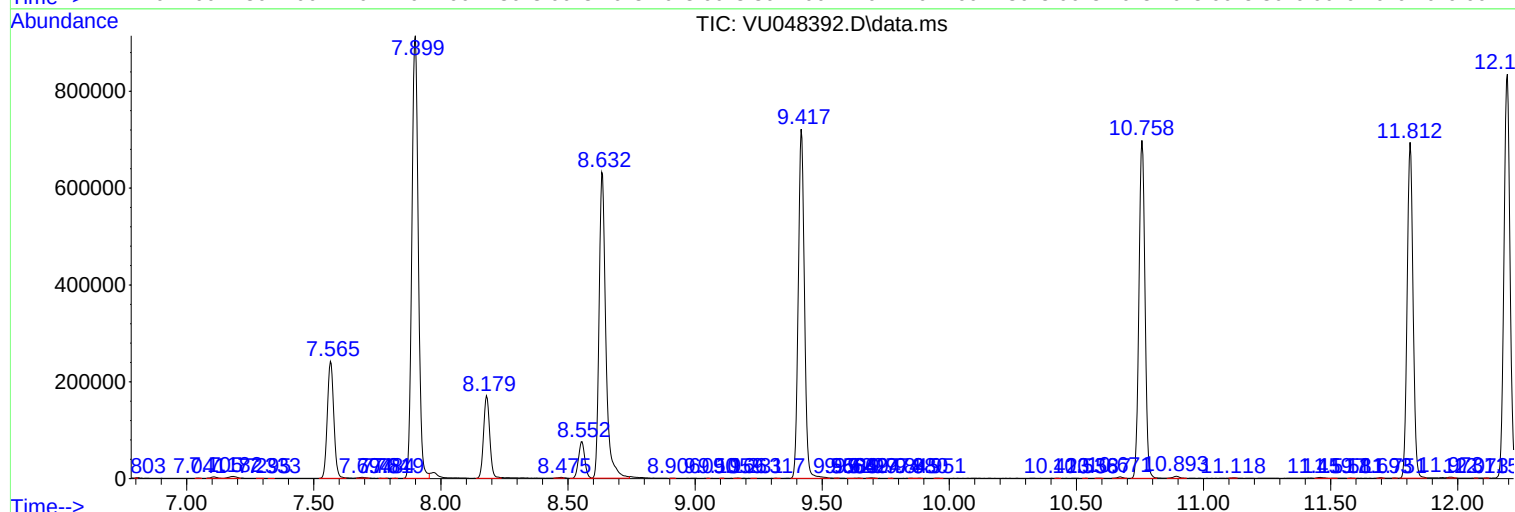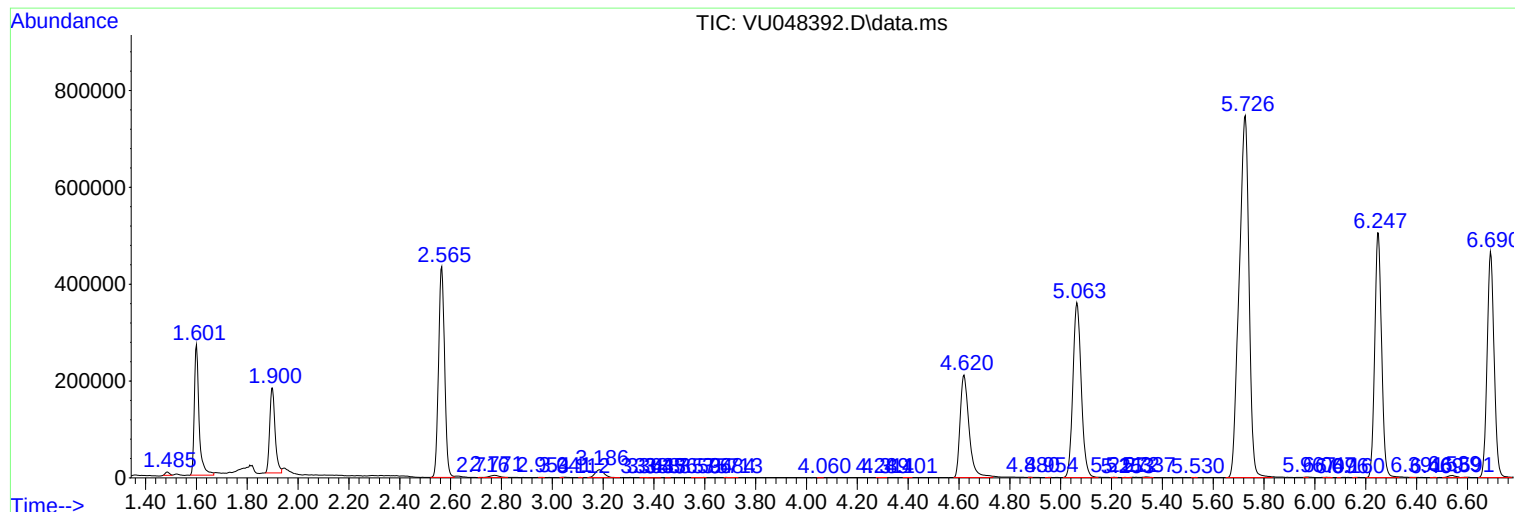

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048392.D
Acq On : 03 May 2022 15:54
Operator : SY/MD
Sample : N2668-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048392.D
Acq On : 03 May 2022 15:54
Operator : SY/MD
Sample : N2668-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL67

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------