

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048393.D
 Acq On : 03 May 2022 16:18
 Operator : SY/MD
 Sample : N2668-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048393.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	52	rBV3	5318	6120	0.31%	0.043%
2	1.601	73	81	102	rBV	265982	338592	16.90%	2.385%
3	1.900	166	174	186	rBV	176965	251692	12.56%	1.773%
4	2.565	368	381	396	rBV	434129	710653	35.47%	5.006%
5	2.671	412	414	416	rBV2	390	217	0.01%	0.002%
6	2.752	435	439	441	rBV2	565	445	0.02%	0.003%
7	2.938	492	497	499	rBV2	557	538	0.03%	0.004%
8	3.044	522	530	537	rVV5	1411	2196	0.11%	0.015%
9	3.076	537	540	544	rVV3	461	429	0.02%	0.003%
10	3.182	558	573	592	rVB2	8004	19486	0.97%	0.137%
11	3.292	605	607	612	rVV2	304	243	0.01%	0.002%
12	3.353	621	626	627	rBV	326	232	0.01%	0.002%
13	3.620	706	709	715	rVB	266	222	0.01%	0.002%
14	3.668	721	724	728	rBV2	214	224	0.01%	0.002%
15	3.861	779	784	789	rBV3	293	370	0.02%	0.003%
16	4.362	935	940	943	rBV2	237	206	0.01%	0.001%
17	4.440	961	964	970	rBV2	196	235	0.01%	0.002%
18	4.494	978	981	985	rBV2	286	202	0.01%	0.001%
19	4.620	1007	1020	1049	rBV	213579	511246	25.52%	3.601%
20	4.928	1113	1116	1119	rVB2	333	205	0.01%	0.001%
21	5.063	1141	1158	1191	rBV	370989	819261	40.89%	5.771%
22	5.256	1214	1218	1221	rVB4	321	250	0.01%	0.002%
23	5.282	1221	1226	1227	rBV3	761	517	0.03%	0.004%
24	5.321	1235	1238	1239	rBV	575	306	0.02%	0.002%
25	5.510	1290	1297	1299	rBV3	500	430	0.02%	0.003%
26	5.726	1340	1364	1409	rBV2	748556	2003664	100.00%	14.113%
27	5.960	1433	1437	1438	rBV3	459	278	0.01%	0.002%
28	6.022	1453	1456	1458	rBV3	324	251	0.01%	0.002%
29	6.073	1469	1472	1477	rBV2	251	230	0.01%	0.002%
30	6.121	1482	1487	1490	rBV2	399	359	0.02%	0.003%
31	6.182	1500	1506	1509	rBV3	282	284	0.01%	0.002%
32	6.250	1511	1527	1544	rBV	420403	790471	39.45%	5.568%
33	6.536	1607	1616	1626	rVV7	2427	4712	0.24%	0.033%
34	6.616	1638	1641	1645	rVB2	432	329	0.02%	0.002%
35	6.690	1648	1664	1685	rBV	451065	883693	44.10%	6.225%
36	6.800	1695	1698	1699	rBV3	736	411	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048393.D
 Acq On : 03 May 2022 16:18
 Operator : SY/MD
 Sample : N2668-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.845	1711	1712	1718	rVB2	302	293	0.01%	0.002%
38	6.896	1724	1728	1735	rBV2	308	331	0.02%	0.002%
39	6.951	1741	1745	1747	rBV2	306	196	0.01%	0.001%
40	7.047	1772	1775	1779	rBV2	411	317	0.02%	0.002%
41	7.102	1790	1792	1794	rVV	414	228	0.01%	0.002%
42	7.128	1796	1800	1801	rBV2	262	180	0.01%	0.001%
43	7.182	1804	1817	1832	rVV4	3726	7593	0.38%	0.053%
44	7.382	1874	1879	1883	rBV2	297	236	0.01%	0.002%
45	7.417	1884	1890	1893	rBV2	373	315	0.02%	0.002%
46	7.478	1904	1909	1912	rBV	196	186	0.01%	0.001%
47	7.565	1922	1936	1954	rBV	237283	414968	20.71%	2.923%
48	7.687	1966	1974	1978	rBV4	1833	2492	0.12%	0.018%
49	7.793	2004	2007	2013	rVB2	677	690	0.03%	0.005%
50	7.825	2014	2017	2021	rBV3	295	230	0.01%	0.002%
51	7.899	2026	2040	2056	rBV	918439	1582124	78.96%	11.144%
52	8.179	2114	2127	2149	rBV	168282	282886	14.12%	1.993%
53	8.468	2212	2217	2218	rBV4	787	659	0.03%	0.005%
54	8.552	2238	2243	2250	rVB5	731	697	0.03%	0.005%
55	8.632	2256	2268	2302	rBV	610671	1141928	56.99%	8.043%
56	8.951	2365	2367	2373	rBV2	354	317	0.02%	0.002%
57	9.095	2410	2412	2416	rBV2	297	192	0.01%	0.001%
58	9.156	2427	2431	2433	rBV2	642	496	0.02%	0.003%
59	9.240	2454	2457	2461	rBV2	224	211	0.01%	0.001%
60	9.417	2499	2512	2535	rBV	597373	1000805	49.95%	7.049%
61	9.571	2555	2560	2566	rBV2	1036	1257	0.06%	0.009%
62	9.619	2571	2575	2577	rBV2	262	185	0.01%	0.001%
63	9.648	2580	2584	2589	rVB3	501	582	0.03%	0.004%
64	9.697	2590	2599	2606	rBV4	1352	2199	0.11%	0.015%
65	9.780	2622	2625	2630	rBV2	281	205	0.01%	0.001%
66	9.838	2638	2643	2647	rBV2	195	237	0.01%	0.002%
67	9.890	2655	2659	2662	rBV2	352	260	0.01%	0.002%
68	9.918	2665	2668	2673	rBV2	270	220	0.01%	0.002%
69	10.108	2717	2727	2739	rBV7	1103	2393	0.12%	0.017%
70	10.237	2763	2767	2769	rBV2	238	190	0.01%	0.001%
71	10.291	2781	2784	2787	rBV	280	194	0.01%	0.001%
72	10.565	2865	2869	2875	rBV2	329	390	0.02%	0.003%
73	10.671	2895	2902	2913	rVB4	3241	4379	0.22%	0.031%
74	10.758	2916	2929	2950	rVV	694384	1123244	56.06%	7.912%
75	10.861	2958	2961	2963	rBV2	532	386	0.02%	0.003%
76	10.893	2967	2971	2978	rVB5	1361	1858	0.09%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048393.D
 Acq On : 03 May 2022 16:18
 Operator : SY/MD
 Sample : N2668-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL80

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.095	3024	3034	3038	rBV2	804	1249	0.06%	0.009%
78	11.156	3050	3053	3056	rBV2	403	245	0.01%	0.002%
79	11.314	3100	3102	3107	rVB2	294	183	0.01%	0.001%
80	11.410	3129	3132	3136	rVB2	444	286	0.01%	0.002%
81	11.462	3139	3148	3158	rBV6	2399	4244	0.21%	0.030%
82	11.568	3178	3181	3182	rBV	384	203	0.01%	0.001%
83	11.639	3200	3203	3205	rBV	313	200	0.01%	0.001%
84	11.655	3206	3208	3213	rVB2	394	240	0.01%	0.002%
85	11.700	3215	3222	3228	rVB4	1305	1761	0.09%	0.012%
86	11.732	3228	3232	3233	rBV	283	189	0.01%	0.001%
87	11.748	3233	3237	3244	rBV2	605	528	0.03%	0.004%
88	11.812	3244	3257	3277	rBV	570645	911745	45.50%	6.422%
89	12.076	3336	3339	3342	rBV3	290	192	0.01%	0.001%
90	12.131	3352	3356	3359	rBV2	337	251	0.01%	0.002%
91	12.195	3360	3376	3396	rBV	814095	1337162	66.74%	9.419%
92	12.404	3437	3441	3445	rVB4	750	614	0.03%	0.004%
93	12.700	3530	3533	3538	rBV	533	425	0.02%	0.003%
94	12.725	3539	3541	3543	rVV3	434	209	0.01%	0.001%
95	12.770	3543	3555	3567	rVB3	5482	8699	0.43%	0.061%
96	12.877	3586	3588	3592	rVB	306	193	0.01%	0.001%
97	13.227	3693	3697	3704	rVB4	520	566	0.03%	0.004%
98	13.860	3888	3894	3898	rBV4	560	700	0.03%	0.005%
99	14.706	4155	4157	4160	rBV2	428	257	0.01%	0.002%
100	15.616	4437	4440	4442	rBV2	933	642	0.03%	0.005%




Sum of corrected areas: 14196931

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048393.D
Acq On : 03 May 2022 16:18
Operator : SY/MD
Sample : N2668-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

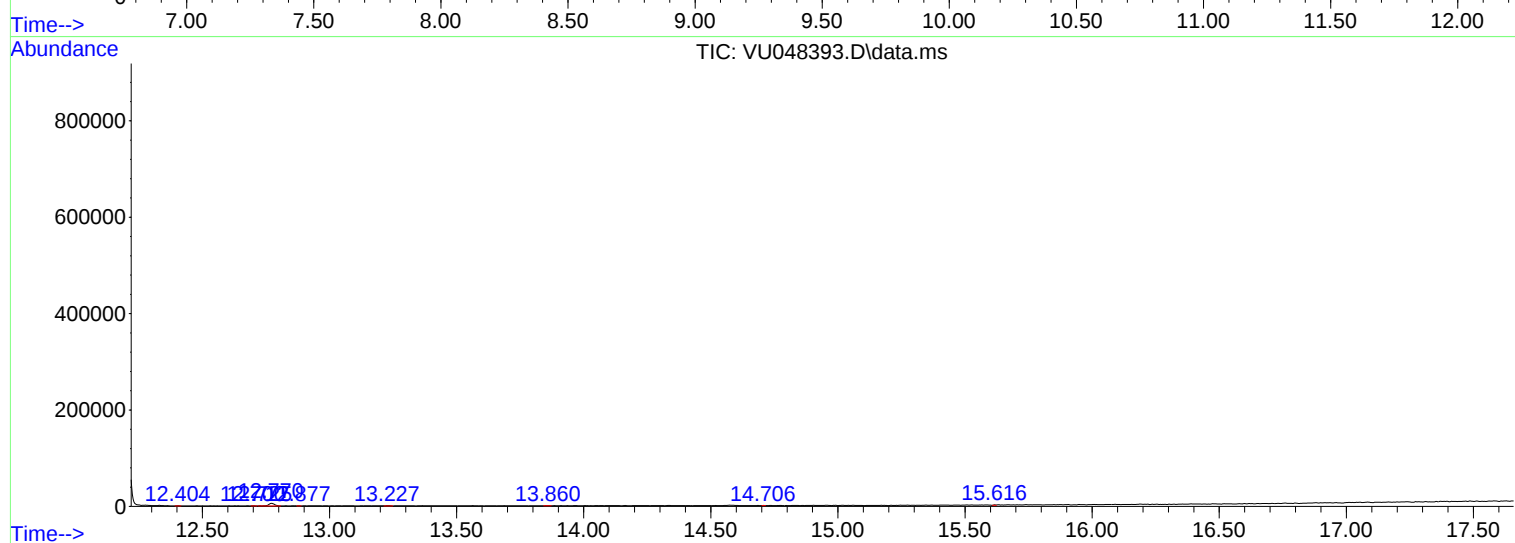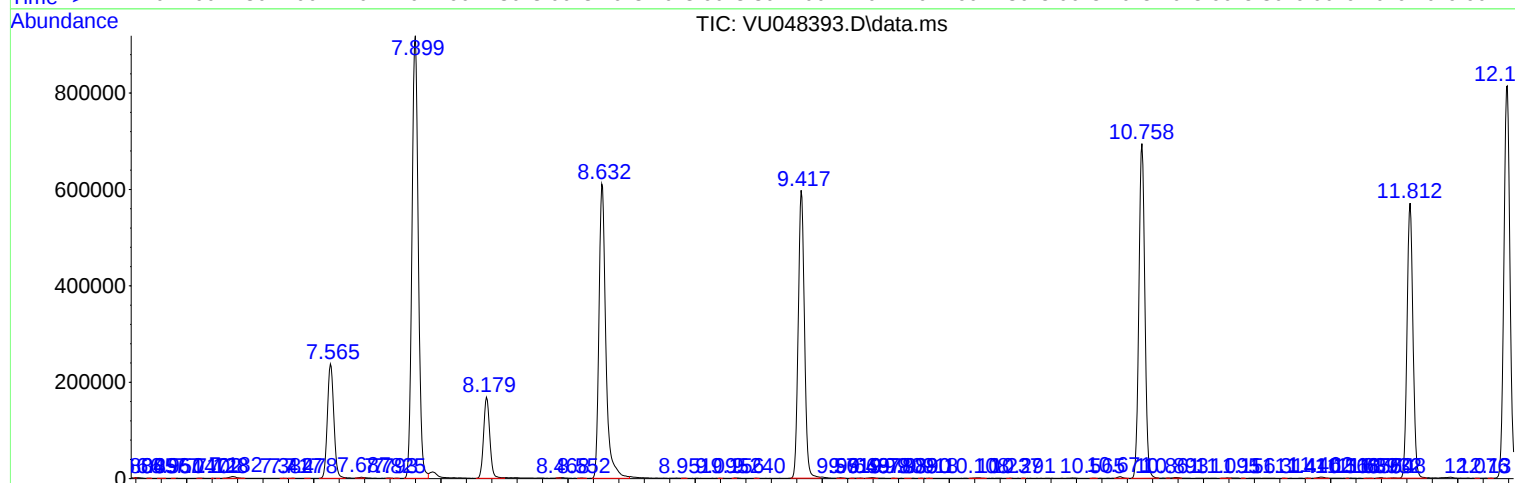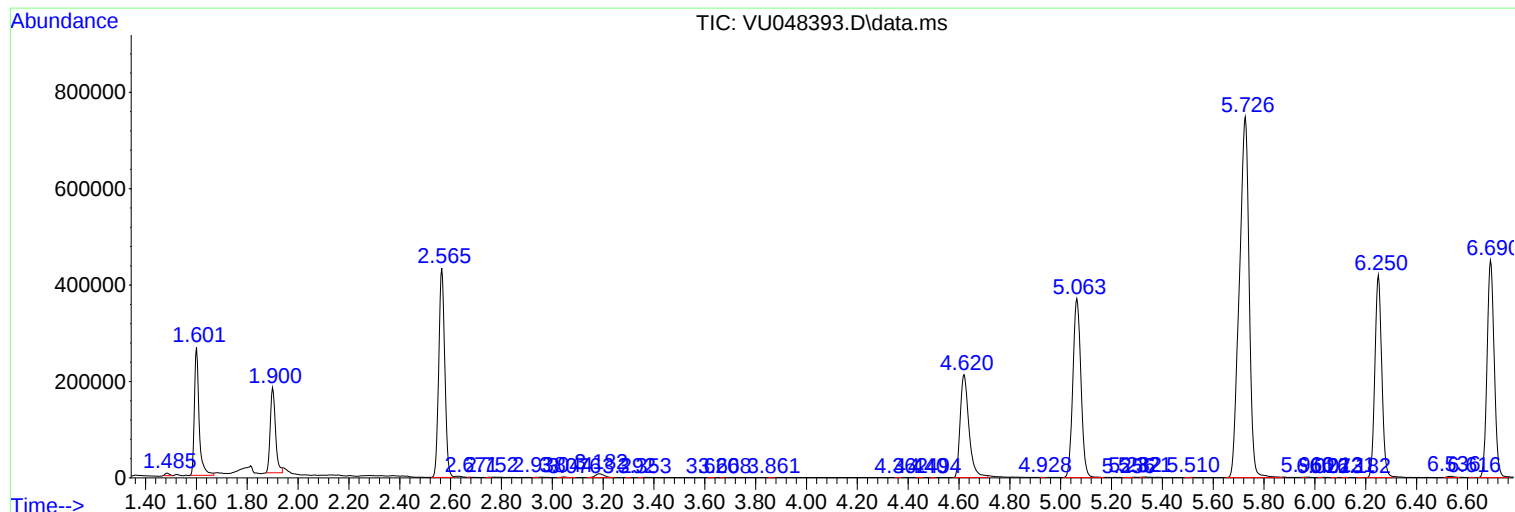

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048393.D
Acq On : 03 May 2022 16:18
Operator : SY/MD
Sample : N2668-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048393.D
Acq On : 03 May 2022 16:18
Operator : SY/MD
Sample : N2668-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL80

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------