

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048394.D
 Acq On : 03 May 2022 16:42
 Operator : SY/MD
 Sample : N2668-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	52	rBV4	6477	8160	0.46%	0.063%
2	1.601	73	81	99	rBV	234357	303934	17.02%	2.341%
3	1.893	164	172	186	rBV	152066	220621	12.35%	1.699%
4	2.562	368	380	398	rBV	382459	628625	35.20%	4.842%
5	2.755	437	440	441	rBV2	371	180	0.01%	0.001%
6	2.790	449	451	462	rVB4	1120	1061	0.06%	0.008%
7	2.855	469	471	477	rVV2	282	249	0.01%	0.002%
8	2.906	484	487	494	rBV2	293	300	0.02%	0.002%
9	2.964	499	505	510	rVB2	642	720	0.04%	0.006%
10	3.035	521	527	528	rBV3	666	472	0.03%	0.004%
11	3.186	560	574	595	rBV2	8401	19863	1.11%	0.153%
12	3.269	595	600	602	rBV	282	192	0.01%	0.001%
13	3.285	602	605	608	rBV2	254	192	0.01%	0.001%
14	3.401	637	641	644	rVB3	321	240	0.01%	0.002%
15	3.578	693	696	701	rBV2	226	203	0.01%	0.002%
16	3.803	763	766	774	rVB2	180	206	0.01%	0.002%
17	4.195	885	888	895	rVB2	163	202	0.01%	0.002%
18	4.292	914	918	924	rVB2	236	247	0.01%	0.002%
19	4.620	1006	1020	1044	rBV	186758	446808	25.02%	3.442%
20	5.002	1135	1139	1141	rBV3	251	172	0.01%	0.001%
21	5.063	1141	1158	1183	rBV	331456	730497	40.91%	5.627%
22	5.199	1198	1200	1204	rVB2	417	295	0.02%	0.002%
23	5.224	1204	1208	1209	rBV2	317	218	0.01%	0.002%
24	5.244	1209	1214	1222	rVB3	516	666	0.04%	0.005%
25	5.289	1222	1228	1230	rBV	826	868	0.05%	0.007%
26	5.340	1235	1244	1255	rVB3	1366	3097	0.17%	0.024%
27	5.385	1255	1258	1263	rVB2	351	275	0.02%	0.002%
28	5.726	1339	1364	1402	rBV2	667639	1785695	100.00%	13.755%
29	5.925	1424	1426	1430	rVB3	401	229	0.01%	0.002%
30	5.961	1434	1437	1439	rBV3	573	403	0.02%	0.003%
31	6.080	1471	1474	1477	rVB2	351	235	0.01%	0.002%
32	6.118	1482	1486	1490	rBV	371	389	0.02%	0.003%
33	6.141	1490	1493	1498	rVB2	248	242	0.01%	0.002%
34	6.250	1512	1527	1552	rBV	410941	786325	44.03%	6.057%
35	6.523	1602	1612	1613	rBV3	1866	1834	0.10%	0.014%
36	6.588	1630	1632	1637	rBV3	336	358	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048394.D
 Acq On : 03 May 2022 16:42
 Operator : SY/MD
 Sample : N2668-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1684	rBV	404354	788233	44.14%	6.071%
38	6.813	1694	1702	1709	rVB6	1507	2287	0.13%	0.018%
39	6.928	1735	1738	1742	rVB	336	259	0.01%	0.002%
40	7.009	1761	1763	1766	rVV2	303	197	0.01%	0.002%
41	7.054	1774	1777	1779	rVV	305	217	0.01%	0.002%
42	7.176	1804	1815	1830	rVB6	3997	7867	0.44%	0.061%
43	7.266	1838	1843	1846	rBV	347	258	0.01%	0.002%
44	7.308	1854	1856	1862	rVB	278	168	0.01%	0.001%
45	7.366	1870	1874	1878	rBV3	232	191	0.01%	0.001%
46	7.388	1878	1881	1883	rBV2	298	214	0.01%	0.002%
47	7.465	1900	1905	1912	rBV2	422	429	0.02%	0.003%
48	7.565	1923	1936	1959	rBV	212313	371459	20.80%	2.861%
49	7.694	1967	1976	1981	rBV6	1438	2530	0.14%	0.019%
50	7.771	1997	2000	2002	rBV2	348	178	0.01%	0.001%
51	7.800	2004	2009	2010	rBV3	280	197	0.01%	0.002%
52	7.835	2016	2020	2022	rBV2	356	258	0.01%	0.002%
53	7.899	2026	2040	2056	rBV	804156	1394819	78.11%	10.744%
54	8.118	2106	2108	2111	rVB3	447	193	0.01%	0.001%
55	8.179	2115	2127	2142	rBV	151054	250047	14.00%	1.926%
56	8.507	2227	2229	2237	rVB3	419	351	0.02%	0.003%
57	8.552	2238	2243	2244	rBV3	550	378	0.02%	0.003%
58	8.636	2256	2269	2310	rBV	554617	1030715	57.72%	7.939%
59	8.899	2349	2351	2359	rVB3	438	445	0.02%	0.003%
60	8.973	2371	2374	2376	rBV2	459	252	0.01%	0.002%
61	9.031	2388	2392	2395	rBV3	301	215	0.01%	0.002%
62	9.160	2429	2432	2433	rBV	301	176	0.01%	0.001%
63	9.417	2499	2512	2536	rBV	597494	1000927	56.05%	7.710%
64	9.565	2554	2558	2565	rVB2	654	670	0.04%	0.005%
65	9.613	2565	2573	2578	rBV2	318	460	0.03%	0.004%
66	9.697	2595	2599	2607	rVB4	1145	1339	0.07%	0.010%
67	9.925	2667	2670	2675	rVB3	287	264	0.01%	0.002%
68	9.989	2687	2690	2696	rVB	214	178	0.01%	0.001%
69	10.105	2720	2726	2729	rBV2	337	346	0.02%	0.003%
70	10.250	2768	2771	2775	rVB2	301	195	0.01%	0.002%
71	10.282	2775	2781	2783	rBV2	272	345	0.02%	0.003%
72	10.321	2789	2793	2796	rBV2	250	228	0.01%	0.002%
73	10.404	2813	2819	2820	rBV	234	216	0.01%	0.002%
74	10.449	2830	2833	2838	rBV2	214	221	0.01%	0.002%
75	10.552	2862	2865	2867	rBV	314	185	0.01%	0.001%
76	10.671	2895	2902	2911	rBV4	2704	3240	0.18%	0.025%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
 Data File : VU048394.D
 Acq On : 03 May 2022 16:42
 Operator : SY/MD
 Sample : N2668-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXL79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.758	2915	2929	2952	rBV	632695	1025261	57.42%	7.897%
78	10.864	2959	2962	2964	rBV	451	279	0.02%	0.002%
79	10.890	2965	2970	2979	rVB5	1148	1877	0.11%	0.014%
80	10.993	2999	3002	3004	rBV	376	261	0.01%	0.002%
81	11.086	3027	3031	3032	rBV2	251	176	0.01%	0.001%
82	11.099	3033	3035	3037	rVV2	461	277	0.02%	0.002%
83	11.121	3037	3042	3049	rVV6	807	1096	0.06%	0.008%
84	11.150	3049	3051	3054	rVB2	312	168	0.01%	0.001%
85	11.237	3075	3078	3083	rVB2	325	219	0.01%	0.002%
86	11.285	3091	3093	3098	rVB2	298	168	0.01%	0.001%
87	11.456	3140	3146	3147	rBV2	1294	1123	0.06%	0.009%
88	11.574	3181	3183	3189	rVB2	536	366	0.02%	0.003%
89	11.703	3215	3223	3228	rBV5	1114	1391	0.08%	0.011%
90	11.812	3244	3257	3274	rBV	576539	916652	51.33%	7.061%
91	12.025	3320	3323	3324	rBV	362	187	0.01%	0.001%
92	12.195	3361	3376	3397	rBV	749565	1218145	68.22%	9.383%
93	12.539	3480	3483	3486	rBV	302	266	0.01%	0.002%
94	12.584	3495	3497	3503	rBV2	251	286	0.02%	0.002%
95	12.771	3548	3555	3565	rVB2	4903	7000	0.39%	0.054%
96	12.851	3577	3580	3581	rBV	421	272	0.02%	0.002%
97	12.902	3593	3596	3601	rVB	334	246	0.01%	0.002%
98	13.102	3655	3658	3663	rBV2	320	324	0.02%	0.002%
99	13.150	3669	3673	3679	rBV4	468	526	0.03%	0.004%
100	14.266	4017	4020	4023	rBV2	465	339	0.02%	0.003%




Sum of corrected areas: 12982525

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048394.D
Acq On : 03 May 2022 16:42
Operator : SY/MD
Sample : N2668-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

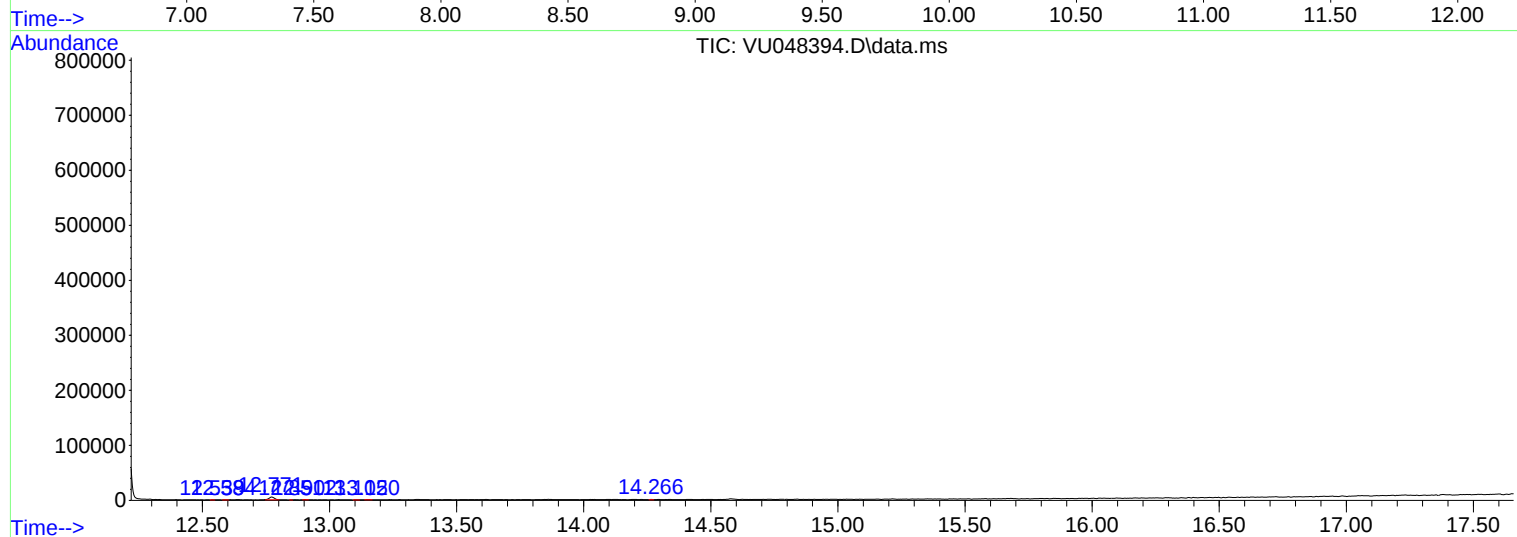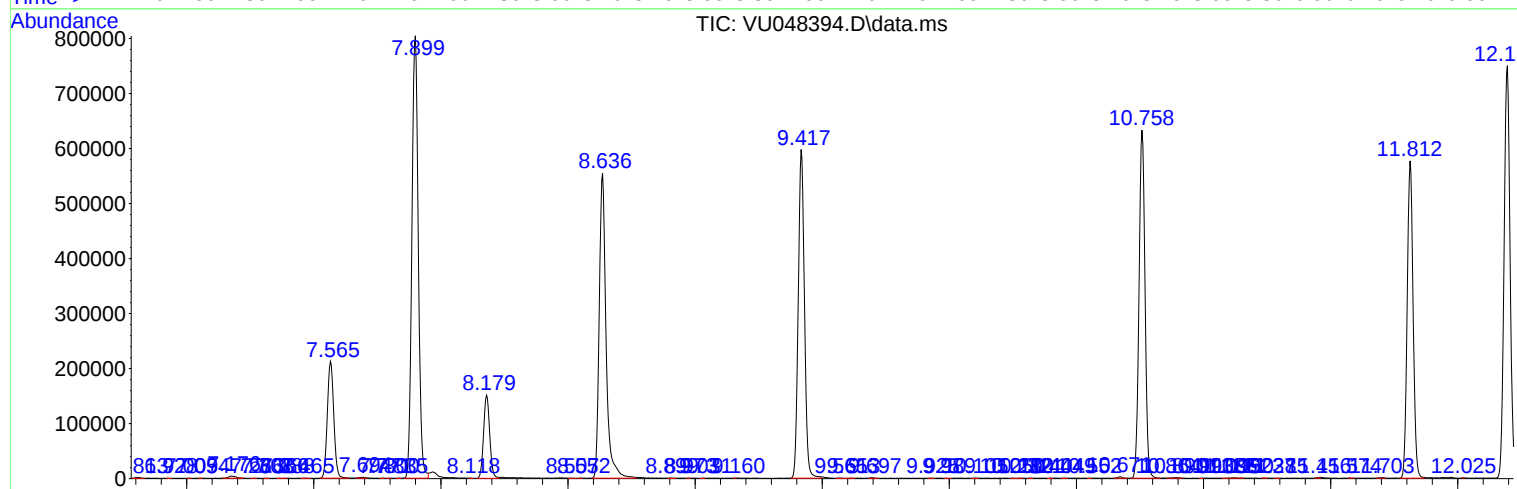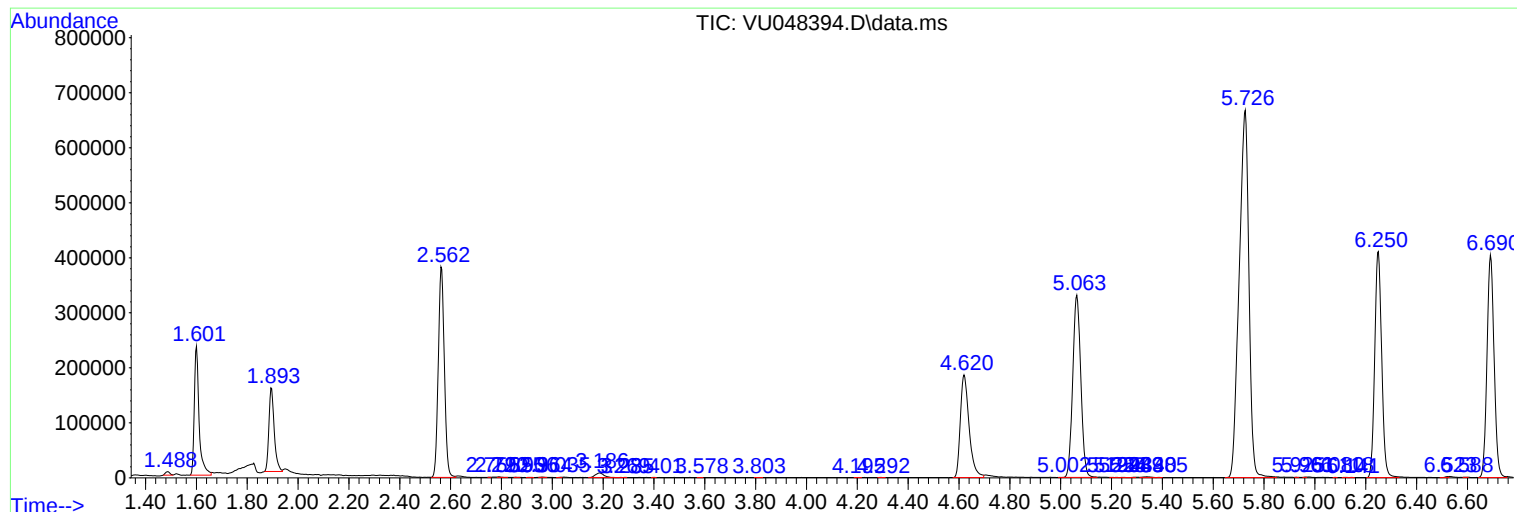

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048394.D
Acq On : 03 May 2022 16:42
Operator : SY/MD
Sample : N2668-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050322\
Data File : VU048394.D
Acq On : 03 May 2022 16:42
Operator : SY/MD
Sample : N2668-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXL79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------